


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070217\
 Data File : BF096404.D
 Acq On : 2 Jul 2017 9:31
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 01:43:12 2017

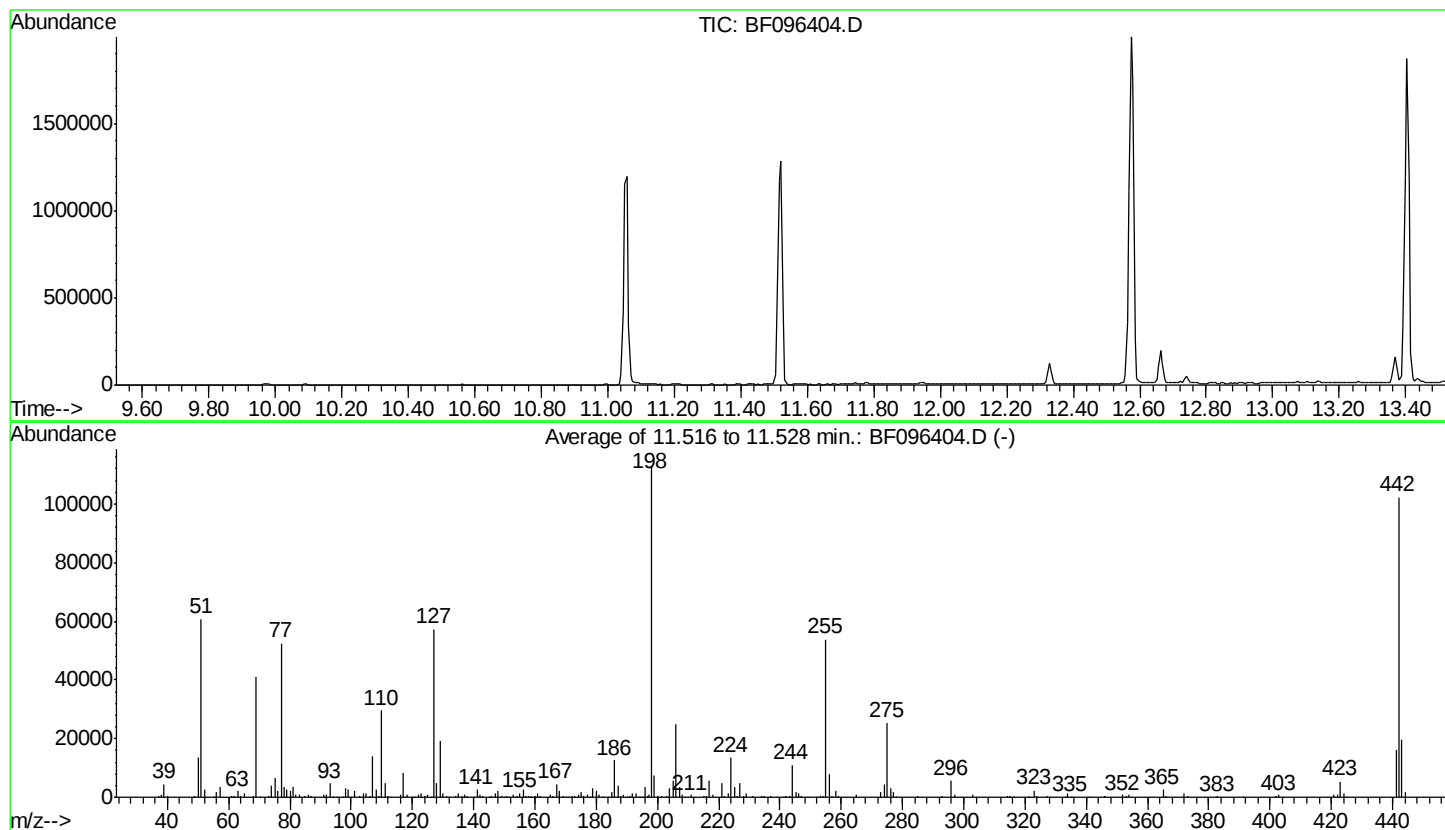

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	60854	PASS
68	69	0.00	2	1.3	523	PASS
69	198	0.00	100	36.3	41013	PASS
70	69	0.00	2	0.4	145	PASS
127	198	10	80	50.8	57386	PASS
197	198	0.00	2	0.8	894	PASS
198	198	100	100	100.0	113064	PASS
199	198	5	9	6.5	7402	PASS
275	198	10	60	22.5	25411	PASS
365	198	1	100	2.3	2598	PASS
441	442	0.01	24	16.0	16363	PASS
442	198	50	100	90.4	102160	PASS
443	442	15	24	19.2	19593	PASS