



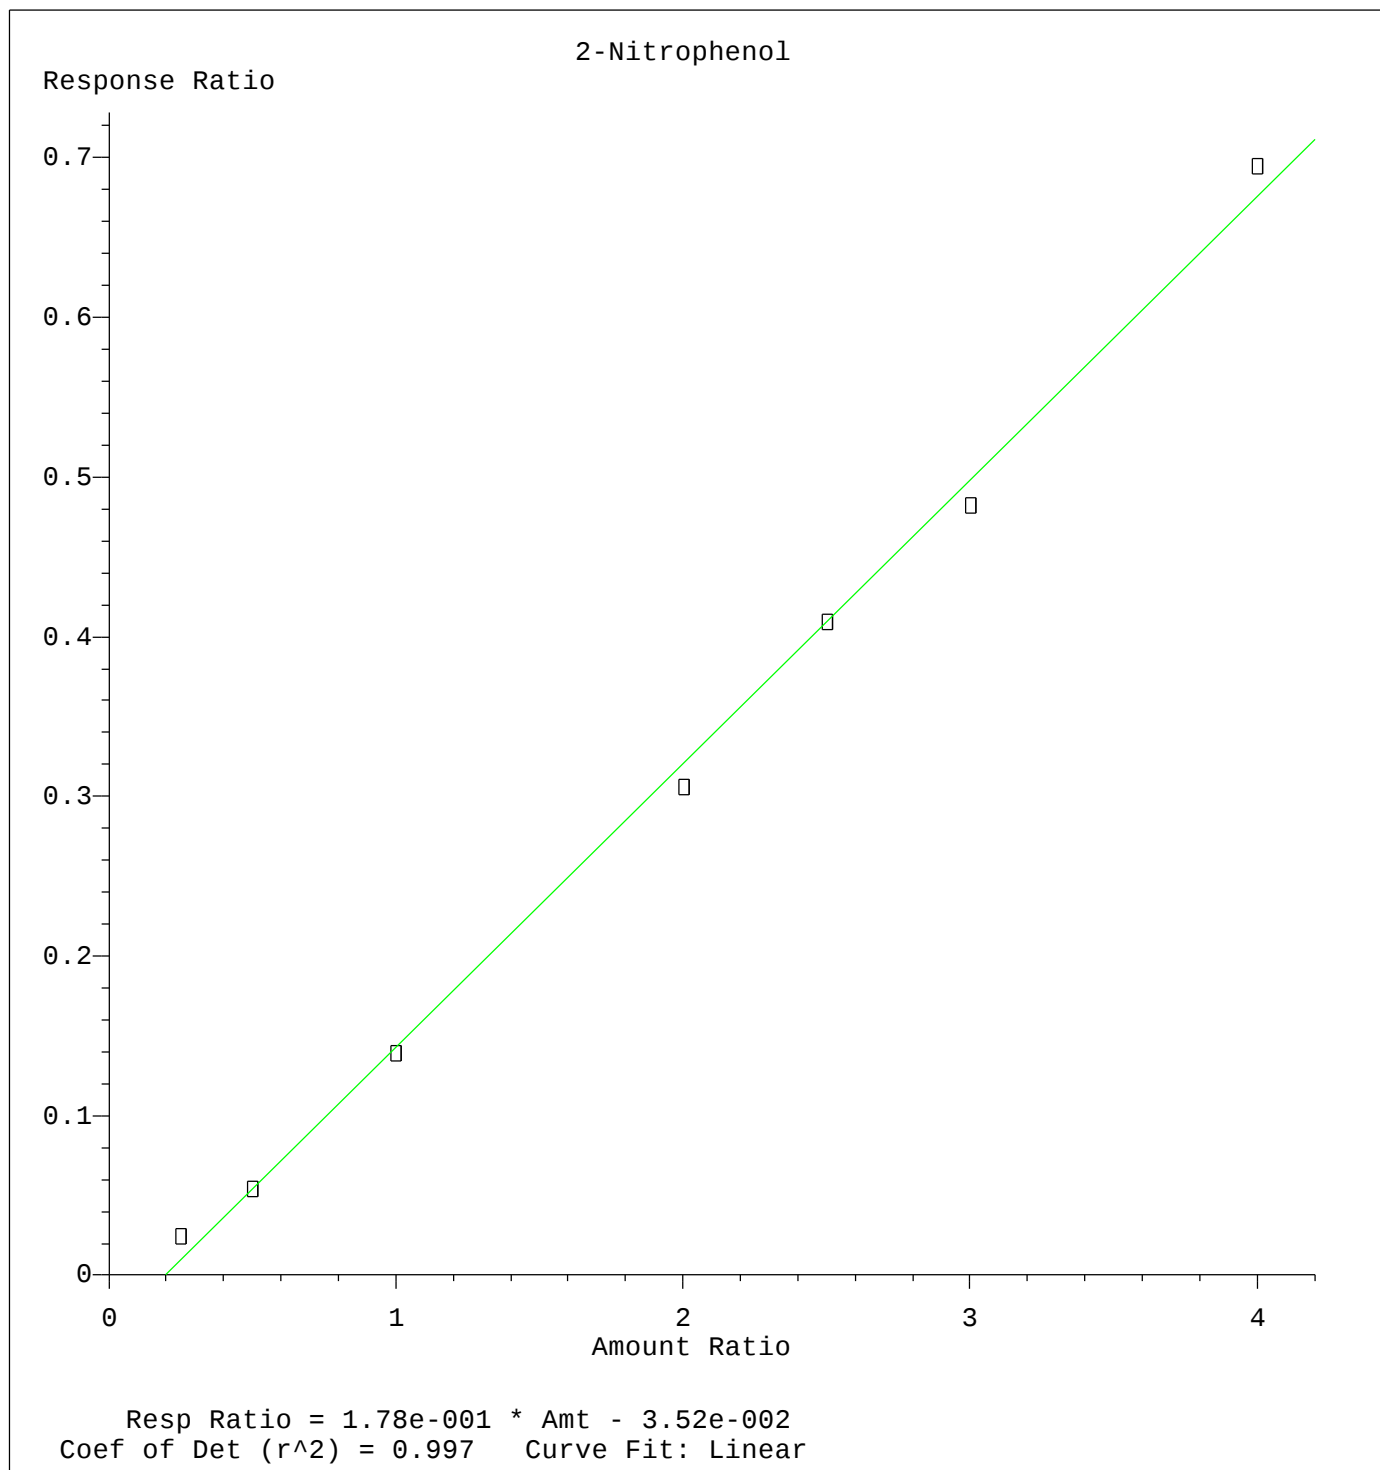


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

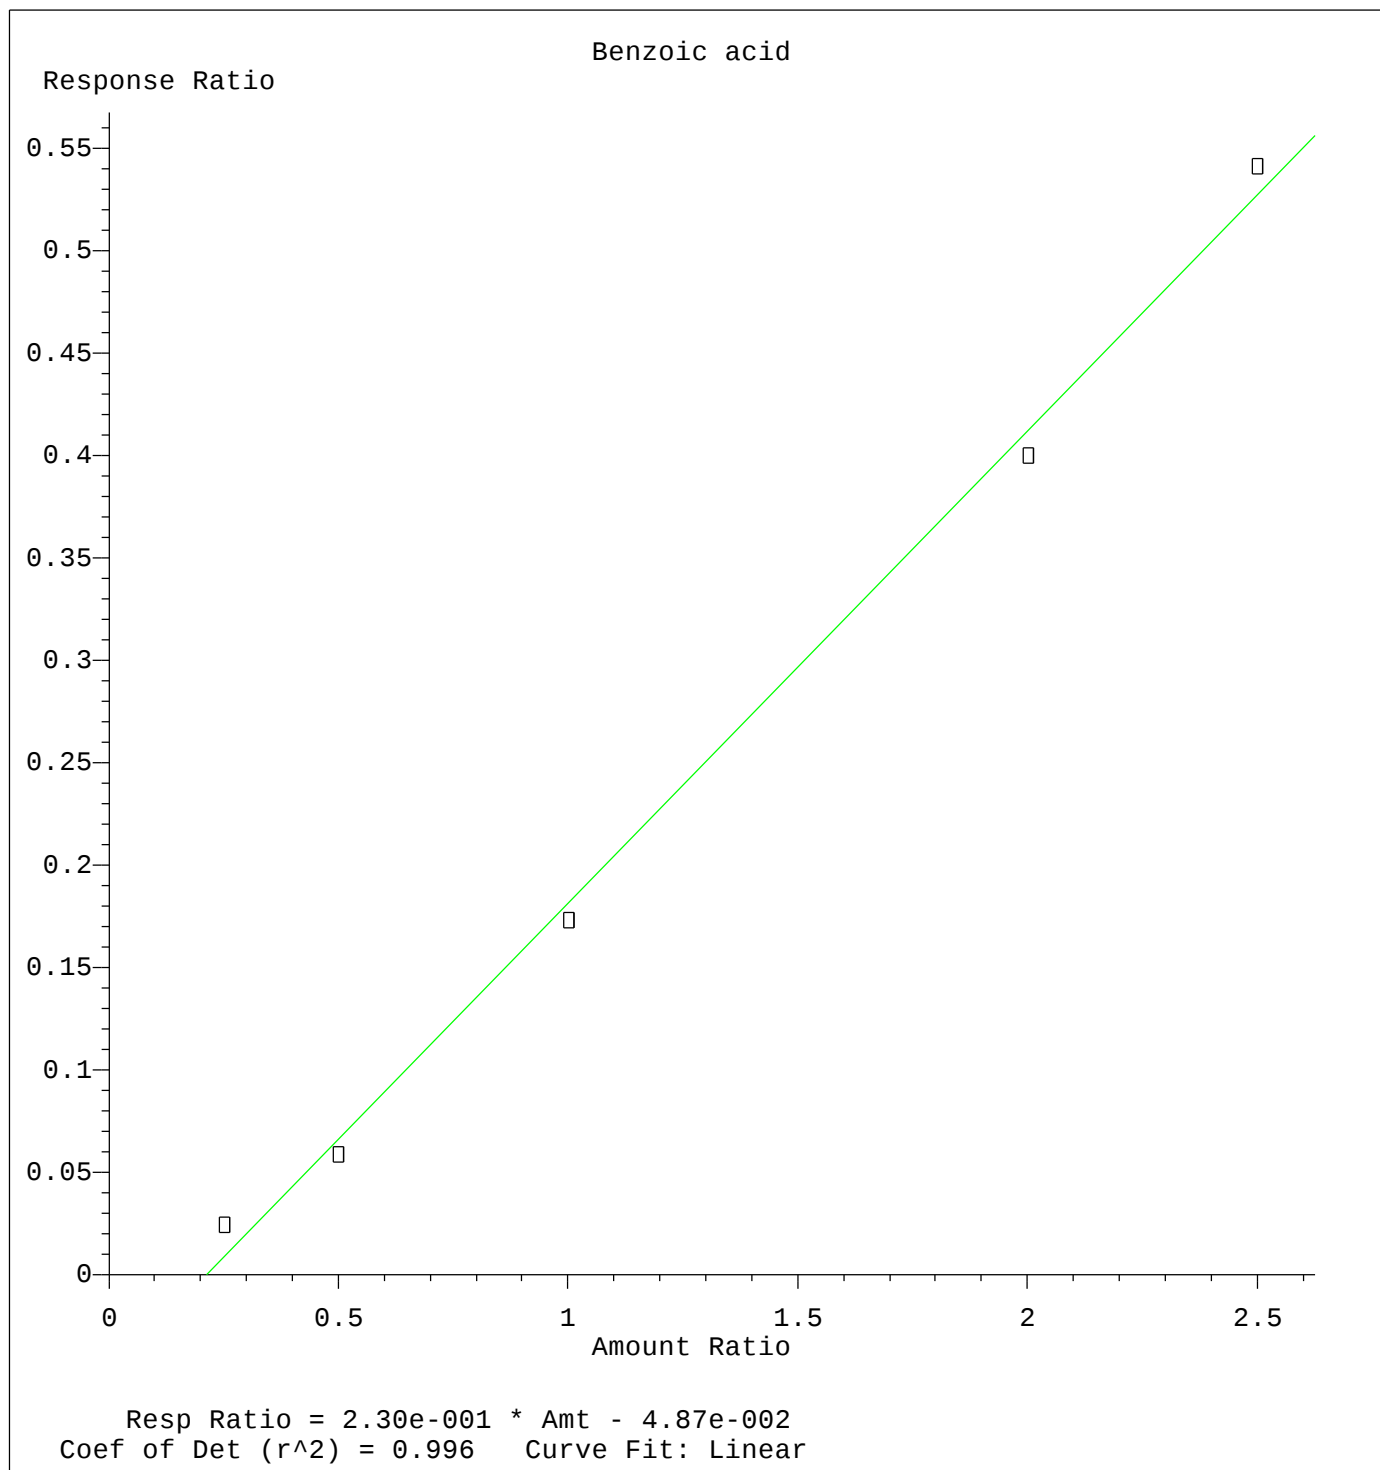

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

2-Nitroaniline

Response Ratio

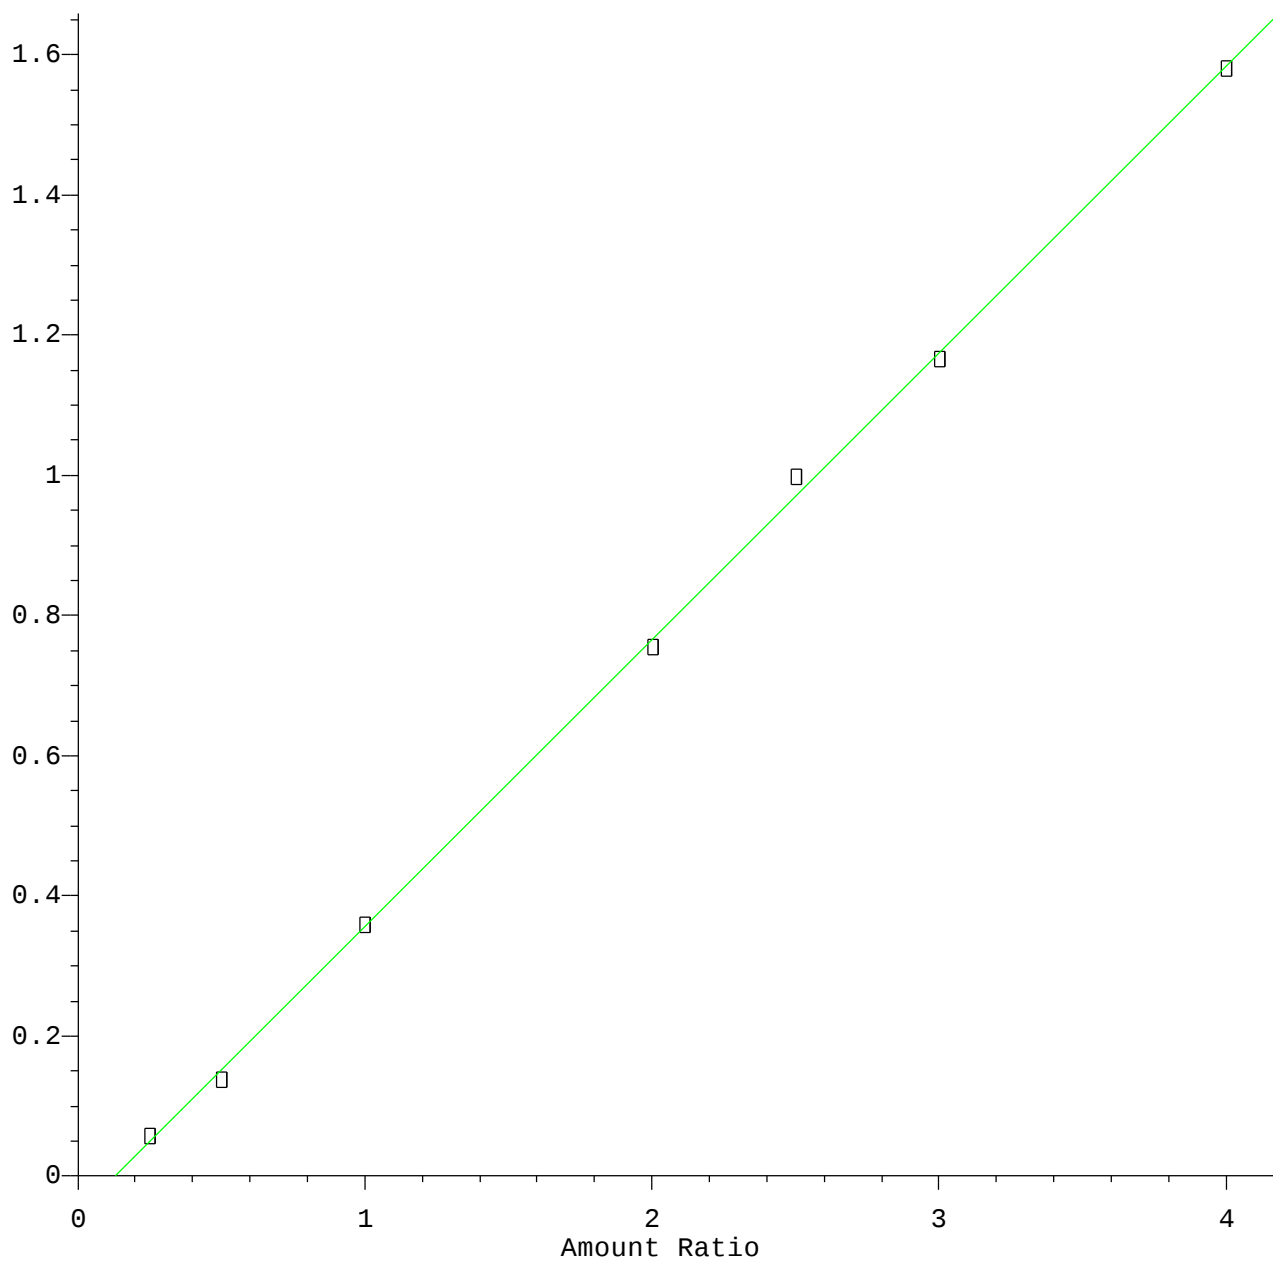


Resp Ratio = $4.09 \times 10^{-1} \times \text{Amt} - 5.36 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

2,6-Dinitrotoluene

Response Ratio

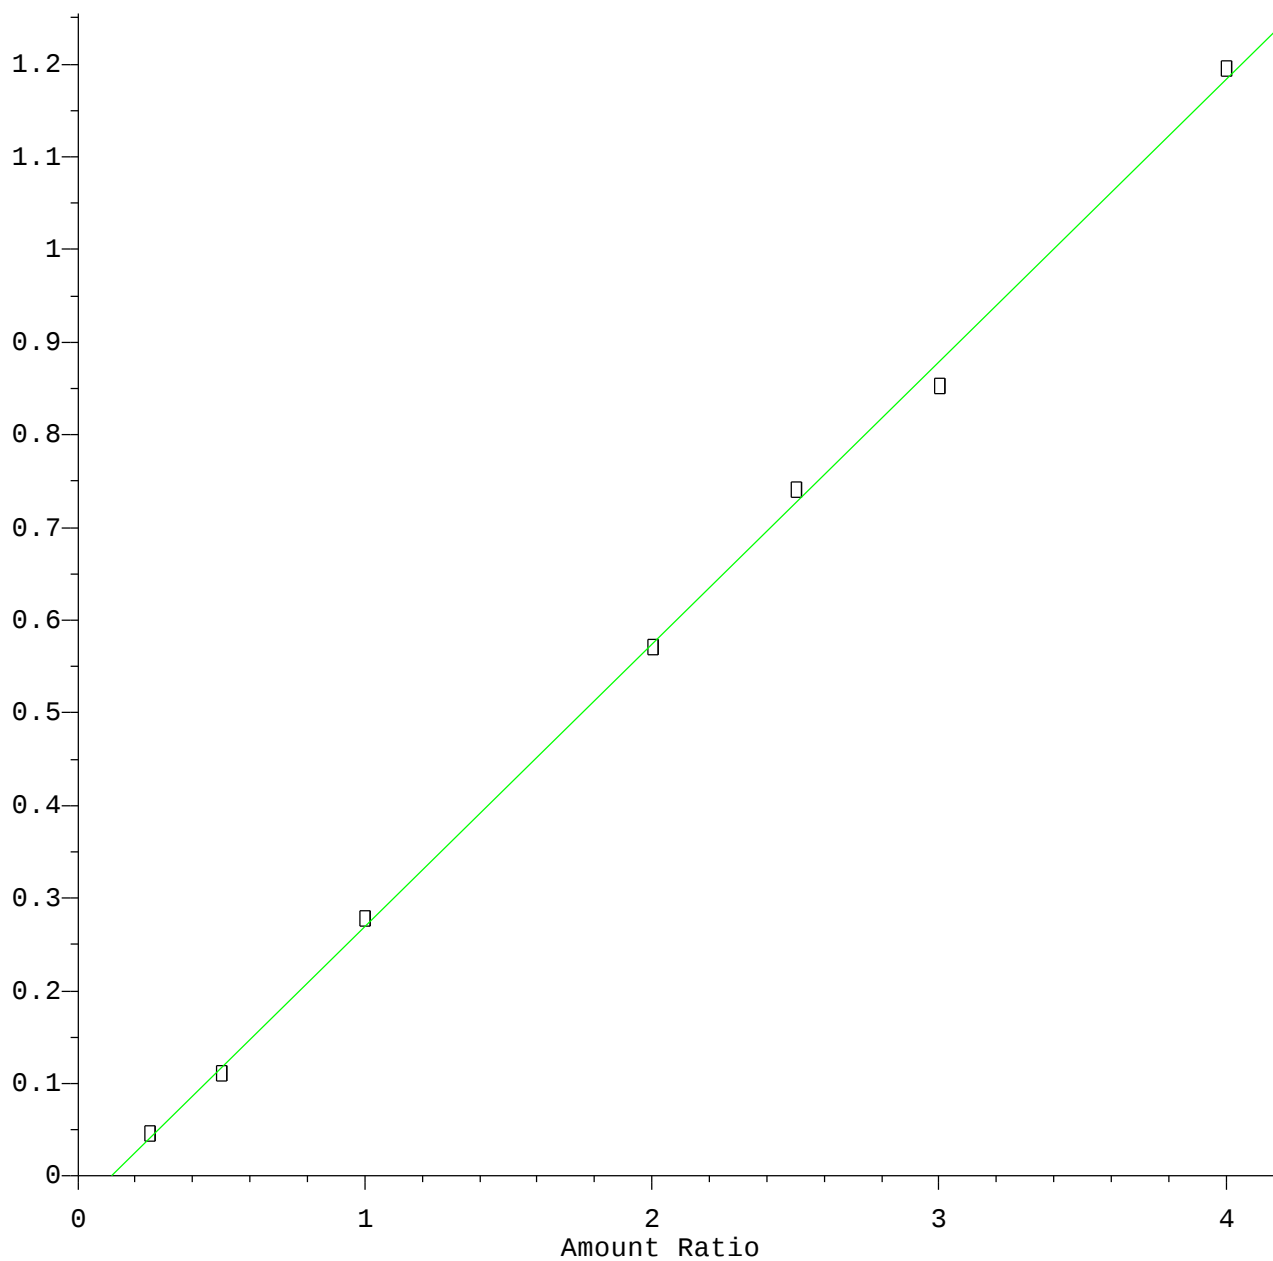


Resp Ratio = $3.04 \times 10^{-1} \times \text{Amt} - 3.47 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020


3-Nitroaniline

Response Ratio

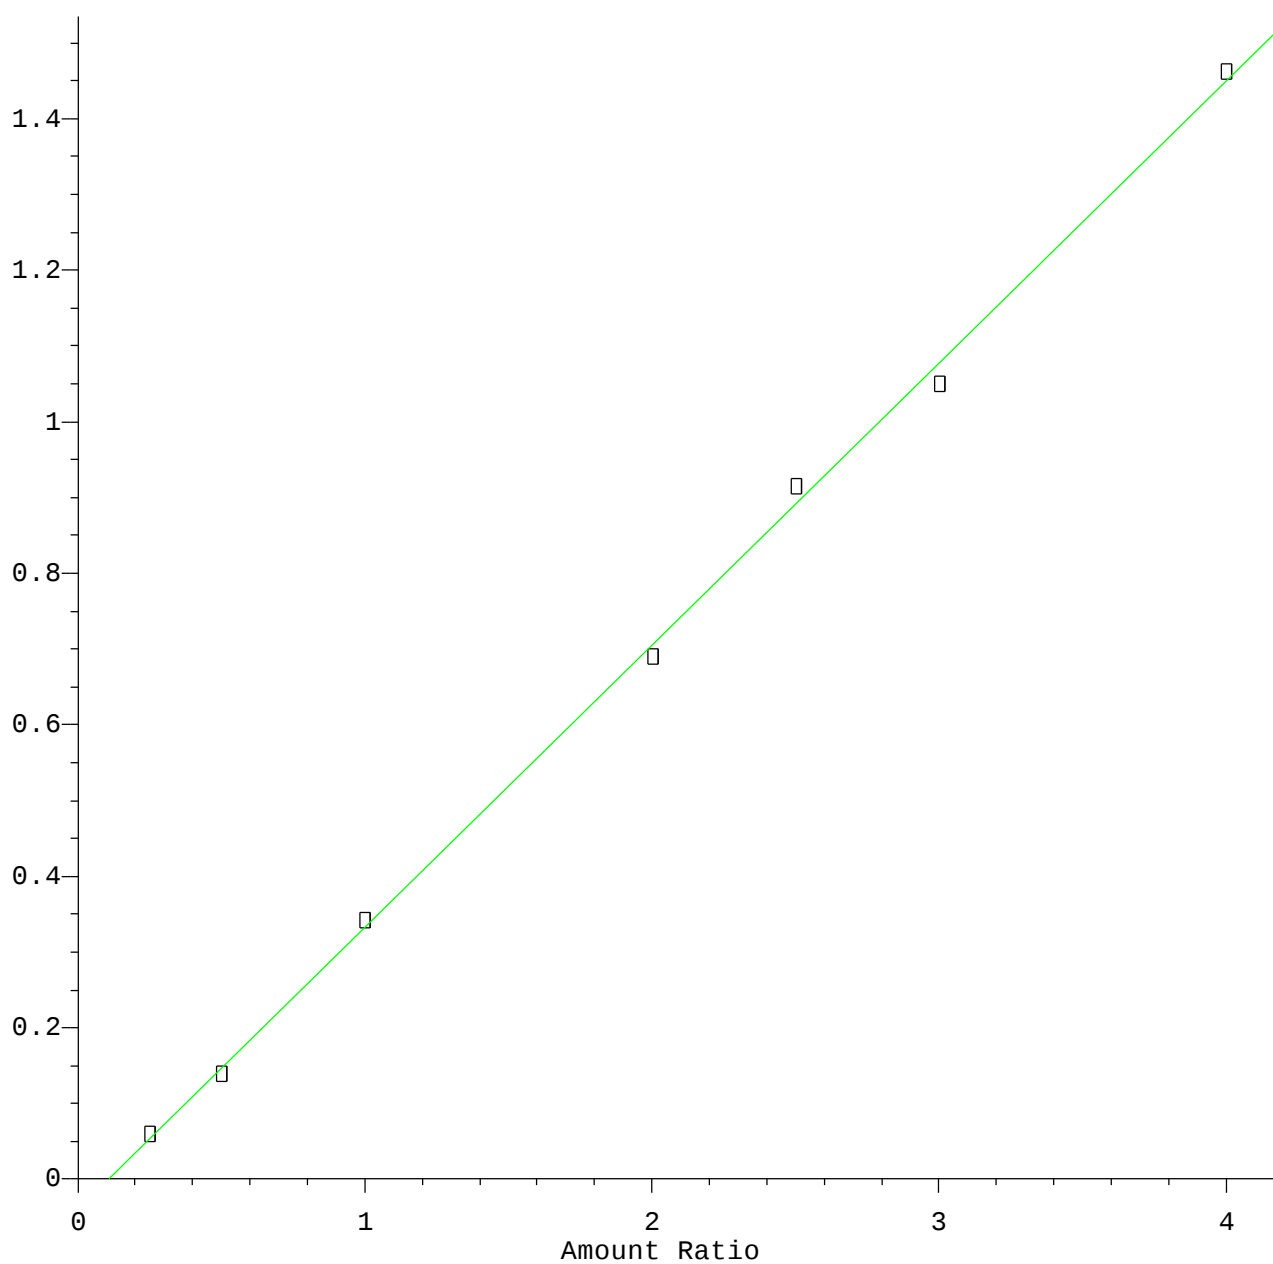


Resp Ratio = $3.72 \times 10^{-1} \times \text{Amt} - 4.03 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

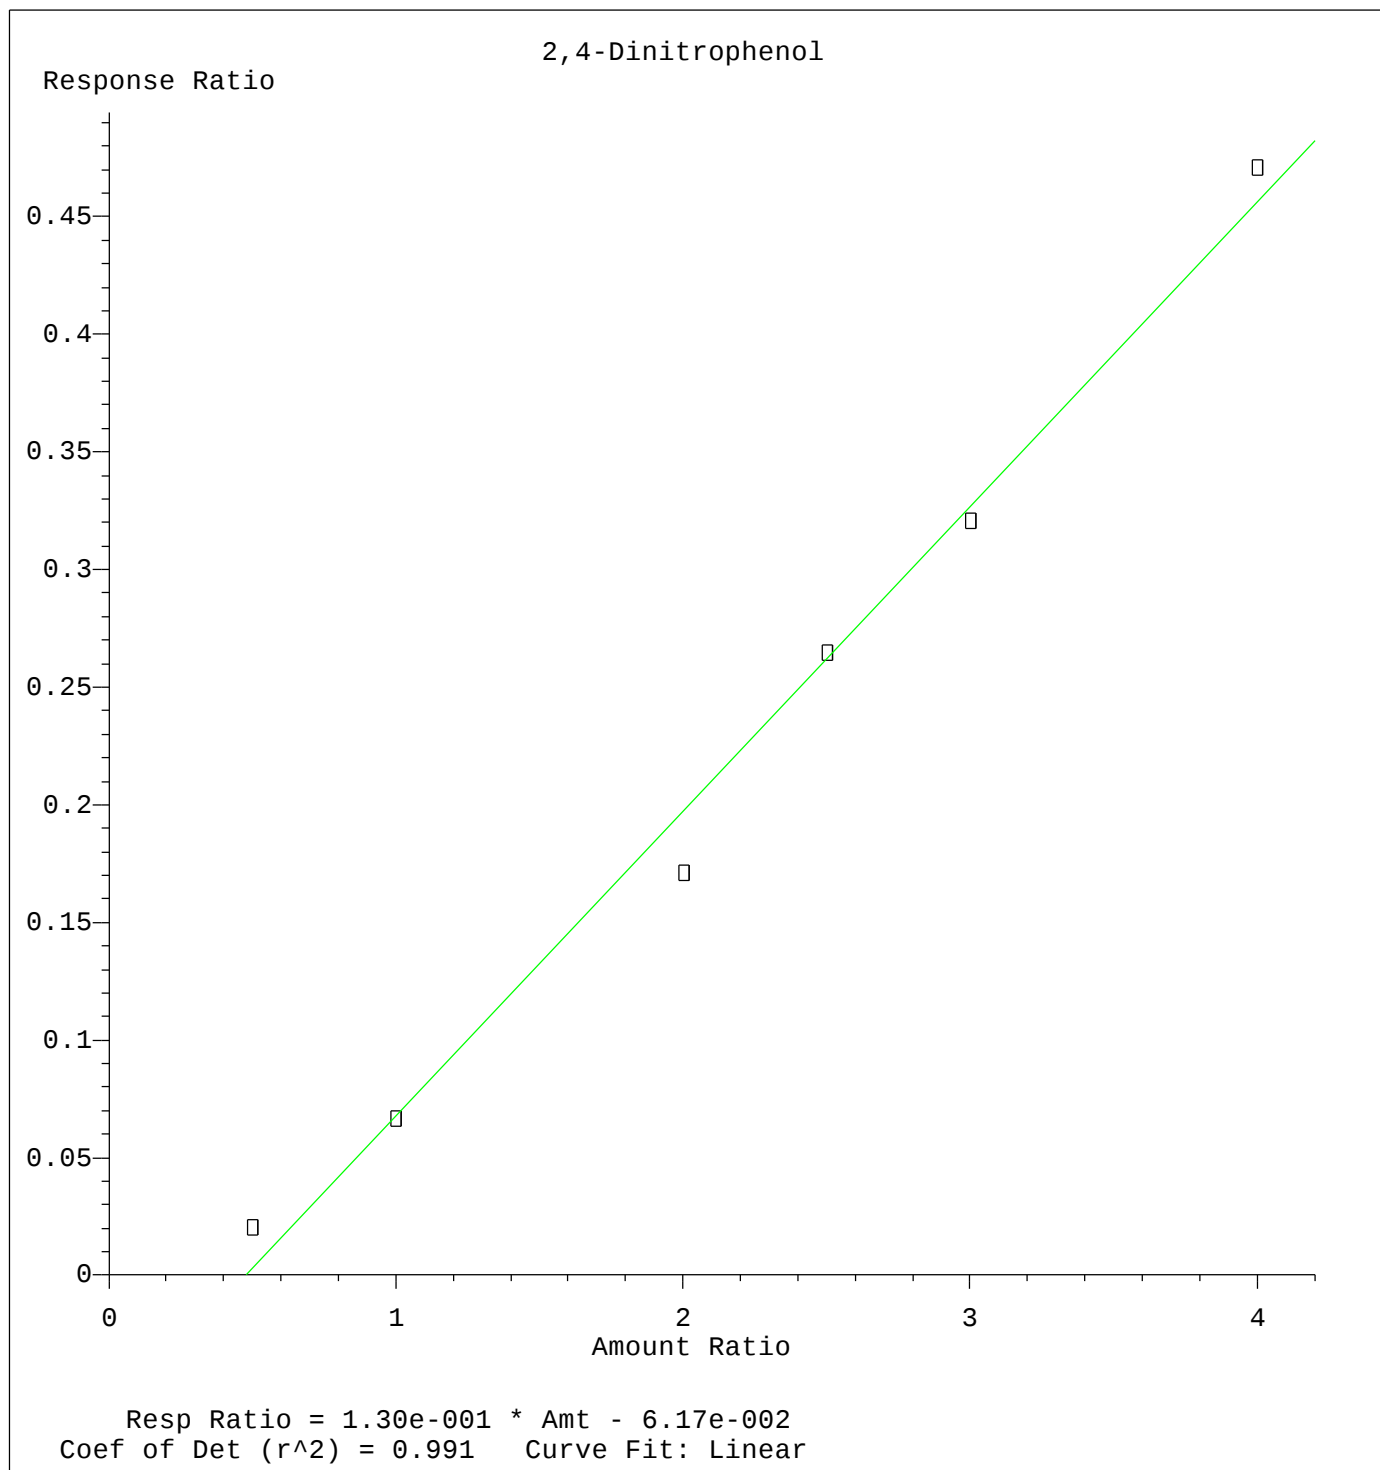


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

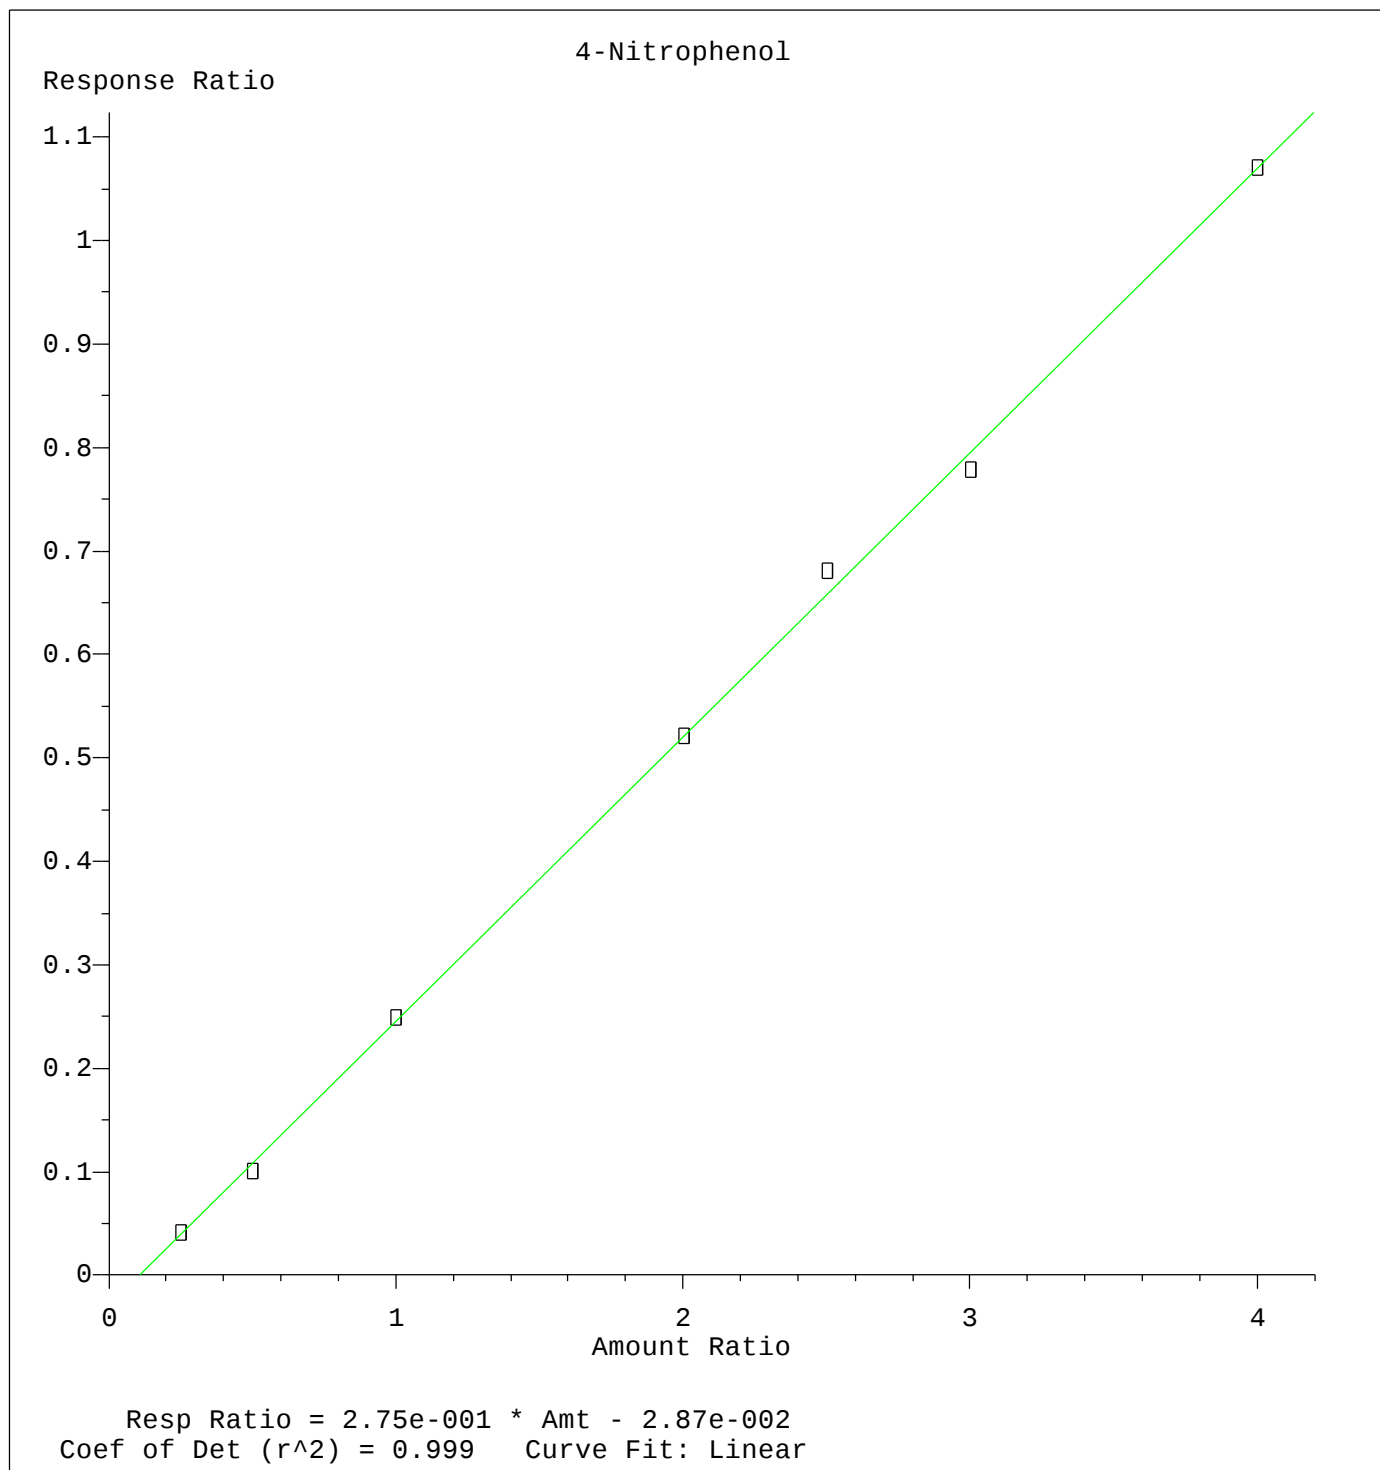

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

2,4-Dinitrotoluene


Response Ratio

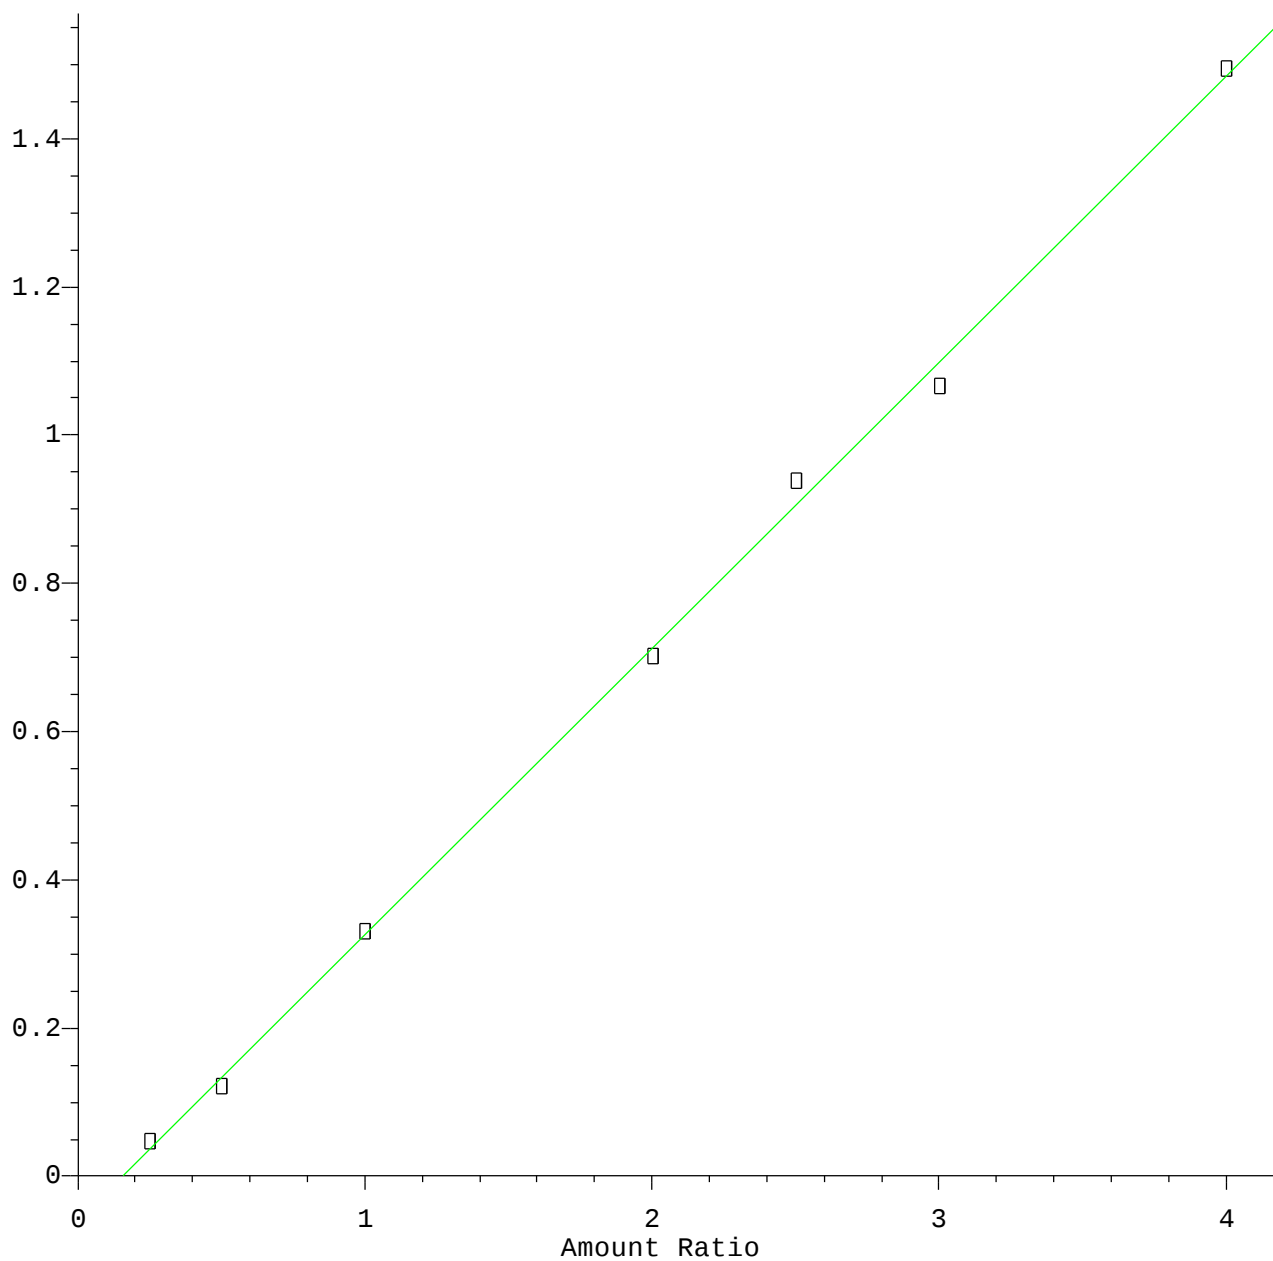

Resp Ratio = $3.86 \times 10^{-1} \times \text{Amt} - 5.93 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020

4,6-Dinitro-2-methylphenol

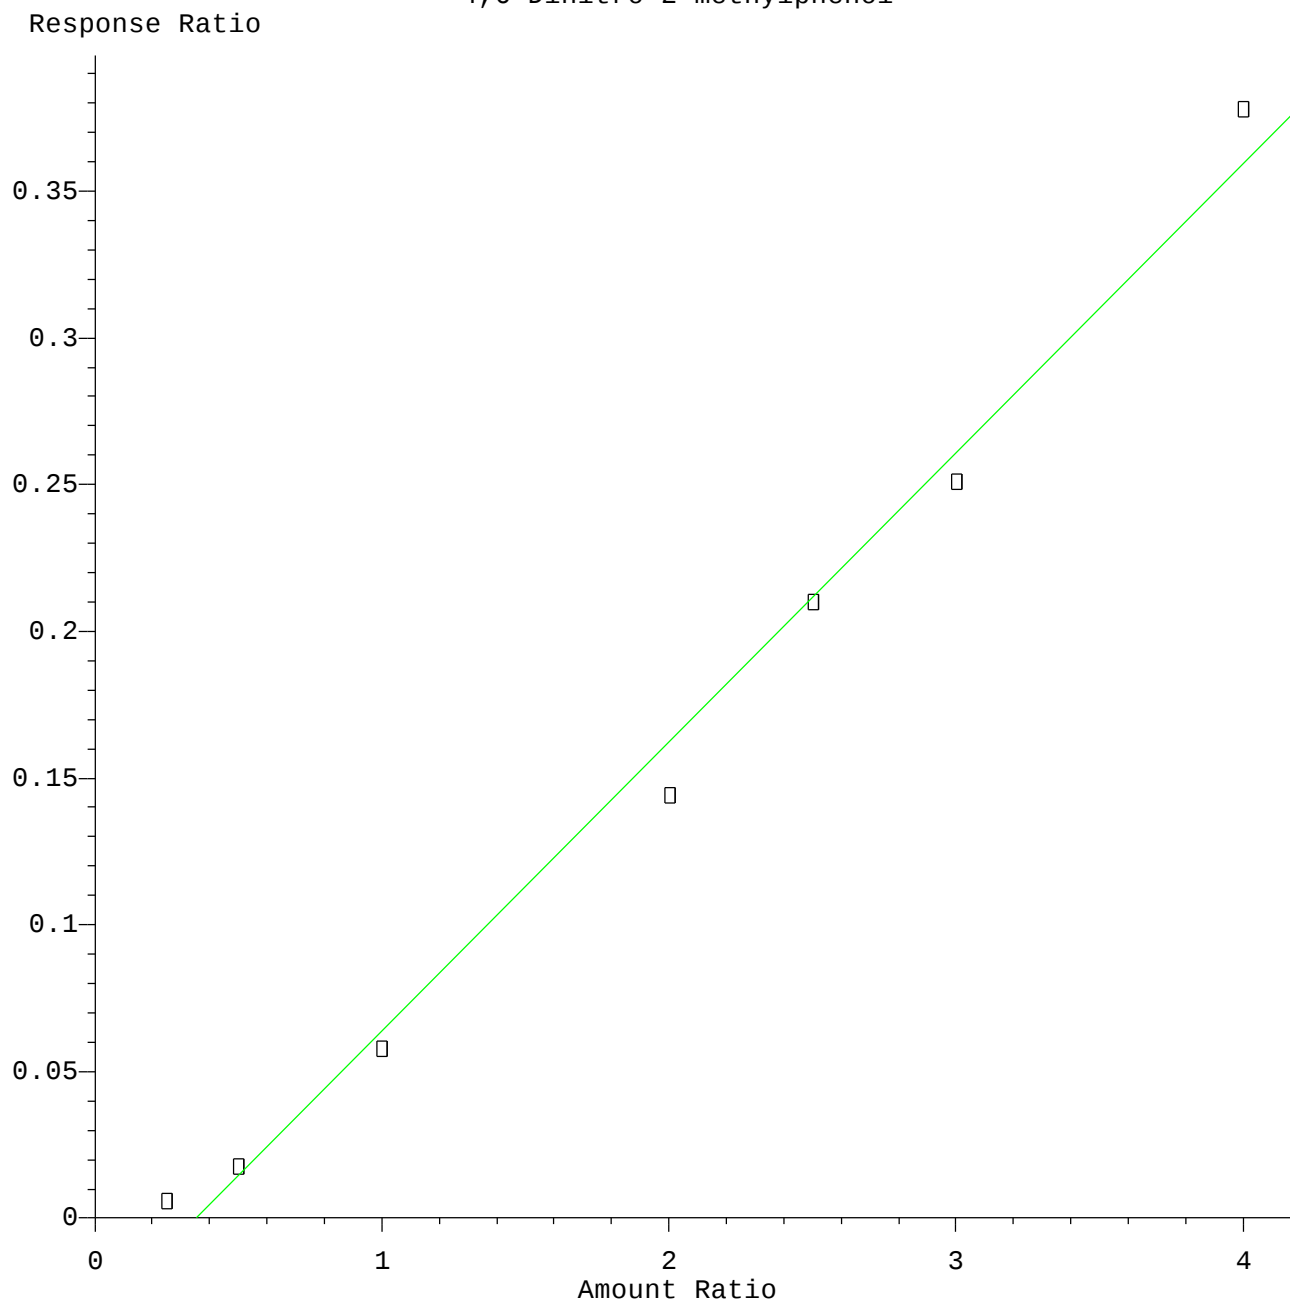

Resp Ratio = $9.85 \times 10^{-2} \times \text{Amt} - 3.45 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Calibration Table Last Updated: Thu Jul 02 18:51:52 2020