
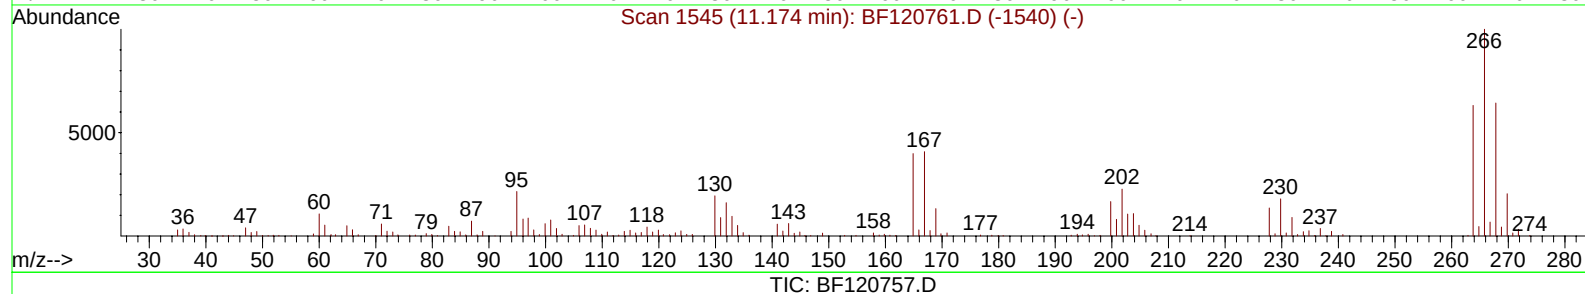
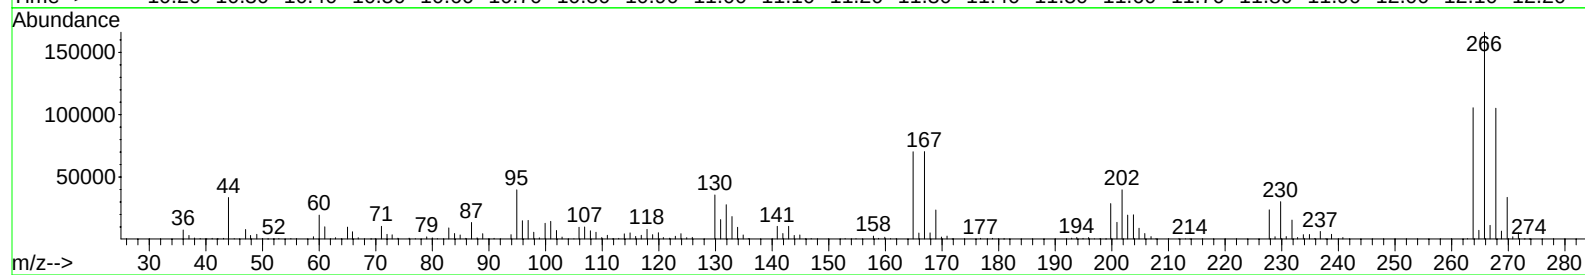


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070220\  
 Data File : BF120757.D  
 Acq On : 2 Jul 2020 14:39  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 19:12:07 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jul 02 18:51:52 2020  
 Response via : Initial Calibration

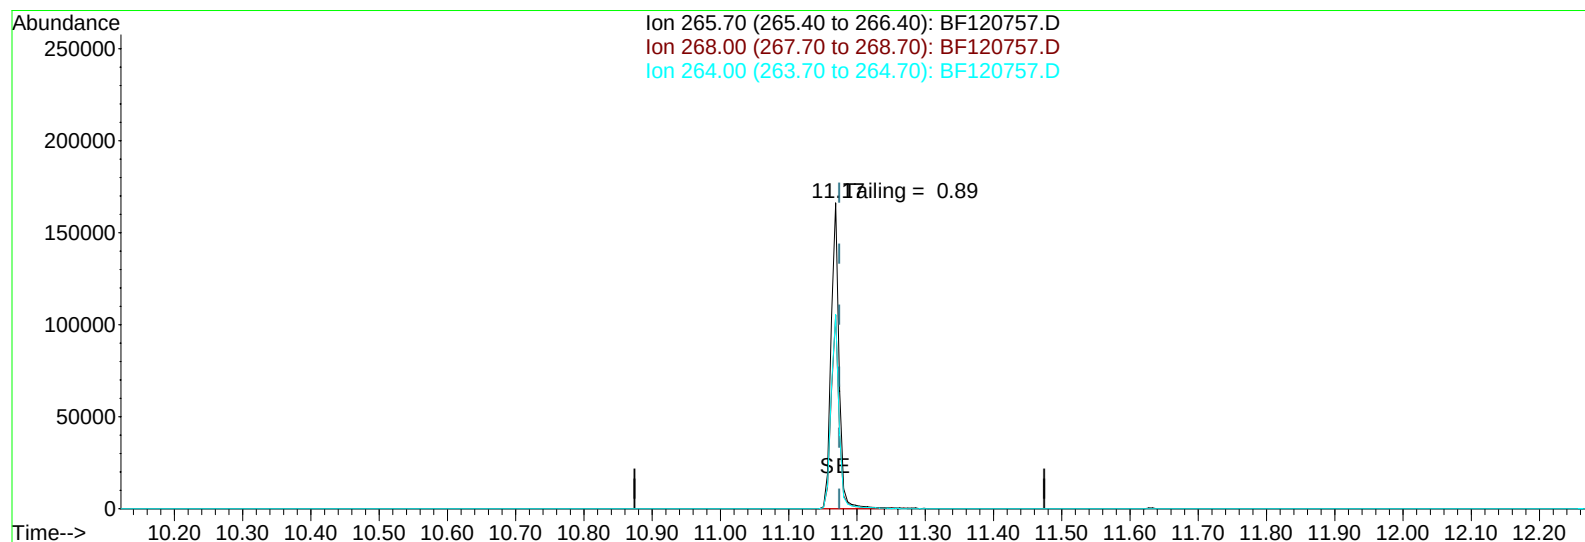

(70) Pentachlorophenol (C)




11.169min (-0.006) 37621.53ng

response 134471

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.30 | 63.30 |
| 264.00 | 63.20 | 63.52 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070220\  
 Data File : BF120757.D  
 Acq On : 2 Jul 2020 14:39  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 19:12:07 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jul 02 18:51:52 2020  
 Response via : Initial Calibration

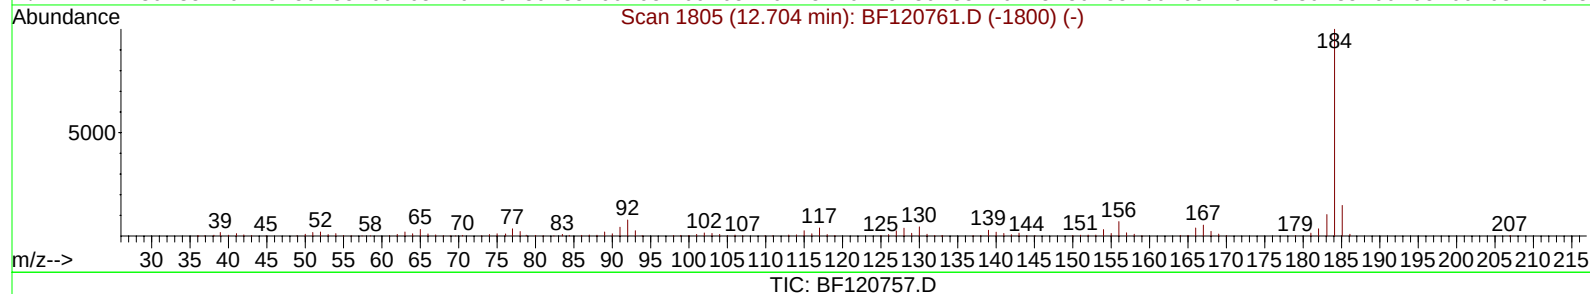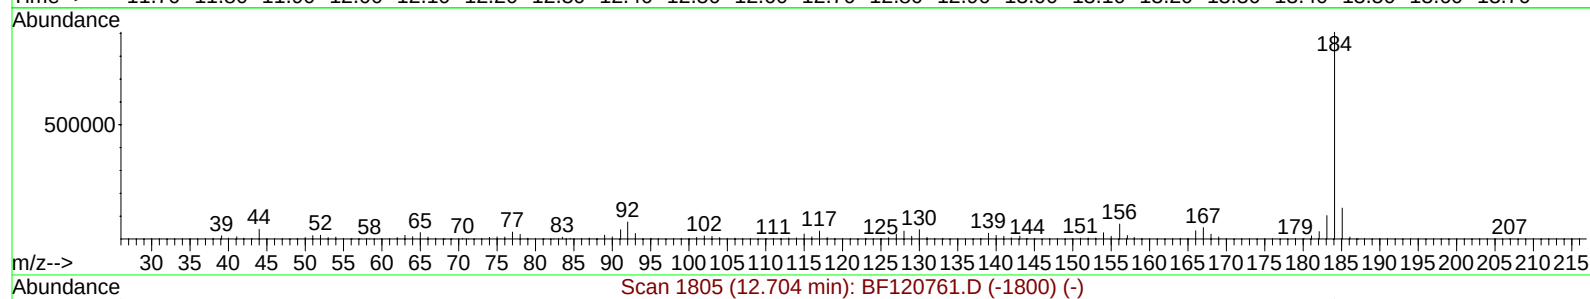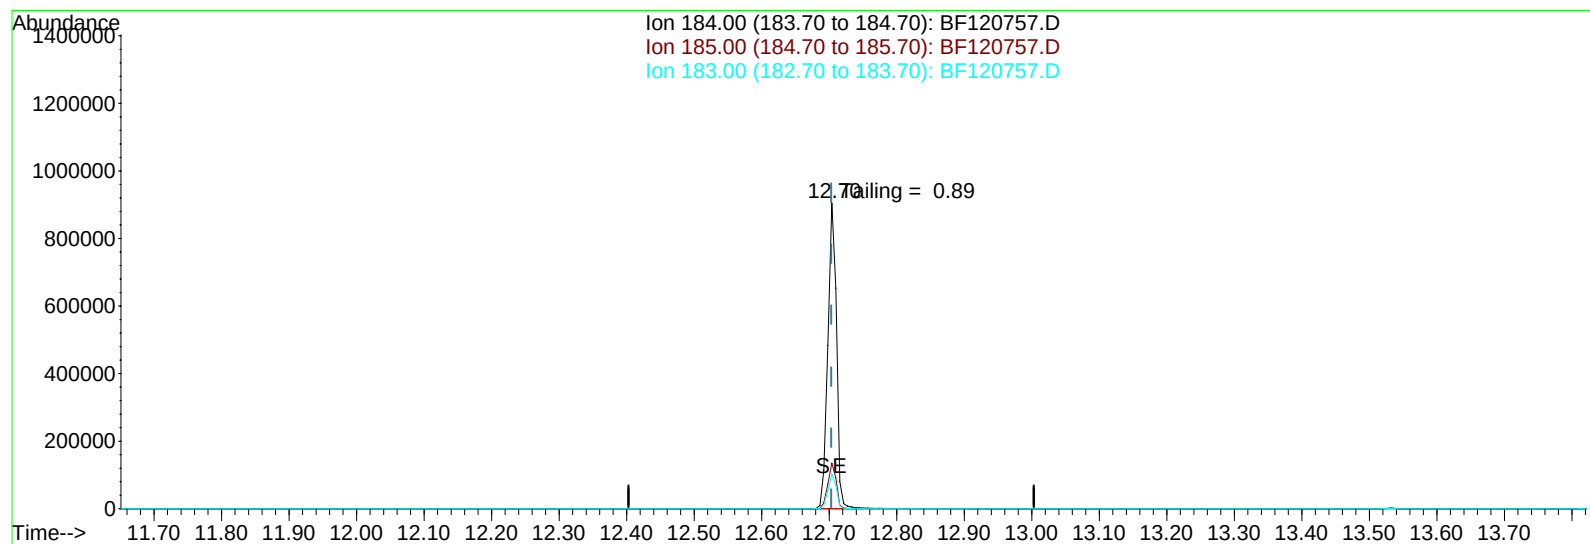

(77) Benzidine

12.704min (+0.001) 0.00ng

response 810205

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.80 | 14.97 |
| 183.00 | 10.40 | 11.37 |
| 0.00   | 0.00  | 0.00  |