


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070220\
 Data File : BF120757.D
 Acq On : 2 Jul 2020 14:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 18:51:52 2020

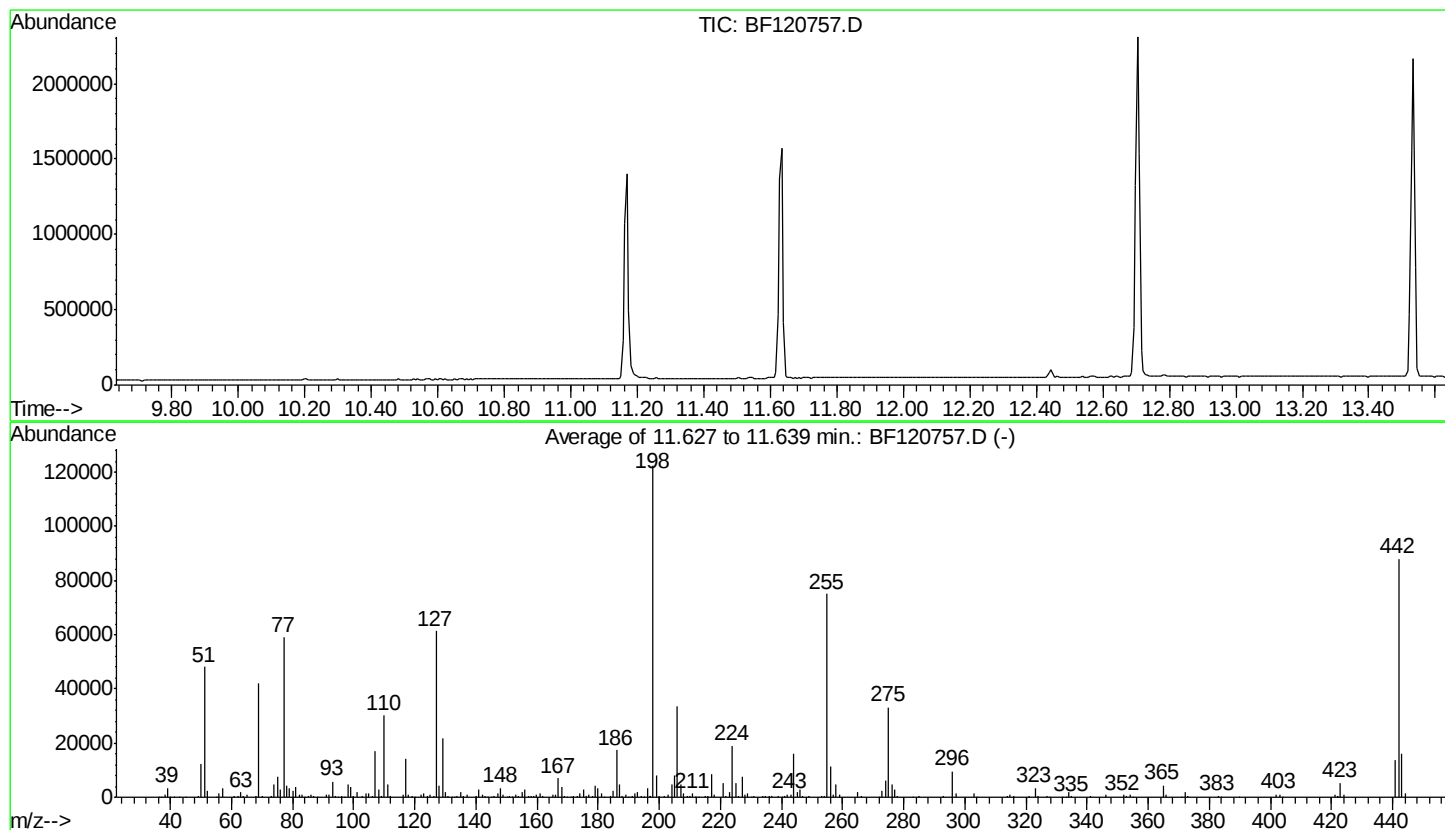

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	48155	PASS
68	69	0.00	2	1.5	647	PASS
69	198	0.00	100	34.2	41894	PASS
70	69	0.00	2	0.8	334	PASS
127	198	10	80	50.0	61281	PASS
197	198	0.00	2	0.4	546	PASS
198	198	100	100	100.0	122464	PASS
199	198	5	9	6.5	7937	PASS
275	198	10	60	27.2	33337	PASS
365	198	1	100	3.7	4494	PASS
441	198	0.01	100	11.3	13806	PASS
442	198	50	100	72.0	88176	PASS
443	442	15	24	18.1	15935	PASS