
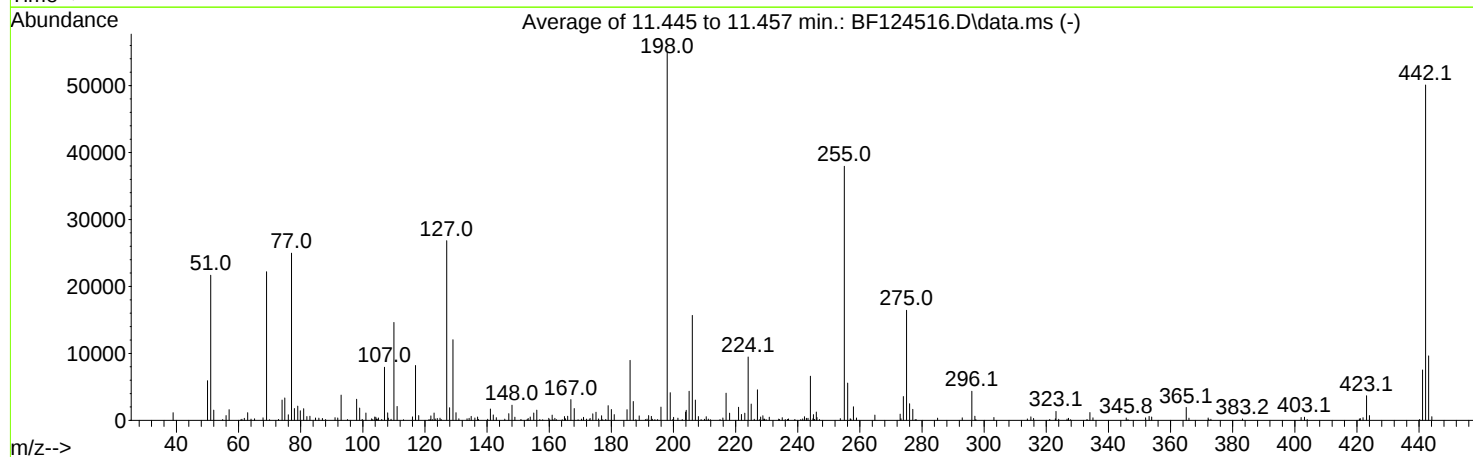


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070221\
 Data File : BF124516.D
 Acq On : 2 Jul 2021 13:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 02 14:41:35 2021

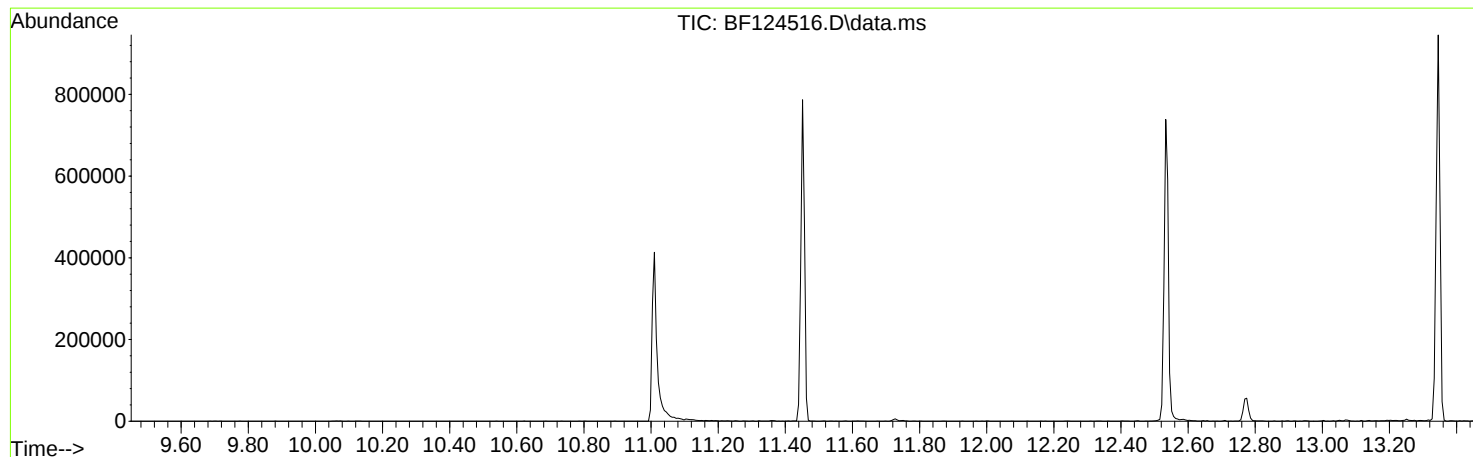

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	21670	PASS
68	69	0.00	2	1.8	393	PASS
69	198	0.00	100	40.4	22203	PASS
70	69	0.00	2	0.5	108	PASS
127	198	10	80	48.8	26832	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54941	PASS
199	198	5	9	7.5	4135	PASS
275	198	10	60	29.9	16452	PASS
365	198	1	100	3.5	1930	PASS
441	198	0.01	100	13.7	7536	PASS
442	442	50	100	100.0	50098	PASS
443	442	15	24	19.2	9640	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/2/2021	BNA_F	<u>BF124516.D</u>
Compound Name	Response	Retention Time
DDT	140924	13.34
DDD	638	13.05
DDE	143	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
781	141705	0.55

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070221\
 Data File : BF124516.D
 Acq On : 2 Jul 2021 13:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 02 14:38:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 14:15:13 2021
 Response via : Initial Calibration

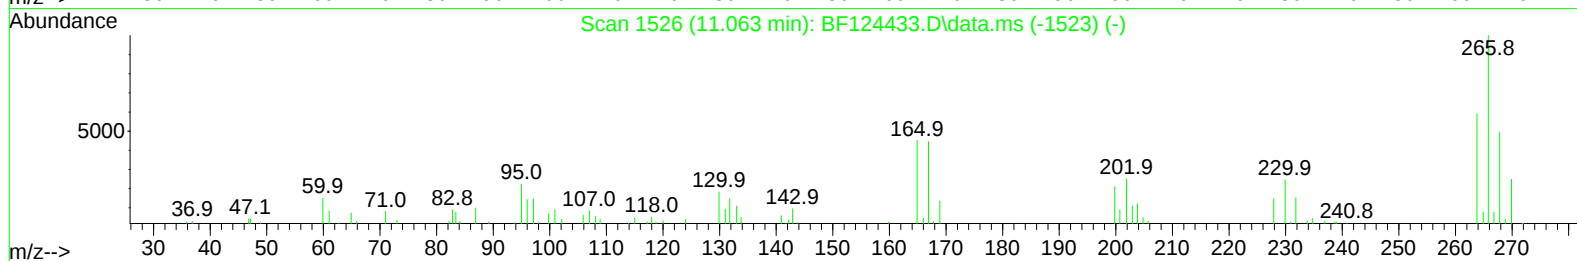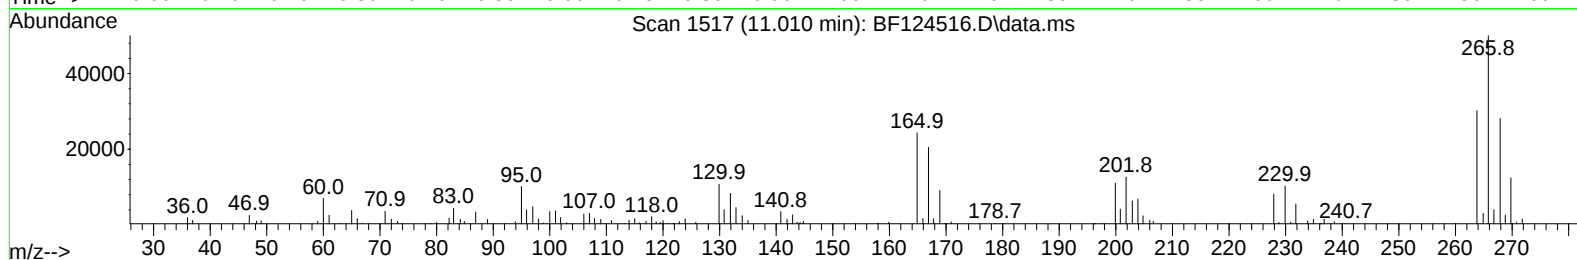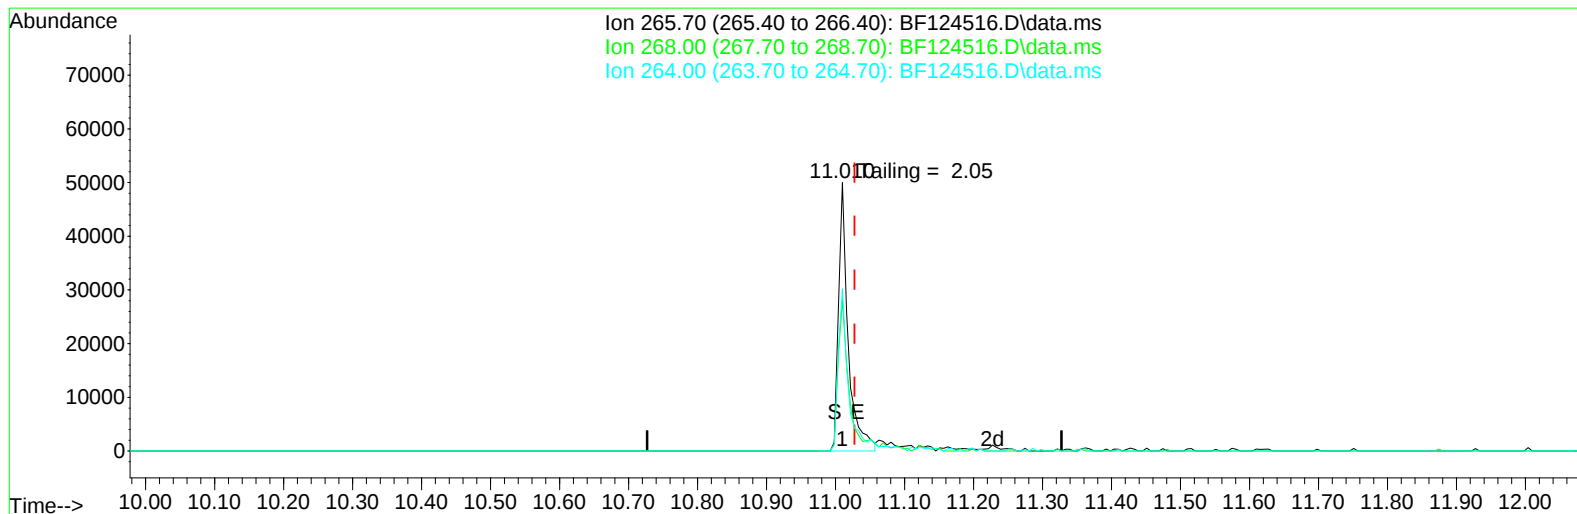

TIC: BF124516.D\data.ms

(70) Pentachlorophenol (C)

11.010min (-0.017) 109478.71 ng




response 48653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	56.31
264.00	65.70	60.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070221\
 Data File : BF124516.D
 Acq On : 2 Jul 2021 13:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 02 14:38:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 14:15:13 2021
 Response via : Initial Calibration

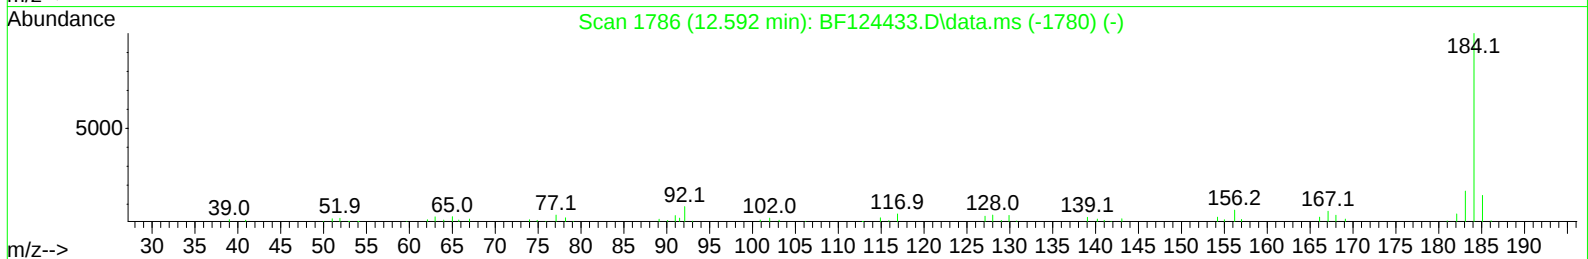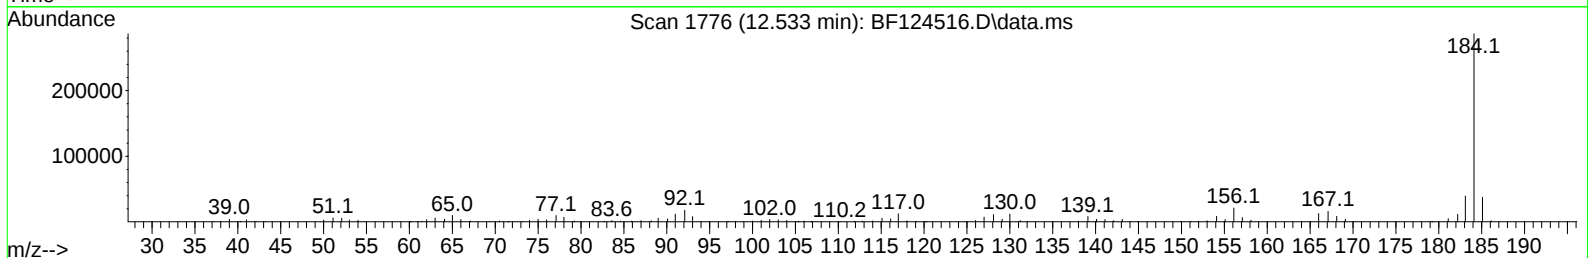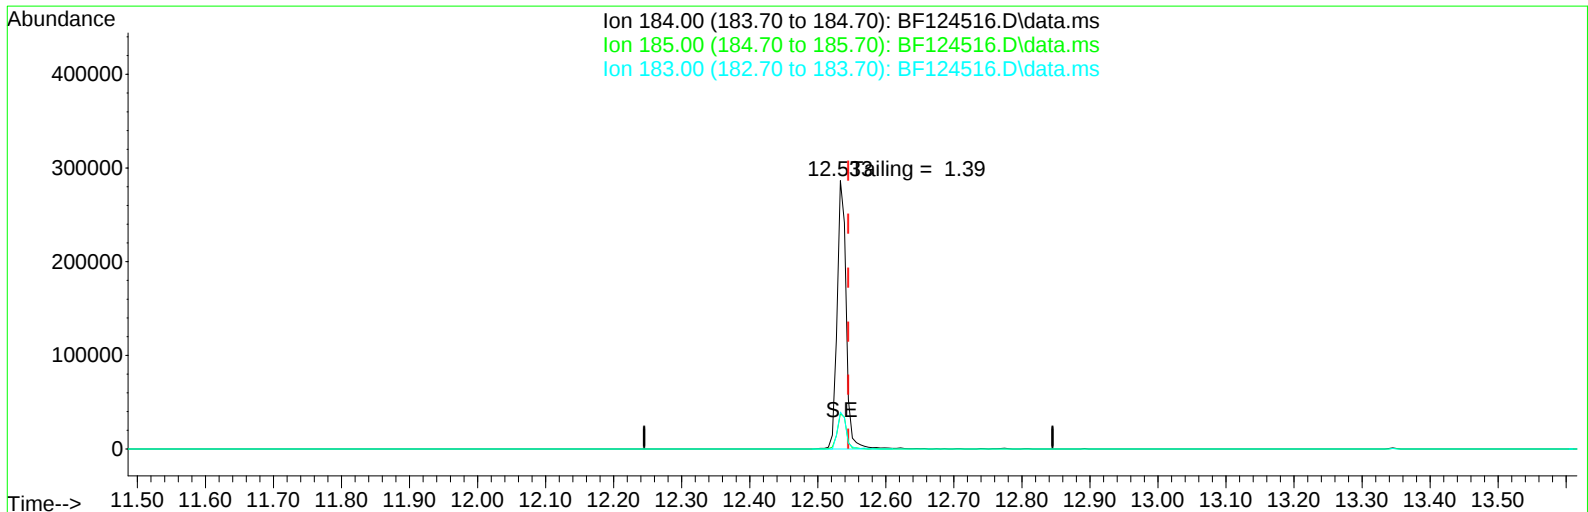

TIC: BF124516.D\data.ms

(77) Benzidine

12.533min (-0.012) 0.00 ng

response 265473

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.13
183.00	9.80	13.79#
0.00	0.00	0.00