

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070316\
 Data File : BF088658.D
 Acq On : 3 Jul 2016 20:24
 Operator : UM/SJ
 Sample : H3817-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BS-3B-10-10.5FT

Quant Time: Jul 04 06:10:35 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 30 18:01:55 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	106773	20.00	ng	-0.02
21) Naphthalene-d8	8.07	136	447682	20.00	ng	-0.03
38) Acenaphthene-d10	9.82	164	214982	20.00	ng	-0.03
63) Phenanthrene-d10	11.29	188	389800	20.00	ng	-0.03
75) Chrysene-d12	13.92	240	344918	20.00	ng	-0.03
86) Perylene-d12	15.31	264	267395	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	691788	97.10	ng	-0.02
7) Phenol-d6	6.42	99	1001706	108.82	ng	-0.02
23) Nitrobenzene-d5	7.35	82	624368	73.09	ng	-0.03
41) 2,4,6-Tribromophenol	10.60	330	219554	109.98	ng	-0.03
44) 2-Fluorobiphenyl	9.14	172	853299	62.70	ng	-0.03
78) Terphenyl-d14	12.88	244	763408	49.30	ng	-0.03
Target Compounds						
49) Dimethylphthalate	9.54	163	250707	16.37	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070316\
Data File : BF088658.D
Acq On : 3 Jul 2016 20:24
Operator : UM/SJ
Sample : H3817-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BS-3B-10-10.5FT

Quant Time: Jul 04 06:10:35 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 30 18:01:55 2016
Response via : Initial Calibration

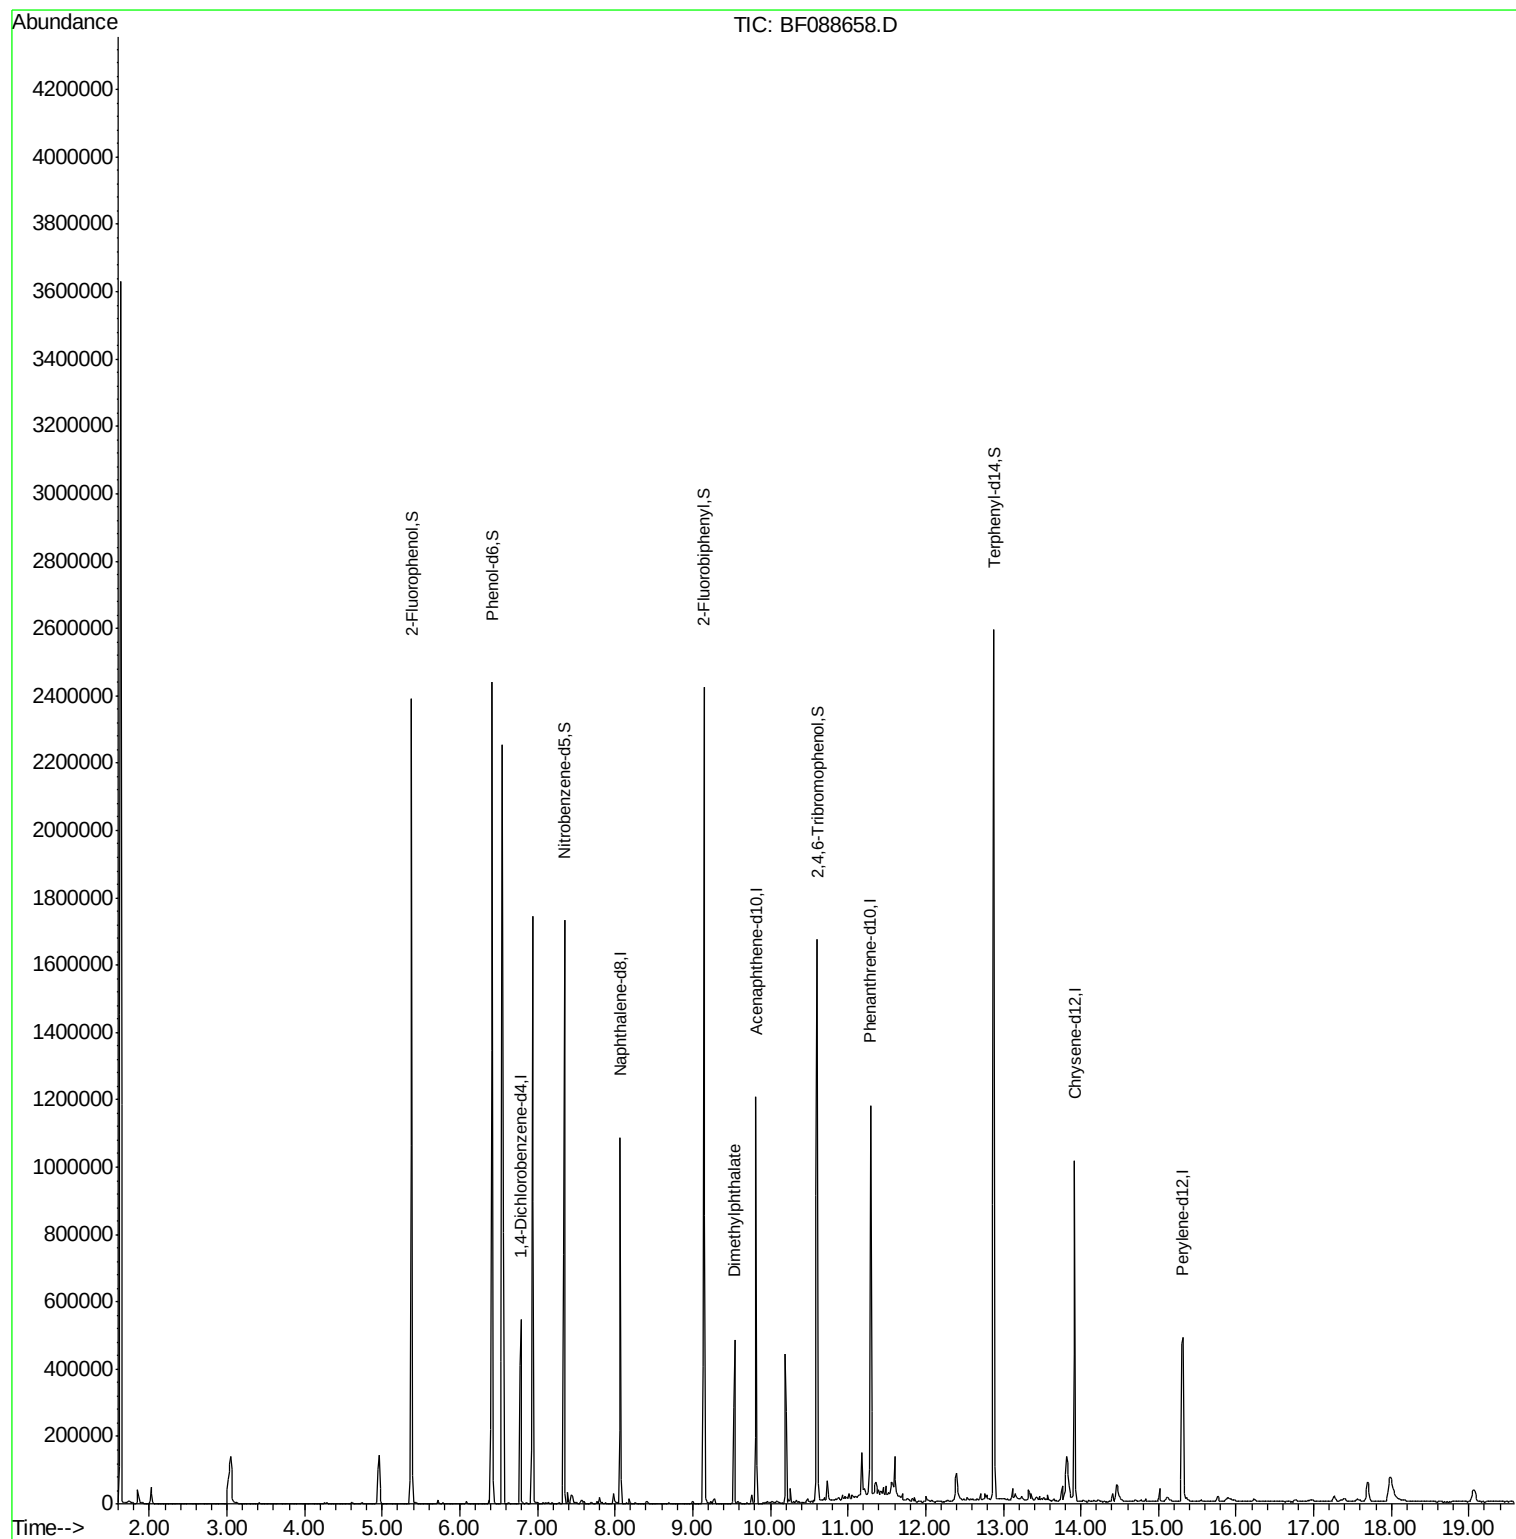

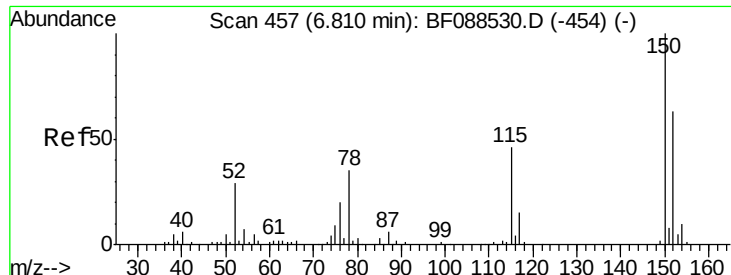

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.79 min Scan# 455

Delta R.T. -0.02 min

Lab File: BF088658.D

Acq: 3 Jul 2016 20:24

Instrument :

BNA_F

ClientSampleId :

BS-3B-10-10.5FT


Tot Ion:152 Resp: 106773

Ion Ratio Lower Upper

152 100

150 154.0 123.8 185.6




115 56.5 39.6 59.4

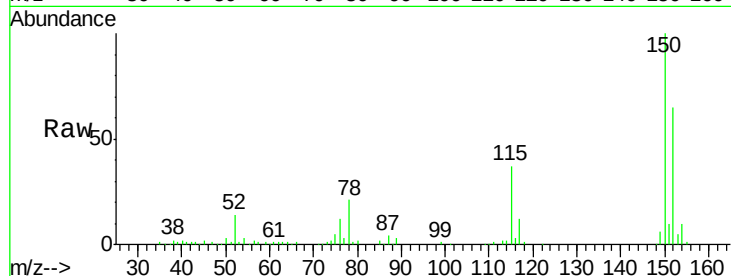

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

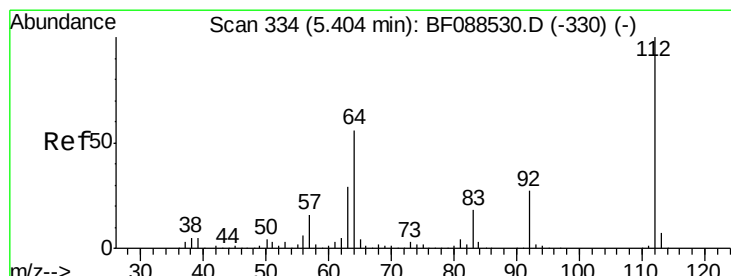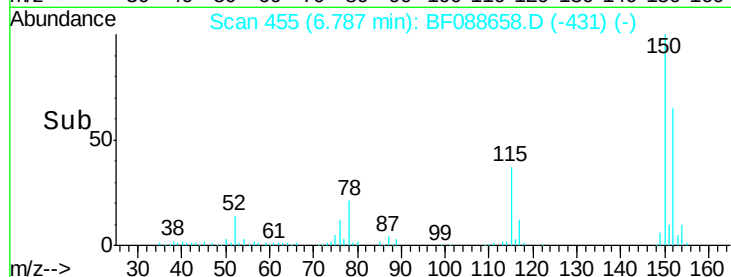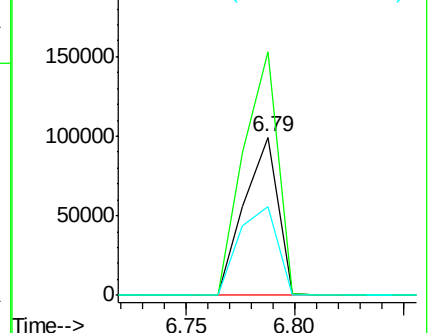

#5

2-Fluorophenol

Concen: 97.10 ng

RT: 5.38 min Scan# 332

Delta R.T. -0.02 min

Lab File: BF088658.D

Acq: 3 Jul 2016 20:24


Tgt Ion:112 Resp: 691788

Ion Ratio Lower Upper

112 100

64 60.6 42.2 63.2



63 32.0 21.8 32.8

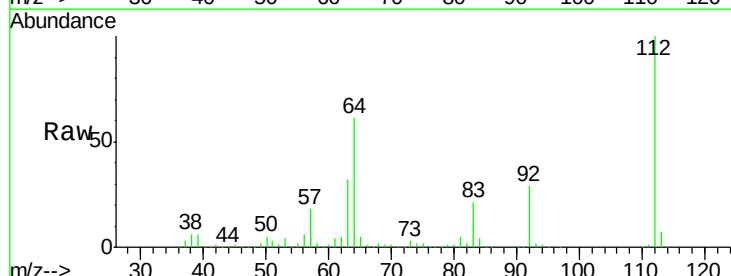


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

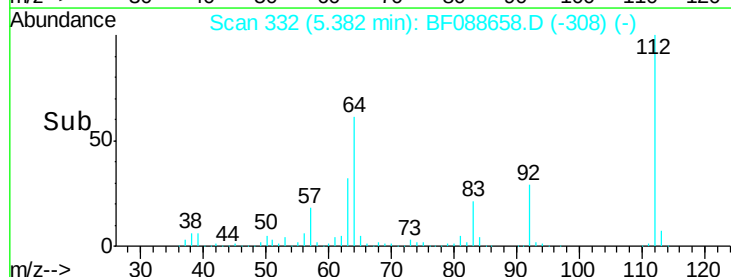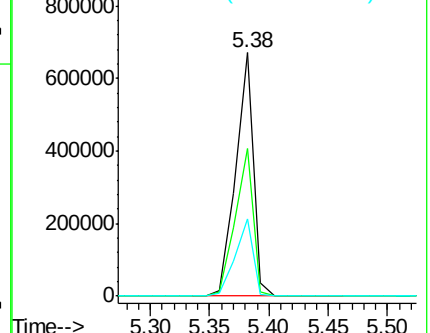

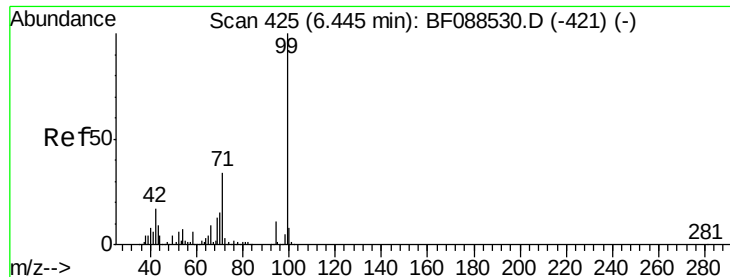

#7

Phenol-d6

Concen: 108.82 ng

RT: 6.42 min Scan# 423

Delta R.T. -0.02 min

Lab File: BF088658.D

Acq: 3 Jul 2016 20:24

Instrument :

BNA_F

ClientSampleId :

BS-3B-10-10.5FT


Tot Ion: 99 Resp: 1001706

Ion Ratio Lower Upper




99 100

42 16.7 12.2 18.2

71 36.0 23.4 35.0#

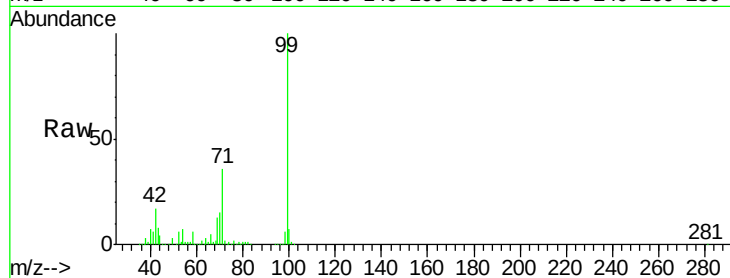

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

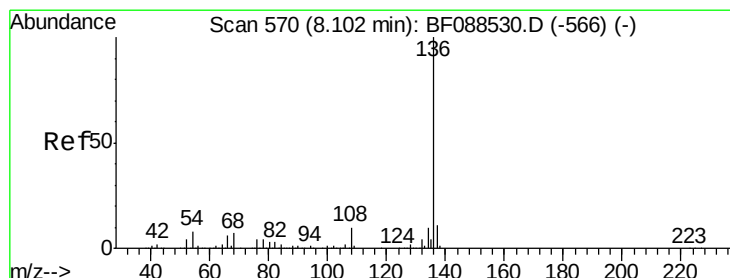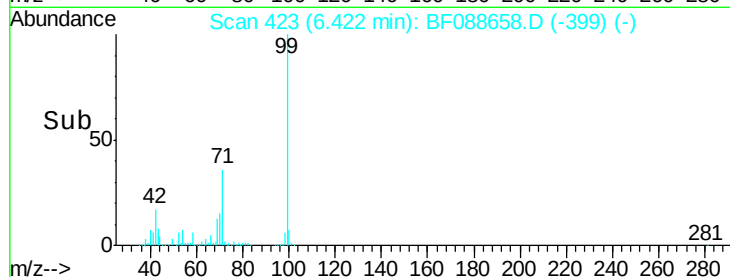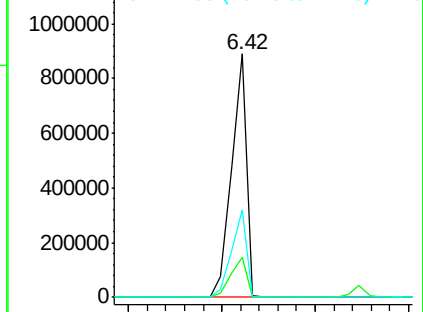

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.07 min Scan# 567

Delta R.T. -0.03 min

Lab File: BF088658.D

Acq: 3 Jul 2016 20:24

Tgt Ion: 136 Resp: 447682


Ion Ratio Lower Upper

136 100



137 11.0 9.1 13.7


54 7.9 6.6 10.0

68 6.9 5.1 7.7

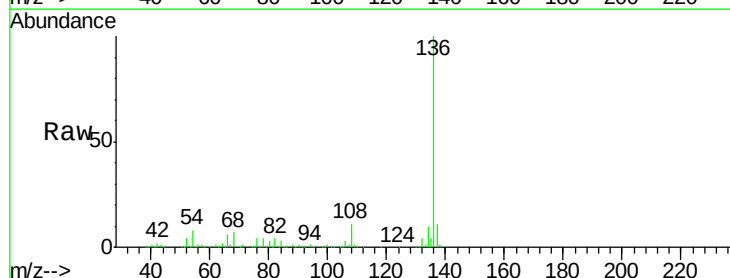

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

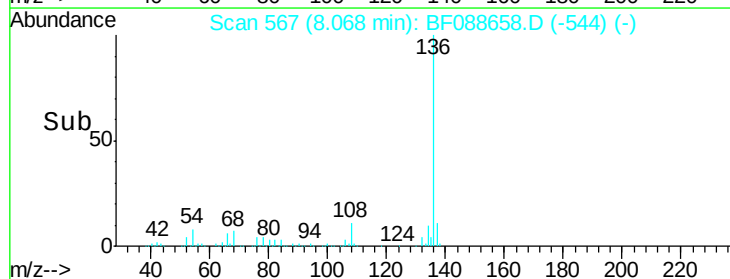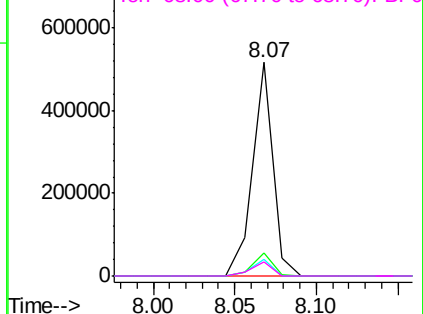


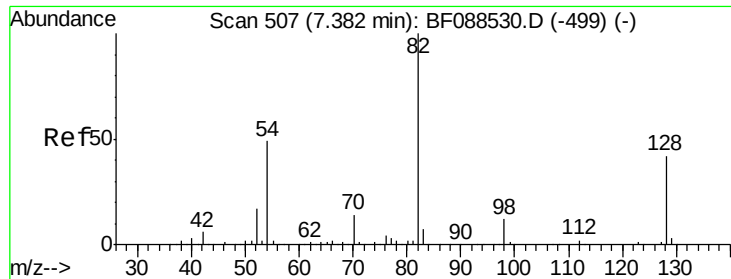




#23
 Nitrobenzene-d5
 Concen: 73.09 ng
 RT: 7.35 min Scan# 504
 Delta R.T. -0.03 min
 Lab File: BF088658.D
 Acq: 3 Jul 2016 20:24

Instrument :
 BNA_F
 ClientSampleId :
 BS-3B-10-10.5FT

Tot Ion	82	Resp	624368
Ion Ratio	100		
Lower	35.9		
Upper	53.9		
54	46.9	40.9	61.3

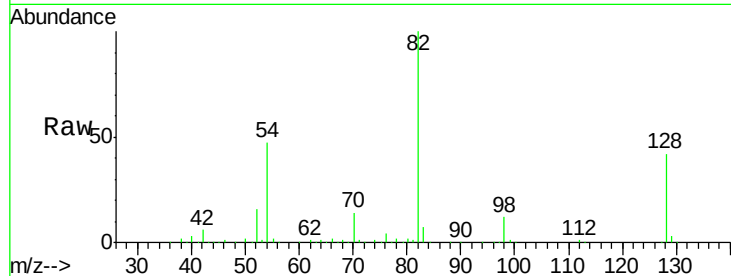


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

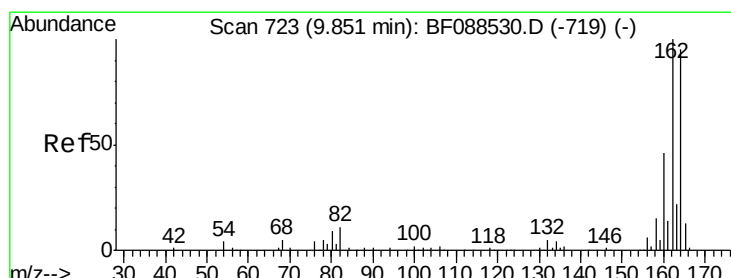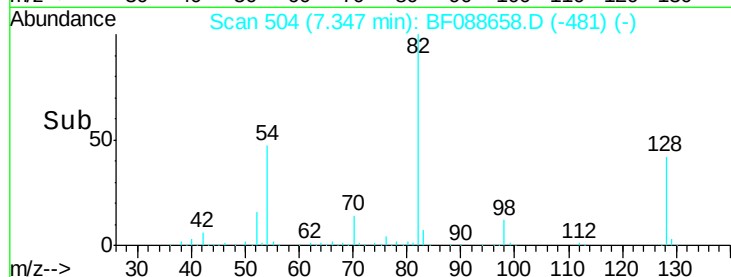
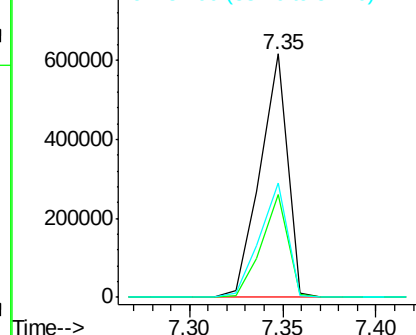



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.82 min Scan# 720
 Delta R.T. -0.03 min
 Lab File: BF088658.D
 Acq: 3 Jul 2016 20:24

Tgt Ion	164	Resp	214982
Ion Ratio	100		
Lower	85.4		
Upper	128.2		
162	105.9	39.5	59.3
160	47.3		

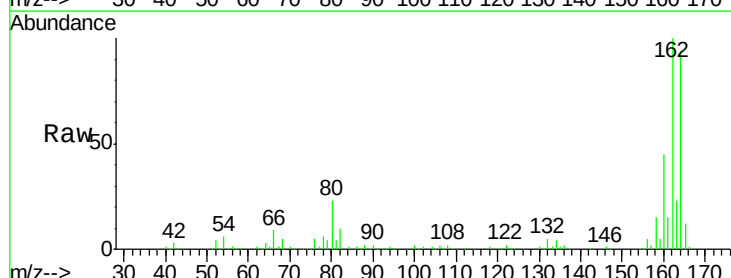

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



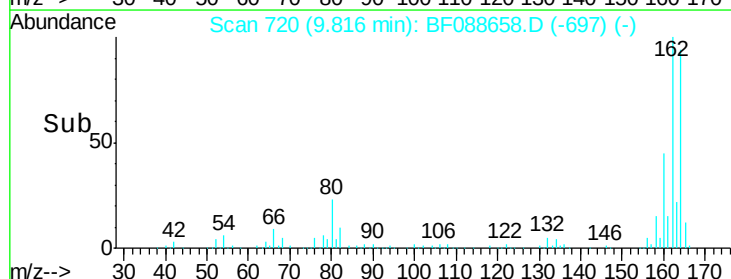
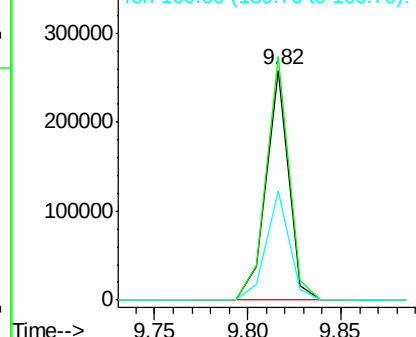


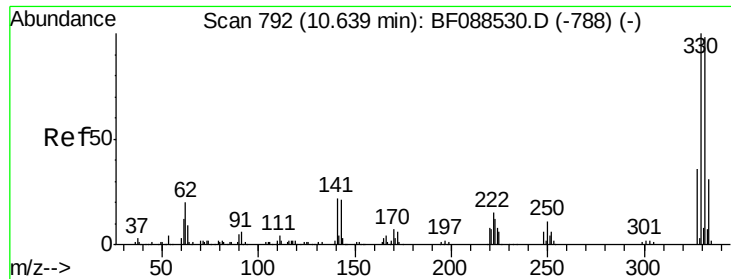

#41
 2,4,6-Tribromophenol
 Concen: 109.98 ng
 RT: 10.60 min Scan# 789
 Delta R.T. -0.03 min
 Lab File: BF088658.D
 Acq: 3 Jul 2016 20:24




Instrument :
 BNA_F
 ClientSampleId :
 BS-3B-10-10.5FT


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	0.0	0.0#
141	40.6	0.0	0.0#

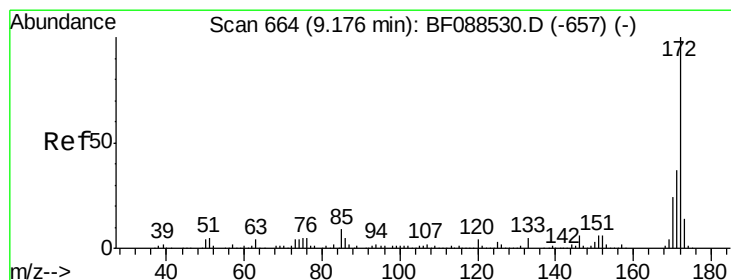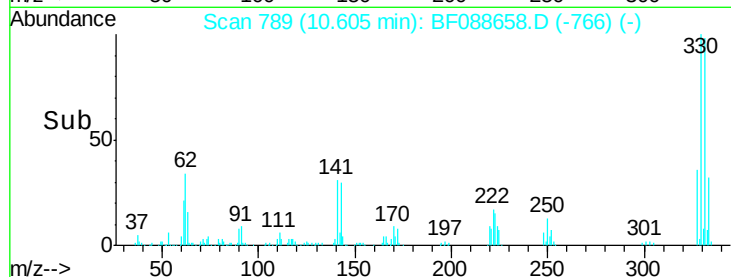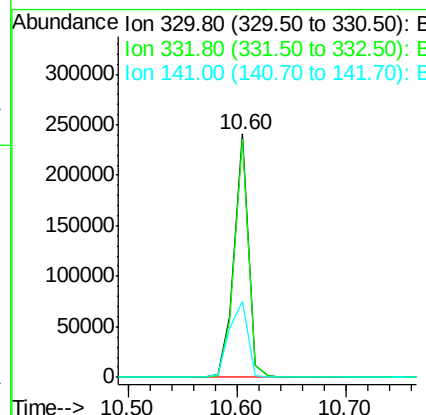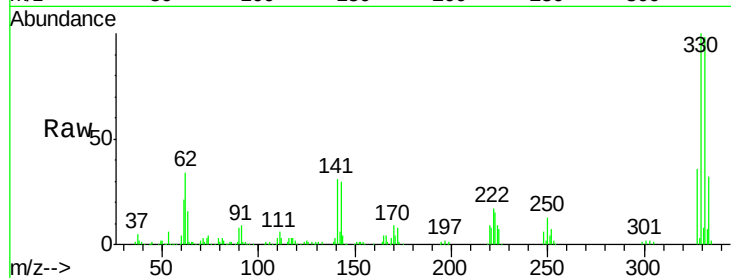

#44
 2-Fluorobiphenyl
 Concen: 62.70 ng
 RT: 9.14 min Scan# 661
 Delta R.T. -0.03 min
 Lab File: BF088658.D
 Acq: 3 Jul 2016 20:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	28.6	43.0
170	24.0	19.2	28.8

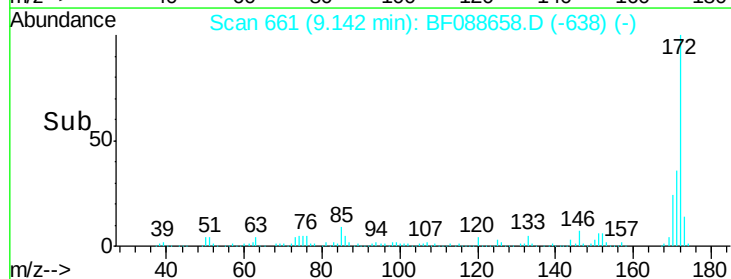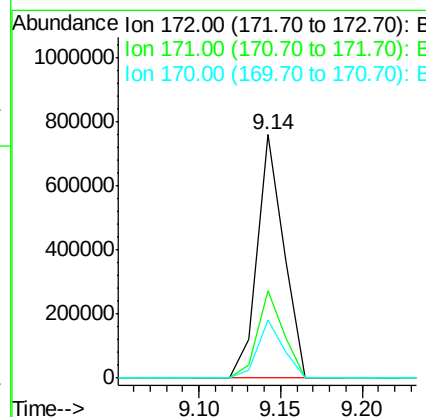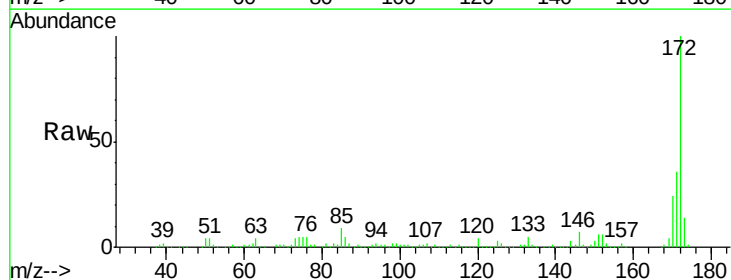


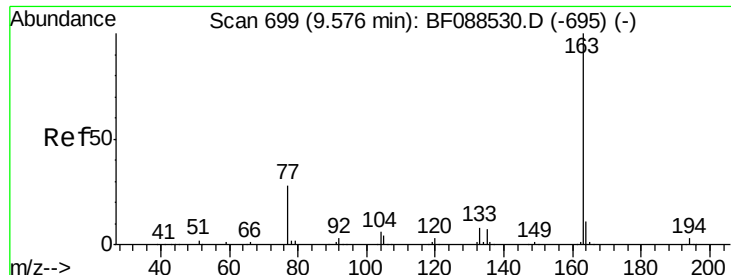




#49
Dimethylphthalate
Concen: 16.37 ng
RT: 9.54 min Scan# 696
Delta R.T. -0.03 min
Lab File: BF088658.D
Acq: 3 Jul 2016 20:24

Instrument :
BNA_F
ClientSampleId :
BS-3B-10-10.5FT

Tot Ion:163 Resp: 250707
Ion Ratio Lower Upper
163 100
194 3.7 2.8 4.2
164 9.7 8.3 12.5

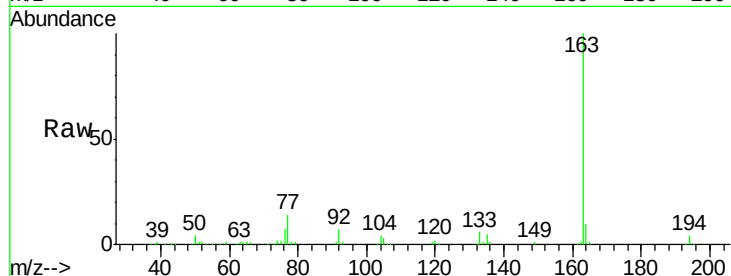


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

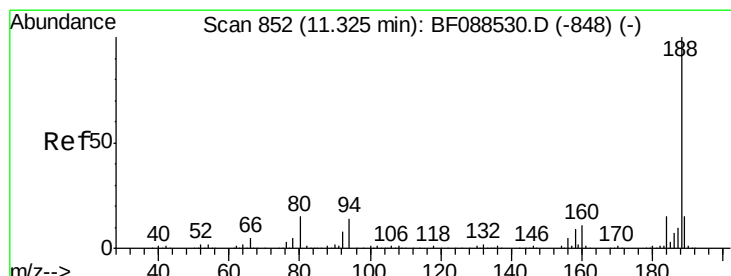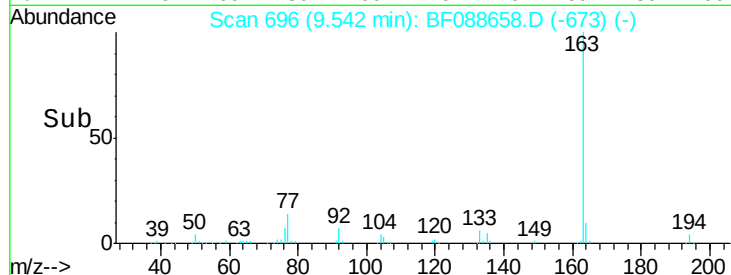
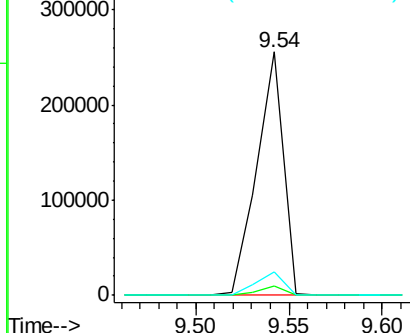



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.29 min Scan# 849
Delta R.T. -0.03 min
Lab File: BF088658.D
Acq: 3 Jul 2016 20:24

Tgt Ion:188 Resp: 389800
Ion Ratio Lower Upper
188 100
94 12.5 9.0 13.6
80 14.3 10.0 15.0

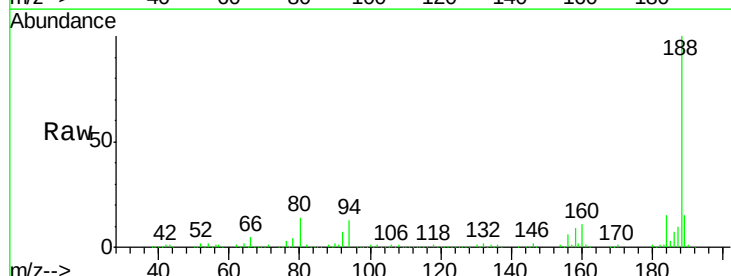

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

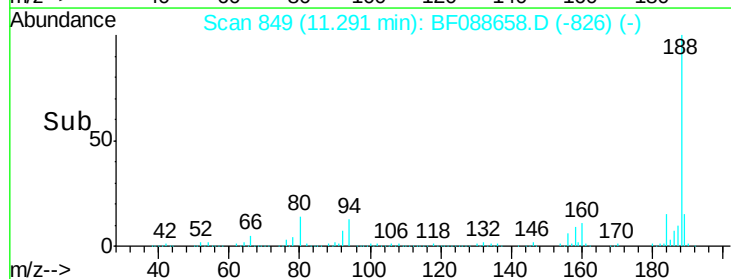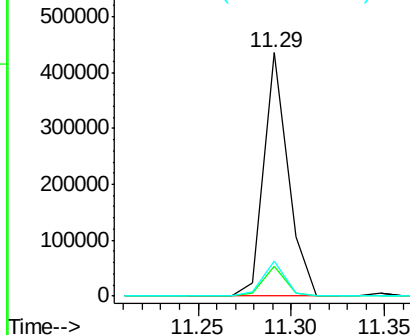

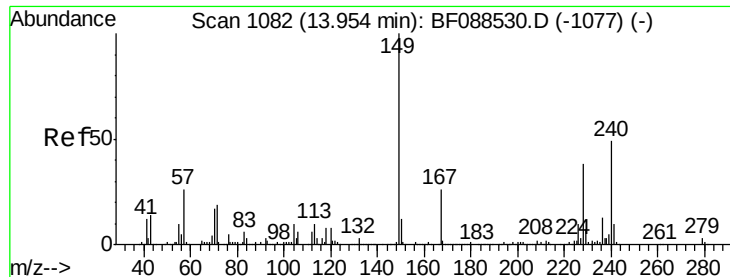

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.92 min Scan# 1079

Delta R.T. -0.03 min

Lab File: BF088658.D

Acq: 3 Jul 2016 20:24

Instrument :

BNA_F

ClientSampleId :

BS-3B-10-10.5FT


Tot Ion:240 Resp: 344918

Ion Ratio Lower Upper




240 100

120 10.5 6.8 10.2#

236 25.7 20.2 30.2

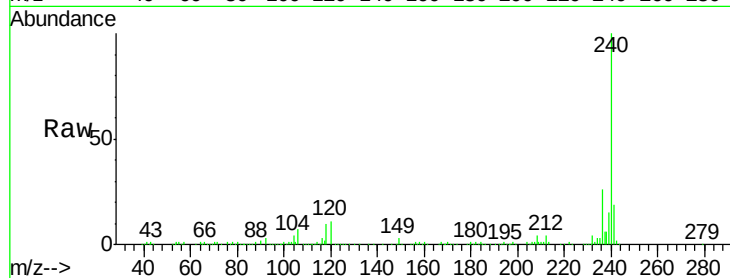

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

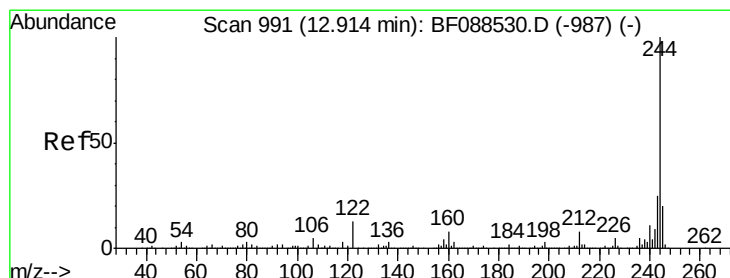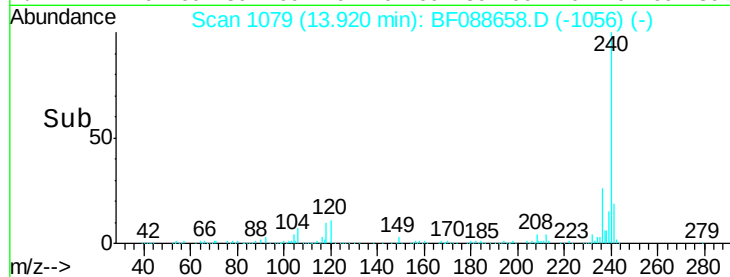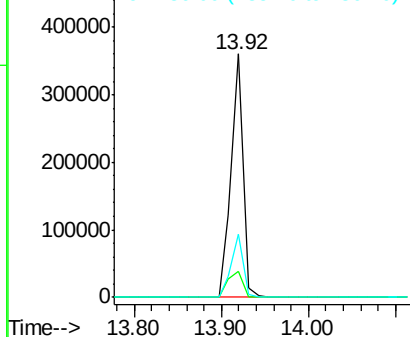

#78

Terphenyl-d14

Concen: 49.30 ng

RT: 12.88 min Scan# 988

Delta R.T. -0.03 min

Lab File: BF088658.D

Acq: 3 Jul 2016 20:24


Tgt Ion:244 Resp: 763408

Ion Ratio Lower Upper



244 100




212 7.9 6.0 9.0

122 12.9 11.2 16.8

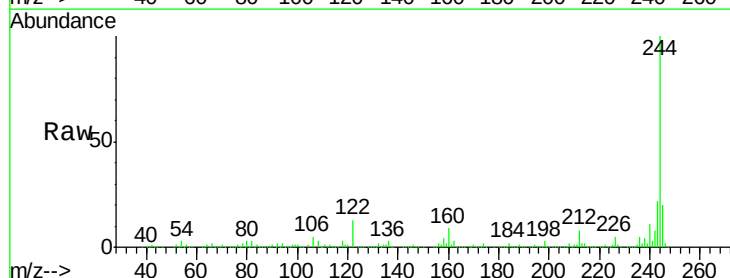

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

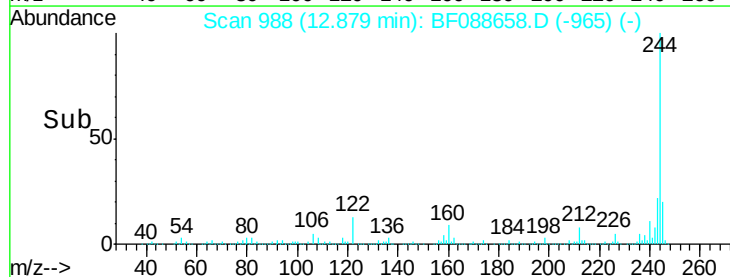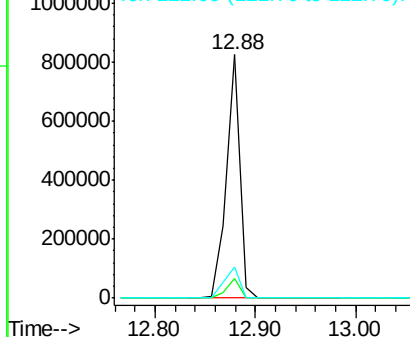

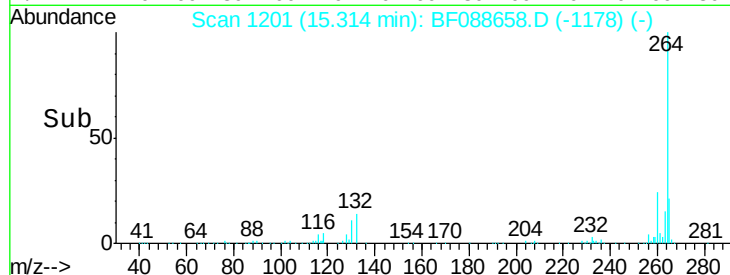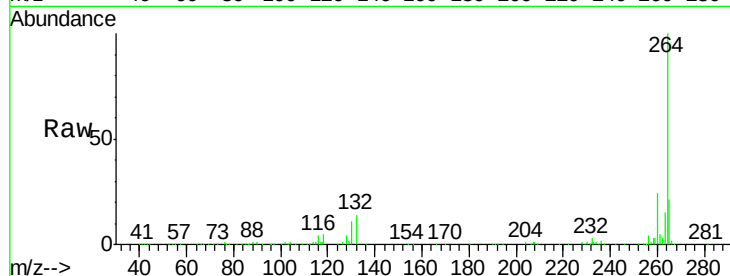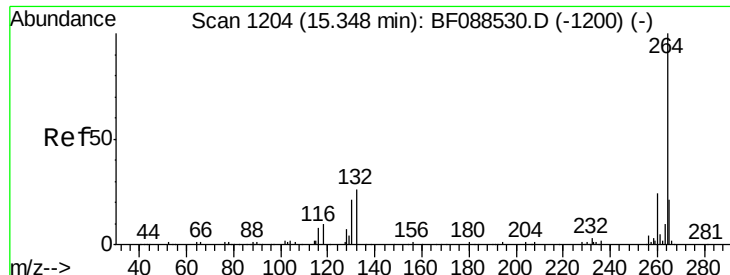

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.31 min Scan# 1201
 Delta R.T. -0.03 min
 Lab File: BF088658.D
 Acq: 3 Jul 2016 20:24

Instrument :
 BNA_F
 ClientSampleId :
 BS-3B-10-10.5FT

Tot Ion:	264	Resp:	267395
Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	21.2	16.9	25.3

