

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070316\
 Data File : BF088695.D
 Acq On : 4 Jul 2016 15:01
 Operator : UM/SJ
 Sample : H3784-08
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D11-B1(0-6)C

Quant Time: Jul 05 01:49:18 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 05 01:06:52 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	111800	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	386441	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	157187	20.00	ng	0.00
63) Phenanthrene-d10	11.30	188	255205	20.00	ng	0.01
75) Chrysene-d12	13.92	240	194859	20.00	ng	0.00
86) Perylene-d12	15.31	264	165418	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	591044	79.23	ng	0.01
7) Phenol-d6	6.42	99	755737	78.40	ng	0.00
23) Nitrobenzene-d5	7.35	82	463861	62.90	ng	0.00
41) 2,4,6-Tribromophenol	10.60	330	124825	85.52	ng	0.00
44) 2-Fluorobiphenyl	9.15	172	909553	91.40	ng	0.00
78) Terphenyl-d14	12.88	244	532087	60.82	ng	0.00
Target Compounds						Qvalue
37) 2-Methylnaphthalene	8.79	142	60109	4.90	ng	98
49) Dimethylphthalate	9.54	163	89669	8.01	ng	98
51) Acenaphthene	9.85	154	34025	3.41	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070316\
Data File : BF088695.D
Acq On : 4 Jul 2016 15:01
Operator : UM/SJ
Sample : H3784-08
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D11-B1(0-6)C

Quant Time: Jul 05 01:49:18 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 01:06:52 2016
Response via : Initial Calibration

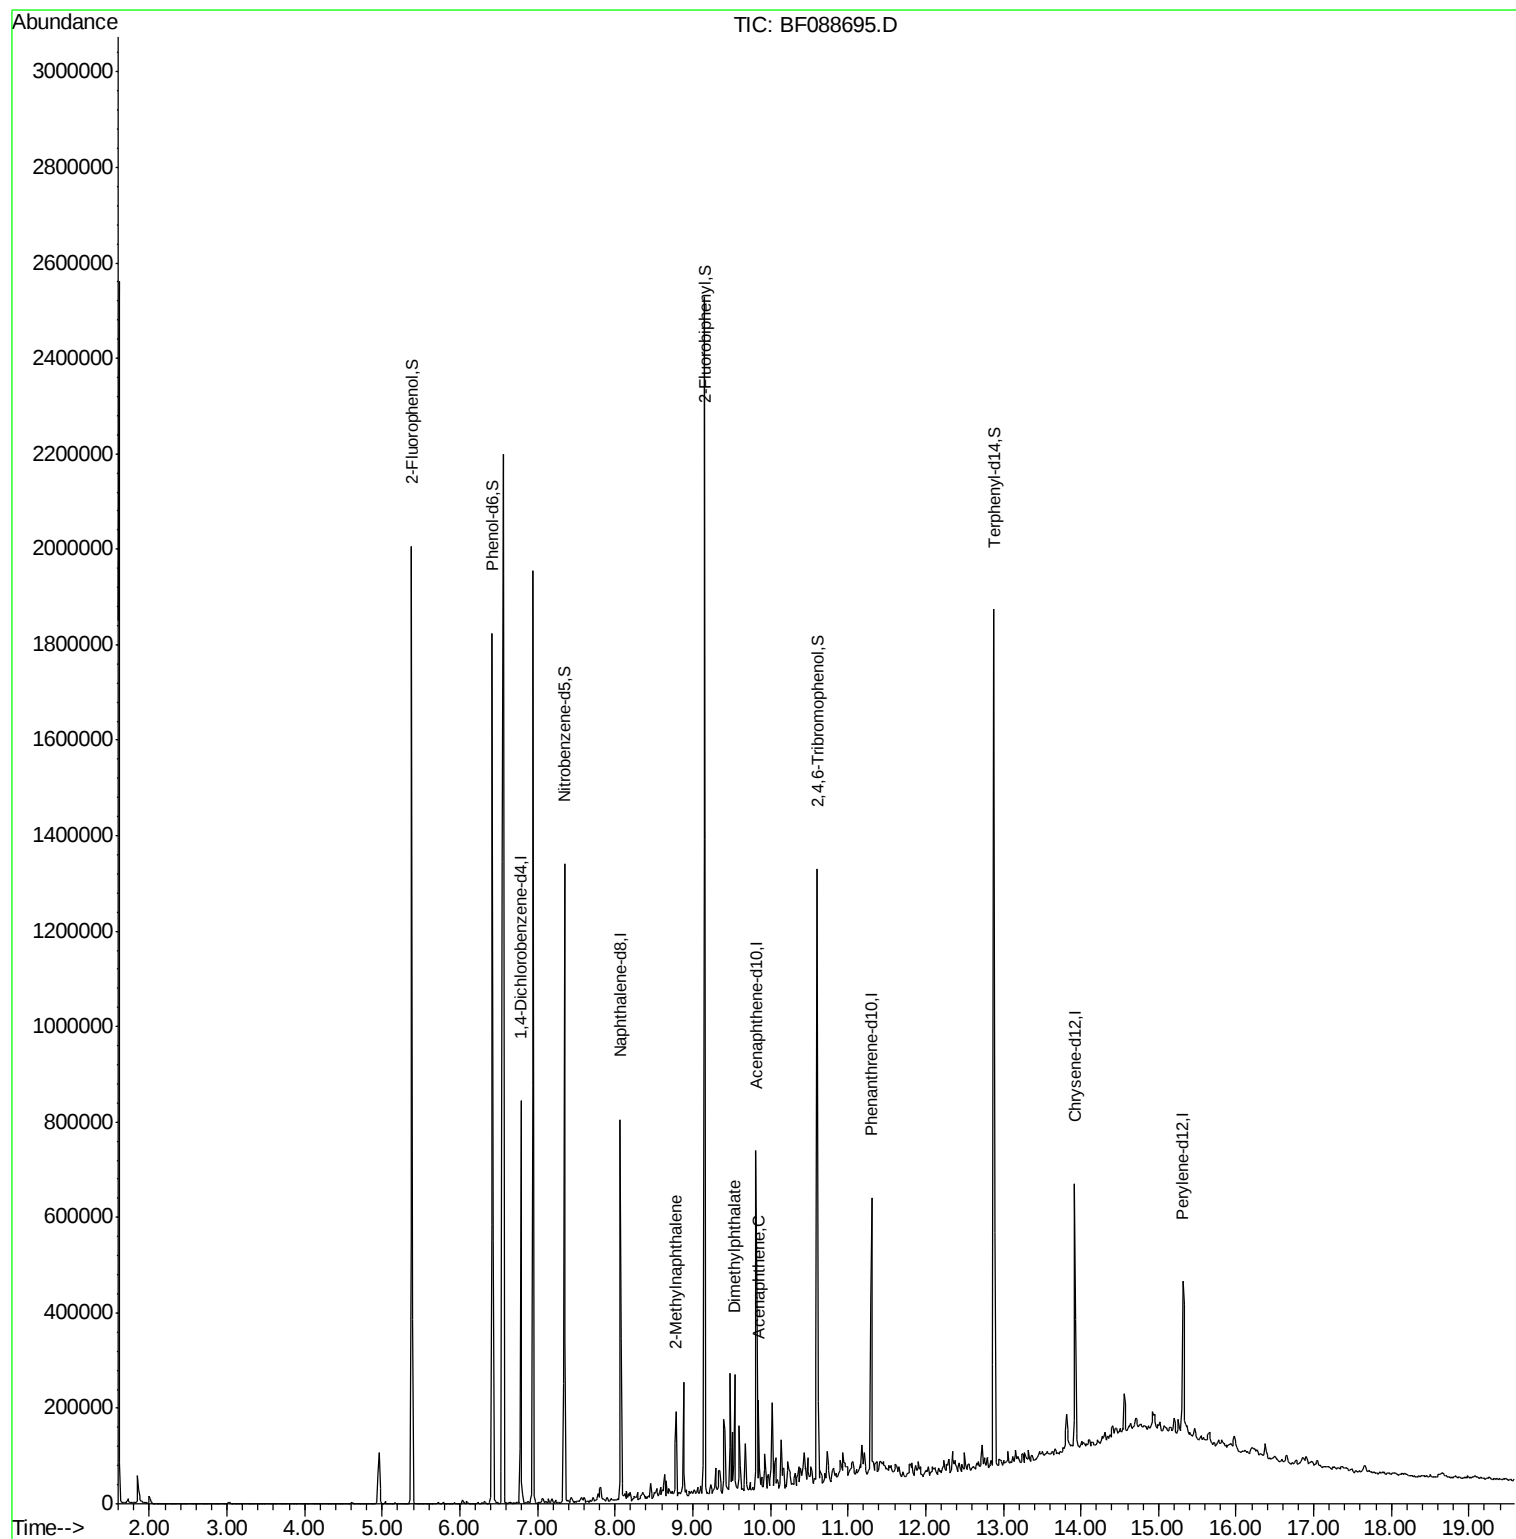



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.79 min Scan# 455

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01

Instrument :

BNA_F

ClientSampleId :

D11-B1(0-6)C


Tot Ion:152 Resp: 111800

Ion Ratio Lower Upper

152 100

150 155.5 123.8 185.6




115 64.3 39.6 59.4#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

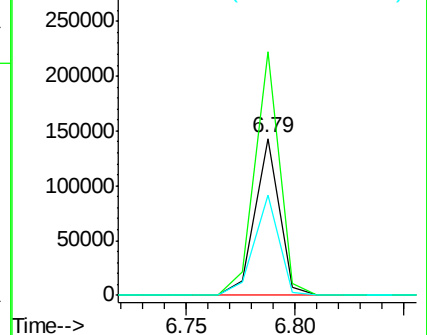

#5

2-Fluorophenol

Concen: 79.23 ng

RT: 5.38 min Scan# 332

Delta R.T. 0.01 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01


Tgt Ion:112 Resp: 591044

Ion Ratio Lower Upper

112 100

64 61.8 42.2 63.2



63 32.5 21.8 32.8



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

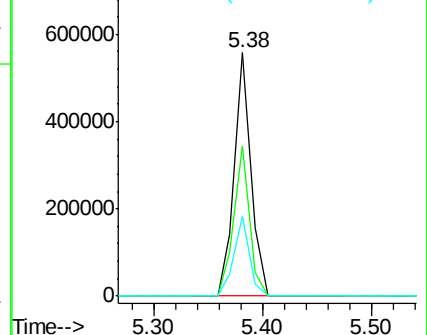



#7

Phenol-d6

Concen: 78.40 ng

RT: 6.42 min Scan# 423

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01

Instrument :

BNA_F

ClientSampleId :

D11-B1(0-6)C





Tot Ion: 99 Resp: 755737

Ion Ratio Lower Upper

99 100

42 17.7 12.2 18.2

71 36.3 23.4 35.0#

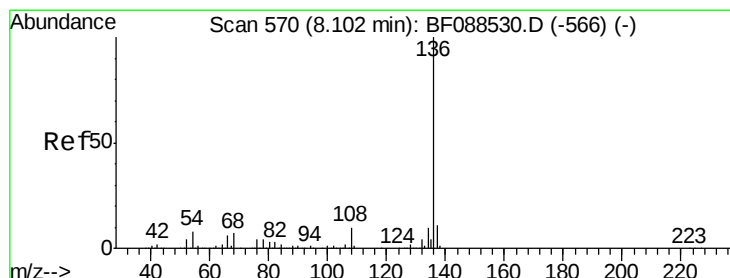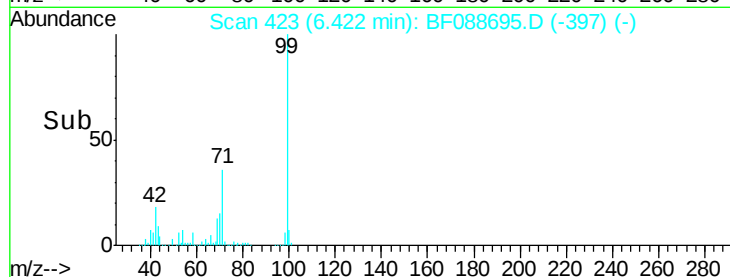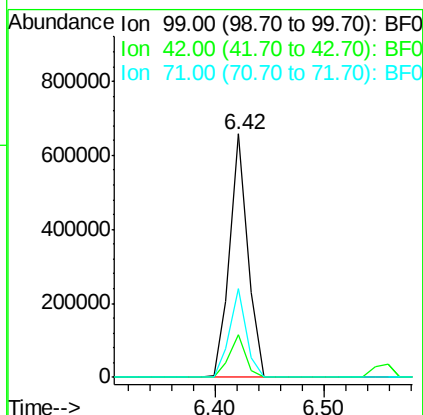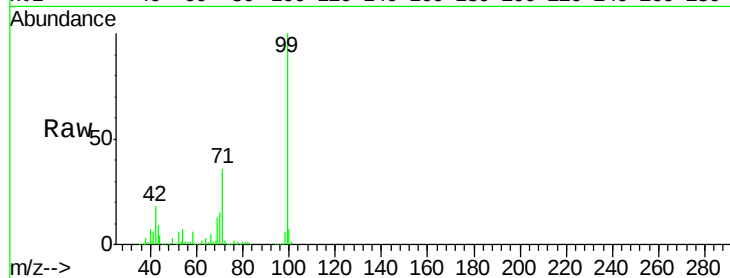

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.07 min Scan# 567

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01

Tgt Ion: 136 Resp: 386441




Ion Ratio Lower Upper


136 100

137 11.4 9.1 13.7

54 9.8 6.6 10.0

68 8.1 5.1 7.7#

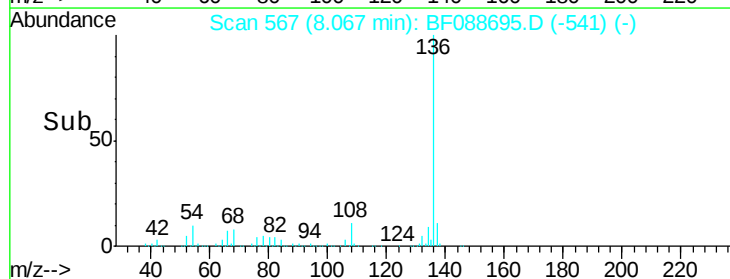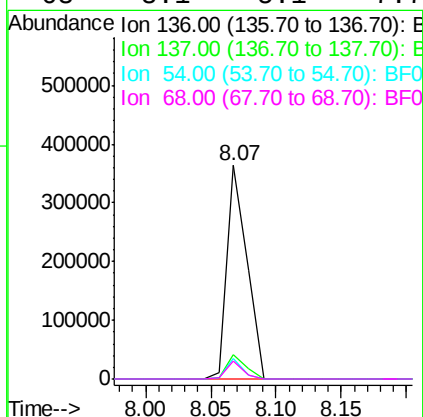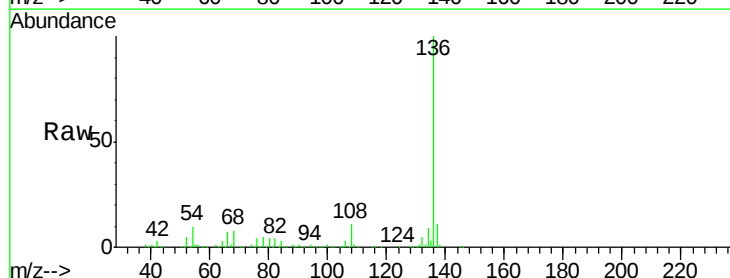







#23
Nitrobenzene-d5
Concen: 62.90 ng
RT: 7.35 min Scan# 504
Delta R.T. 0.00 min
Lab File: BF088695.D
Acq: 4 Jul 2016 15:01

Instrument :
BNA_F
ClientSampleId :
D11-B1(0-6)C

Tot Ion: 82 Resp: 463861
Ion Ratio Lower Upper
82 100
128 40.2 35.9 53.9
54 48.9 40.9 61.3

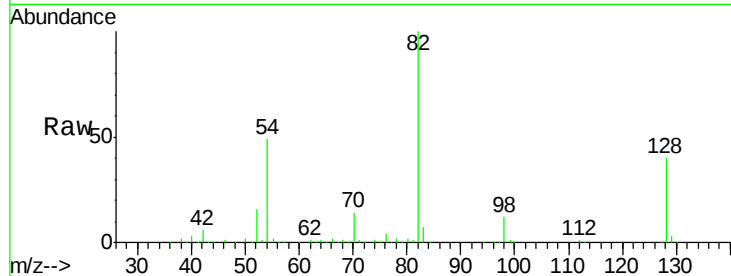


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): B


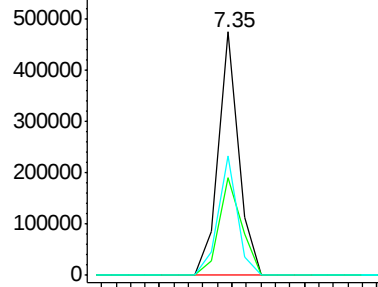



#37
2-Methylnaphthalene
Concen: 4.90 ng
RT: 8.79 min Scan# 630
Delta R.T. 0.00 min
Lab File: BF088695.D
Acq: 4 Jul 2016 15:01

Tgt Ion: 142 Resp: 60109
Ion Ratio Lower Upper
142 100
141 89.7 71.0 106.6
115 31.1 22.6 33.8



Abundance Ion 142.00 (141.70 to 142.70): B
Ion 141.00 (140.70 to 141.70): B
Ion 115.00 (114.70 to 115.70): B

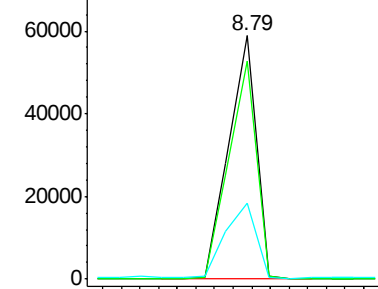

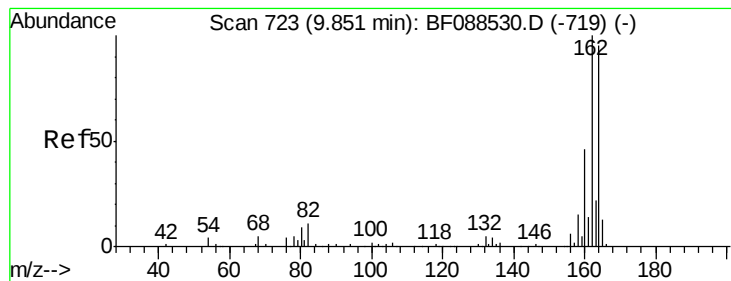

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.82 min Scan# 720

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01

Instrument :

BNA_F

ClientSampleId :

D11-B1(0-6)C


Tot Ion:164 Resp: 157187

Ion Ratio Lower Upper

164 100

162 104.7 85.4 128.2




160 46.3 39.5 59.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

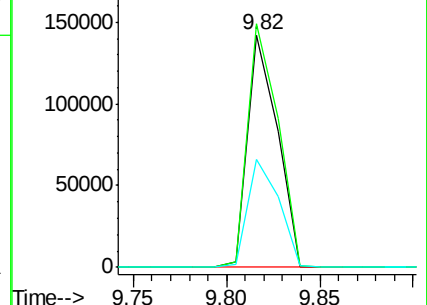

#41

2,4,6-Tribromophenol

Concen: 85.52 ng

RT: 10.60 min Scan# 789

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01


Tgt Ion:330 Resp: 124825

Ion Ratio Lower Upper

330 100

332 97.4 0.0 0.0#



141 46.0 0.0 0.0#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

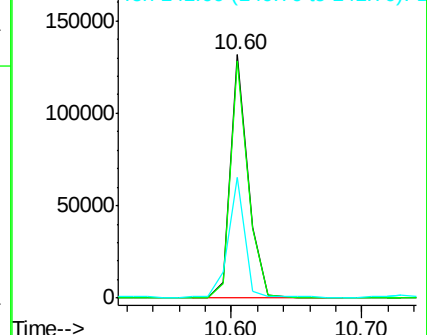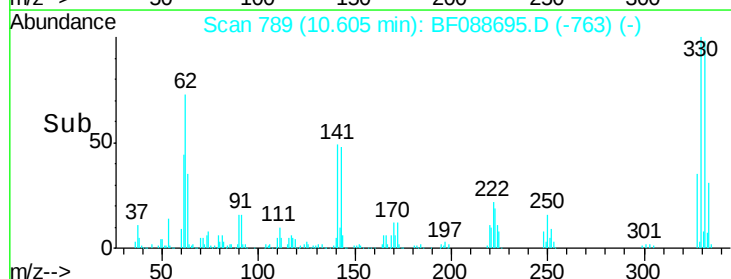







#44
2-Fluorobiphenyl
Concen: 91.40 ng
RT: 9.15 min Scan# 662
Delta R.T. 0.00 min
Lab File: BF088695.D
Acq: 4 Jul 2016 15:01

Instrument :
BNA_F
ClientSampleId :
D11-B1(0-6)C

Tot Ion:172 Resp: 909553
Ion Ratio Lower Upper
172 100
171 36.4 28.6 43.0
170 24.2 19.2 28.8




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


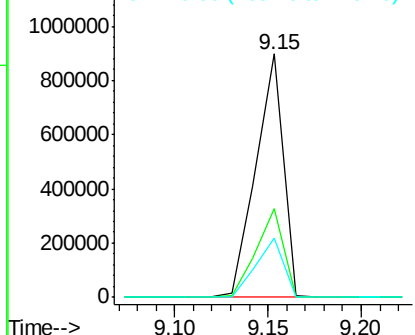



#49
Dimethylphthalate
Concen: 8.01 ng
RT: 9.54 min Scan# 696
Delta R.T. -0.01 min
Lab File: BF088695.D
Acq: 4 Jul 2016 15:01

Tgt Ion:163 Resp: 89669
Ion Ratio Lower Upper
163 100
194 3.9 2.8 4.2
164 9.7 8.3 12.5



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

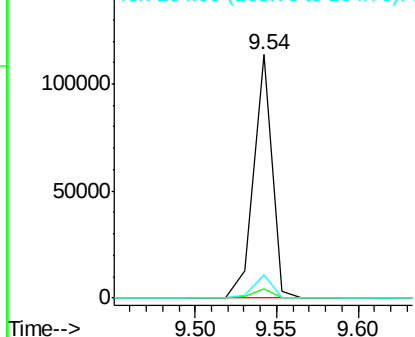



#51

Acenaphthene

Concen: 3.41 ng

RT: 9.85 min Scan# 723

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01

Instrument :

BNA_F

ClientSampleId :

D11-B1(0-6)C


Tot Ion:154 Resp: 34025

Ion Ratio Lower Upper

154 100

153 114.3 89.5 134.3




152 52.7 42.7 64.1

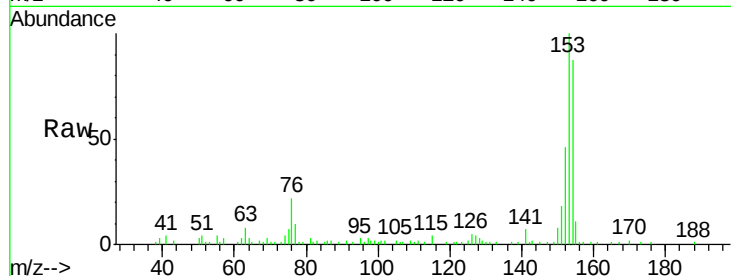

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

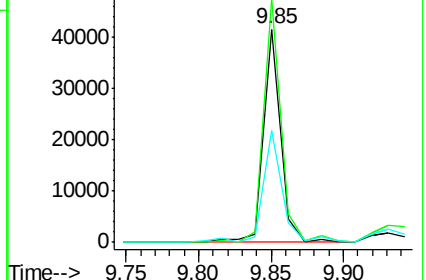

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.30 min Scan# 850

Delta R.T. 0.01 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01


Tgt Ion:188 Resp: 255205

Ion Ratio Lower Upper

188 100

94 7.3 9.0 13.6#



80 7.4 10.0 15.0#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

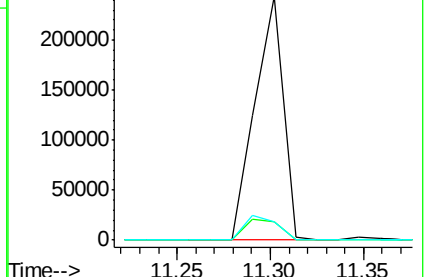



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.92 min Scan# 1079

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01

Instrument :

BNA_F

ClientSampleId :

D11-B1(0-6)C


Tot Ion:240 Resp: 194859

Ion Ratio Lower Upper

240 100

120 17.7 6.8 10.2#




236 25.4 20.2 30.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

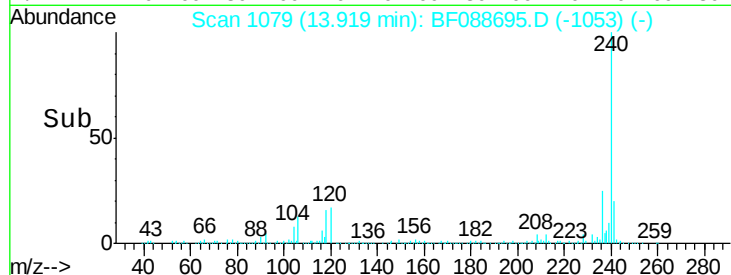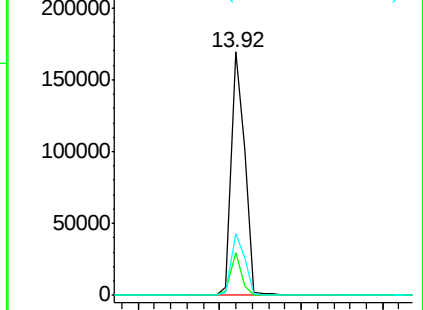

#78

Terphenyl-d14

Concen: 60.82 ng

RT: 12.88 min Scan# 988

Delta R.T. 0.00 min

Lab File: BF088695.D

Acq: 4 Jul 2016 15:01


Tgt Ion:244 Resp: 532087

Ion Ratio Lower Upper

244 100

212 7.9 6.0 9.0



122 16.4 11.2 16.8






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

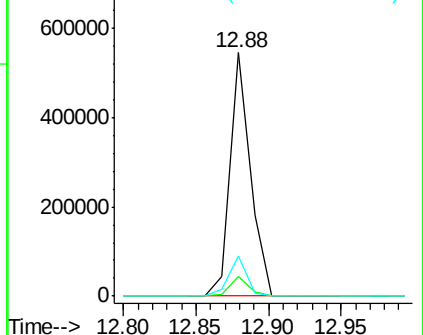

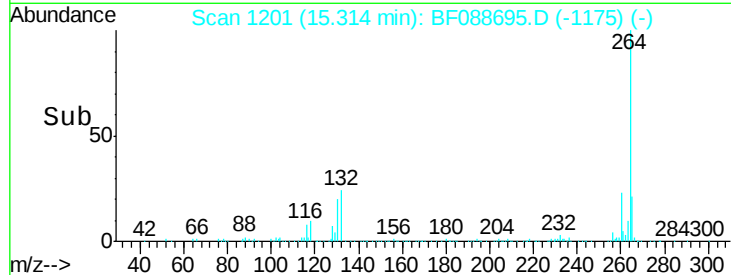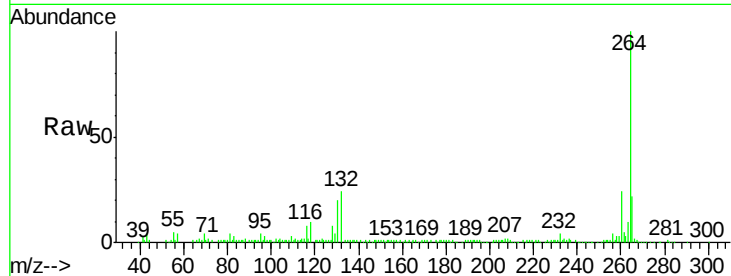

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.31 min Scan# 1201
Delta R.T. 0.00 min
Lab File: BF088695.D
Acq: 4 Jul 2016 15:01

Instrument :
BNA_F
ClientSampleId :
D11-B1(0-6)C

Tot Ion:	264	Resp:	165418
Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.2	28.8
265	21.8	16.9	25.3

