


Data Path : Z:\HPCHEM1\BNA F\DATA\BF070316\
 Data File : BF088636.D
 Acq On : 3 Jul 2016 8:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 17:15:08 2016

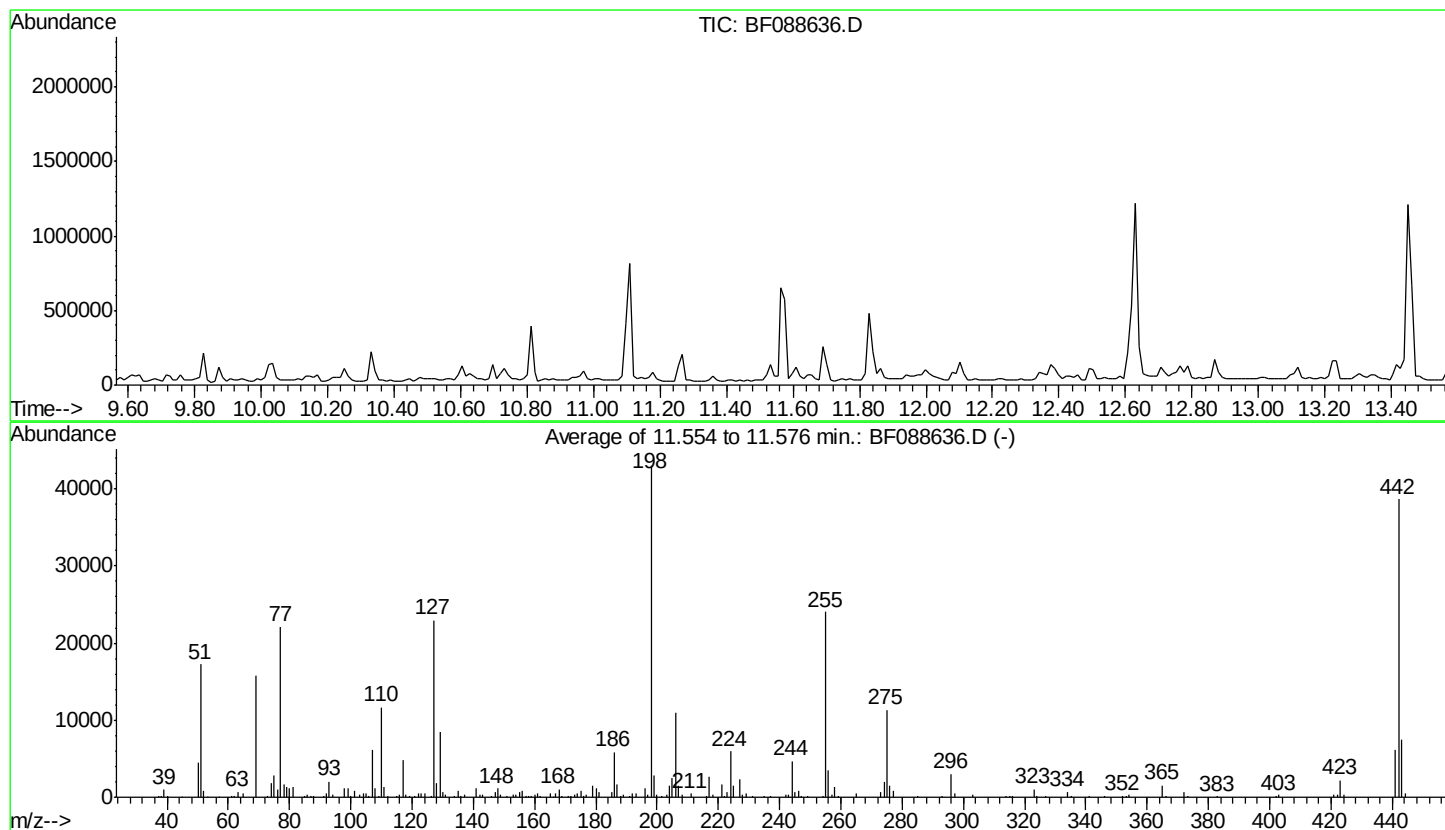

AutoFind: Scans 872, 873, 874; Background Corrected with Scan 869

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	17270	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.8	15823	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	22996	PASS
197	198	0.00	2	0.8	355	PASS
198	198	100	100	100.0	43019	PASS
199	198	5	9	6.6	2822	PASS
275	198	10	60	26.3	11331	PASS
365	198	1	100	3.5	1521	PASS
441	442	0.01	24	15.8	6107	PASS
442	198	50	100	89.9	38661	PASS
443	442	15	24	19.2	7407	PASS