

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070317\
 Data File : BF096463.D
 Acq On : 4 Jul 2017 2:47
 Operator : SJ/MA
 Sample : I4029-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-P4-WSW

Quant Time: Jul 04 04:04:56 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 03 01:43:12 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	110179	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	406687	20.00	ng	-0.01
38) Acenaphthene-d10	9.76	164	138660	20.00	ng	-0.01
63) Phenanthrene-d10	11.24	188	246823	20.00	ng	-0.01
75) Chrysene-d12	13.87	240	183774	20.00	ng	-0.01
86) Perylene-d12	15.28	264	126261	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	509716	68.28	ng	0.00
7) Phenol-d6	6.36	99	543697	59.25	ng	-0.01
23) Nitrobenzene-d5	7.28	82	381051	56.30	ng	-0.02
41) 2,4,6-Tribromophenol	10.55	330	68214	62.98	ng	-0.01
44) 2-Fluorobiphenyl	9.09	172	529140	65.25	ng	-0.01
78) Terphenyl-d14	12.82	244	417065	48.49	ng	-0.01
Target Compounds						
10) Phenol	6.37	94	26656	2.550	ng	90
49) Dimethylphthalate	9.47	163	53693	5.187	ng	97
70) Phenanthrene	11.26	178	27006	2.024	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070317\
Data File : BF096463.D
Acq On : 4 Jul 2017 2:47
Operator : SJ/MA
Sample : I4029-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-P4-WSW

Quant Time: Jul 04 04:04:56 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 03 01:43:12 2017
Response via : Initial Calibration

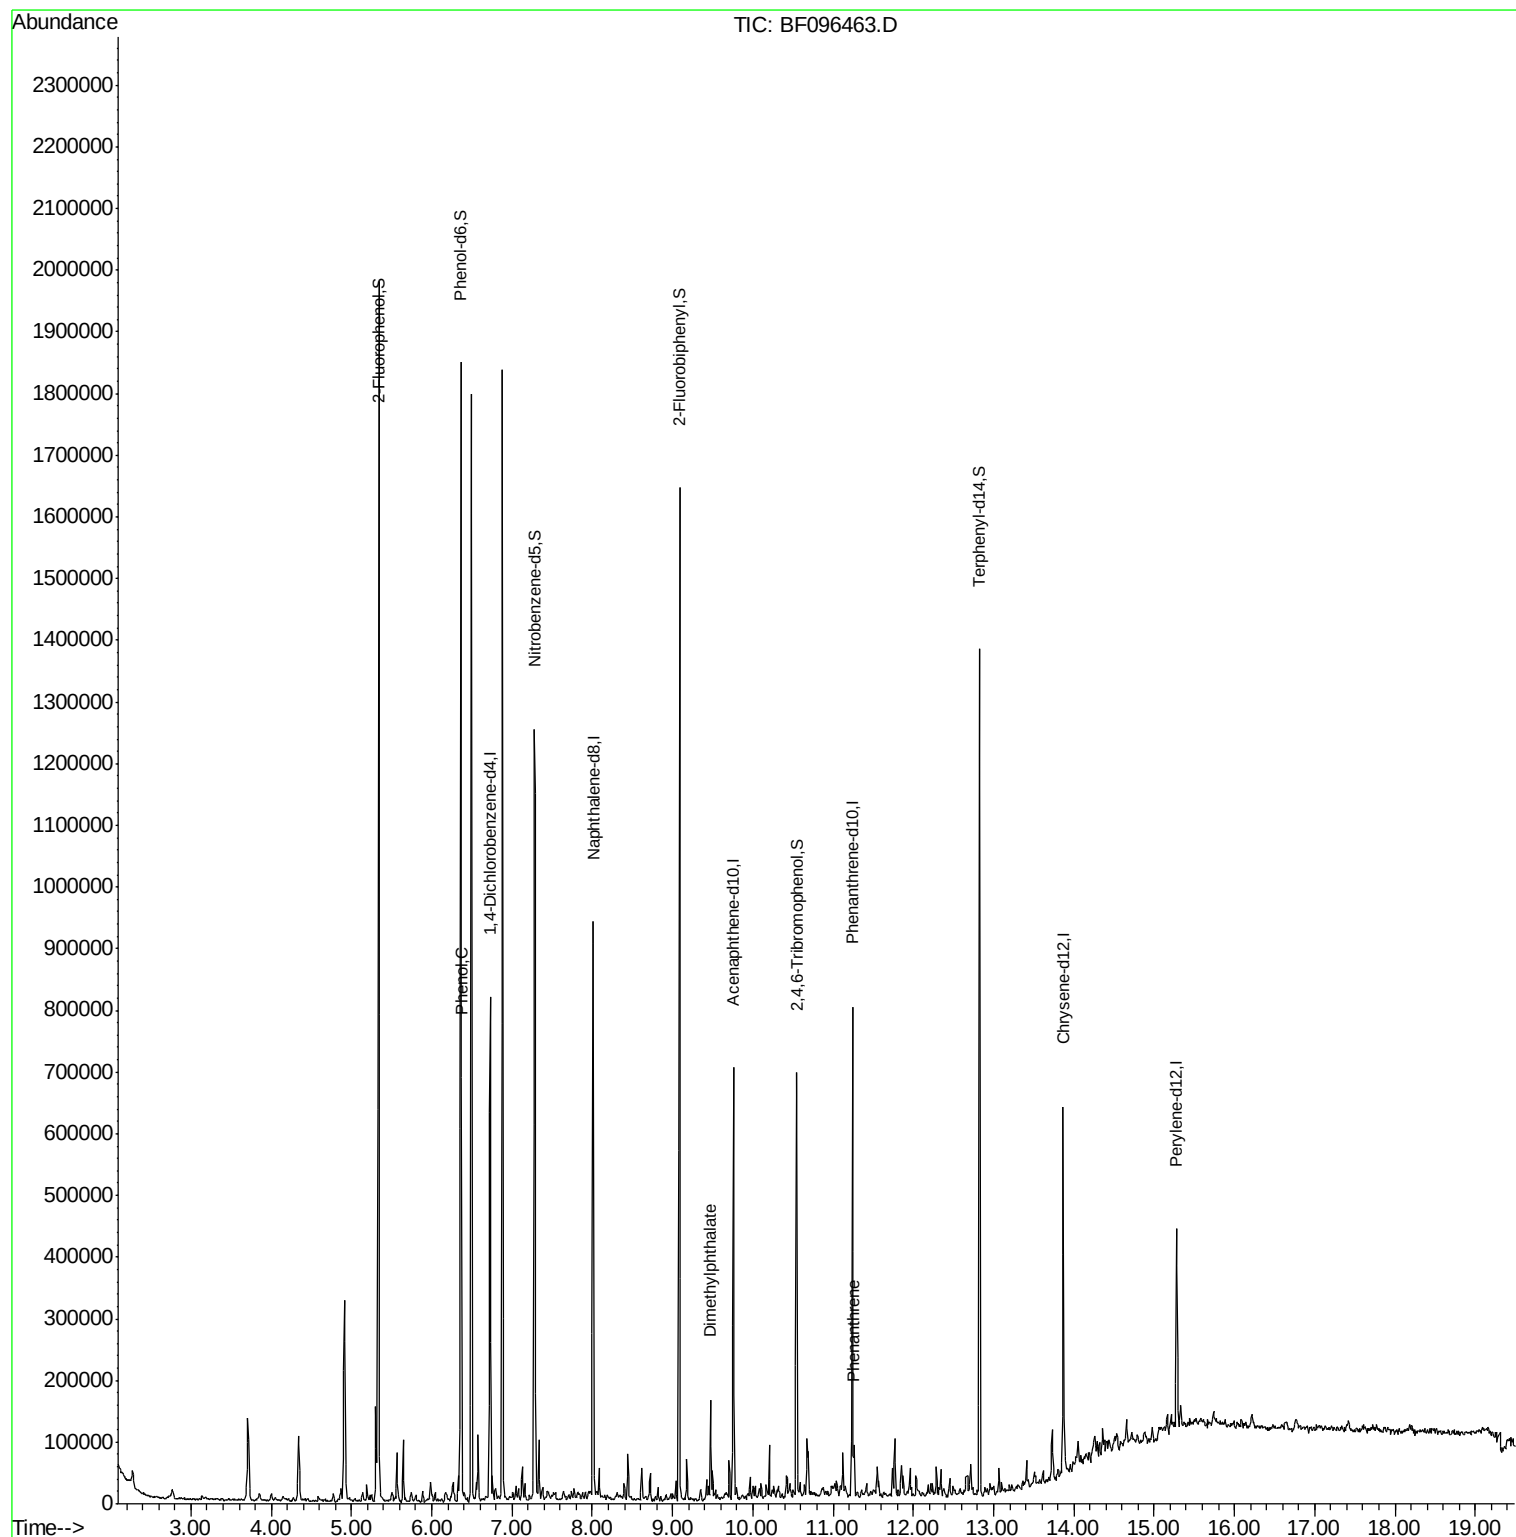







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.73 min Scan# 789
 Delta R.T. -0.01 min
 Lab File: BF096463.D
 Acq: 4 Jul 2017 2:47

Instrument :
 BNA_F
 ClientSampleId :
 E2-P4-WSW

Tgt Ion:152 Resp: 110179
 Ion Ratio Lower Upper
 152 100
 150 158.8 126.2 189.2
 115 64.2 52.2 78.2

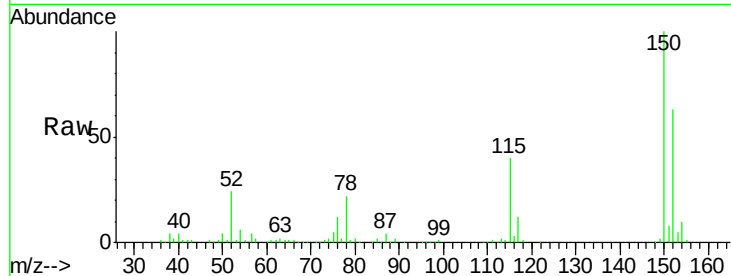


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

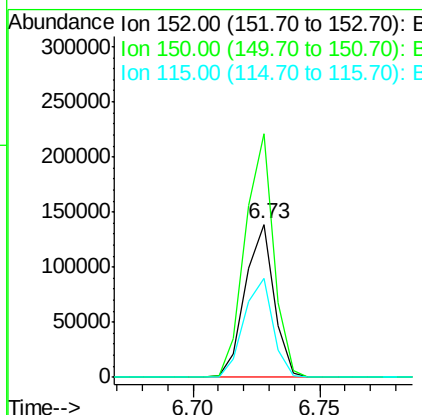




#5
 2-Fluorophenol
 Concen: 68.282 ng
 RT: 5.34 min Scan# 553
 Delta R.T. -0.01 min
 Lab File: BF096463.D
 Acq: 4 Jul 2017 2:47

Tgt Ion:112 Resp: 509716
 Ion Ratio Lower Upper
 112 100
 64 63.9 46.0 69.0
 63 32.1 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

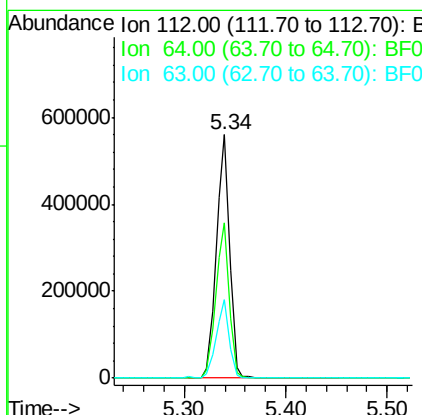

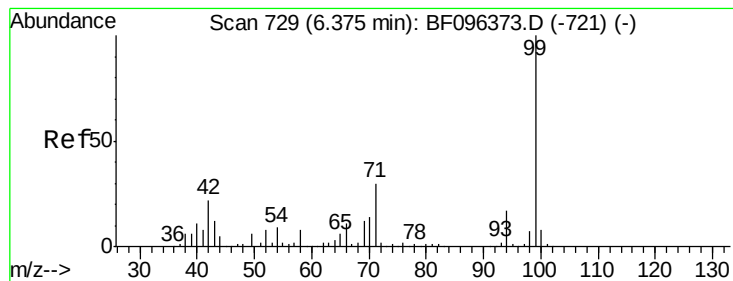

#7

Phenol-d6

Concen: 59.245 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF096463.D

Acq: 4 Jul 2017 2:47

Instrument :

BNA_F

ClientSampleId :

E2-P4-WSW


Tgt Ion: 99 Resp: 543697

Ion Ratio Lower Upper

99 100

42 22.1 13.5 20.3#




71 31.8 24.5 36.7

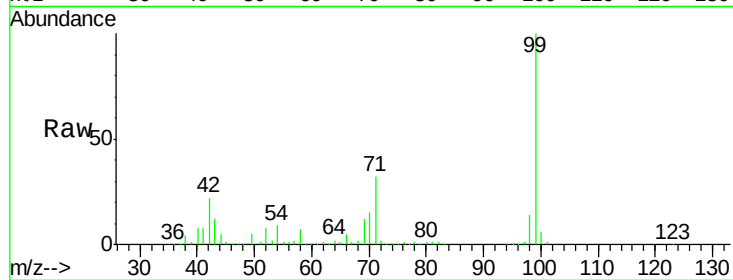

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

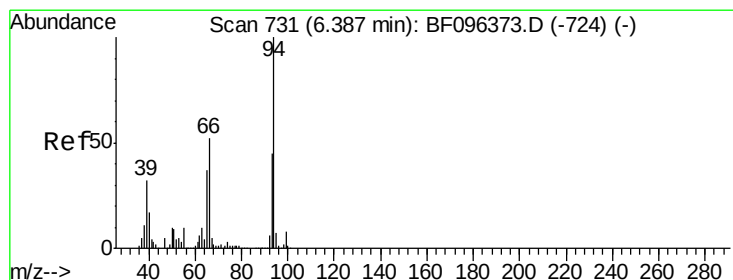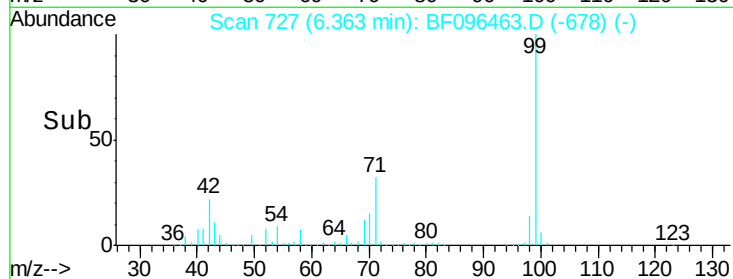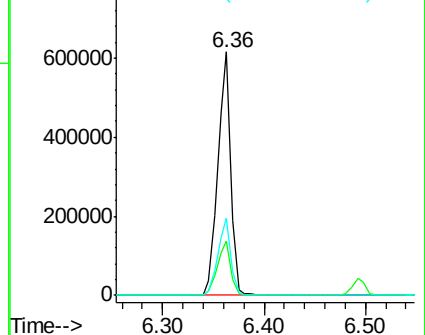

#10

Phenol

Concen: 2.550 ng

RT: 6.37 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF096463.D

Acq: 4 Jul 2017 2:47


Tgt Ion: 94 Resp: 26656

Ion Ratio Lower Upper

94 100

65 27.6 9.9 49.9



66 33.7 23.1 63.1

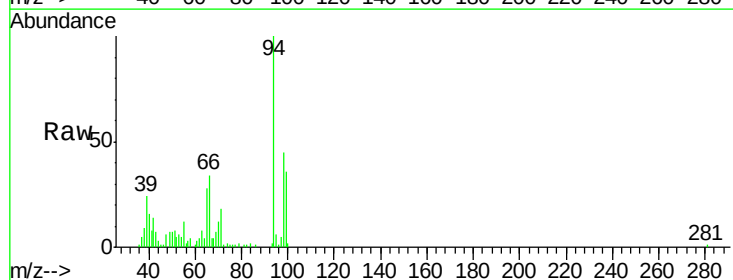


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0



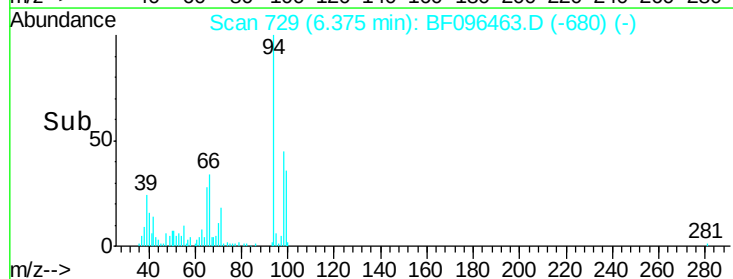
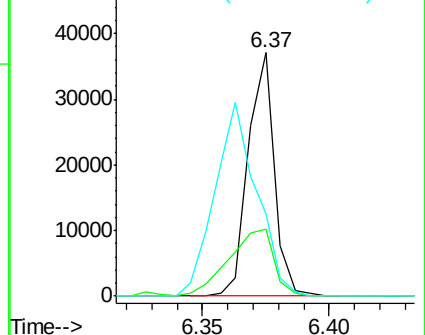




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.01 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BF096463.D
Acq: 4 Jul 2017 2:47




Instrument :
BNA_F
ClientSampleId :
E2-P4-WSW


Tgt Ion:	136	Resp:	406687
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.5	12.7
54	9.4	4.9	7.3#
68	5.8	4.1	6.1

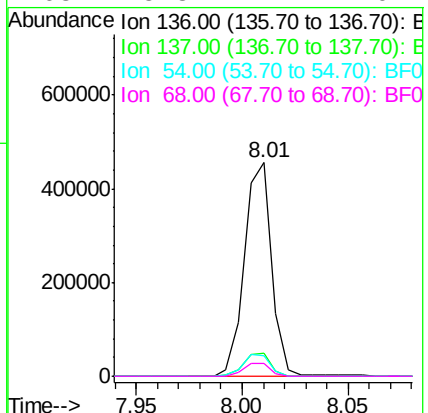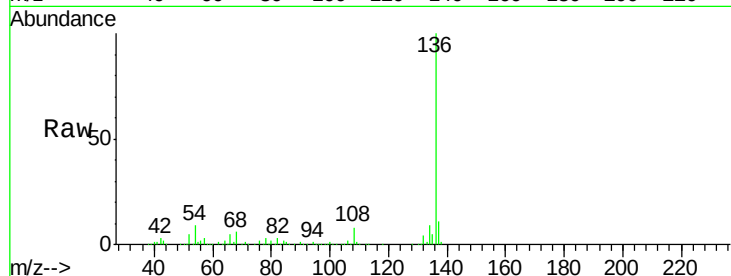

#23
Nitrobenzene-d5
Concen: 56.303 ng
RT: 7.28 min Scan# 883
Delta R.T. -0.02 min
Lab File: BF096463.D
Acq: 4 Jul 2017 2:47

Tgt Ion:	82	Resp:	381051
Ion	Ratio	Lower	Upper
82	100		
128	45.0	34.0	51.0
54	65.9	42.2	63.2#

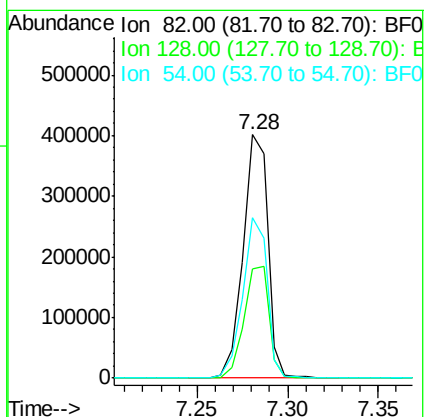



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.76 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BF096463.D

Acq: 4 Jul 2017 2:47

Instrument :

BNA_F

ClientSampleId :

E2-P4-WSW


Tgt Ion:164 Resp: 138660

Ion Ratio Lower Upper

164 100

162 101.2 82.6 123.8




160 45.6 36.2 54.2

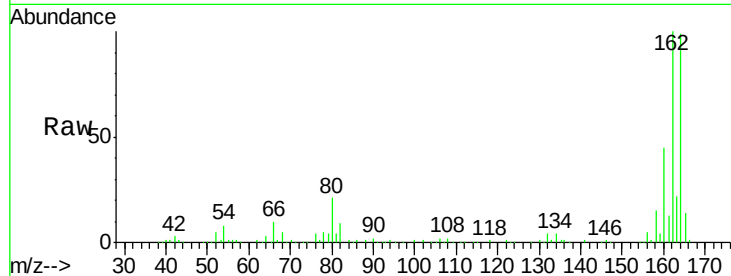

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

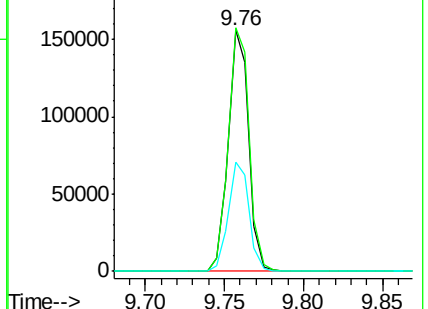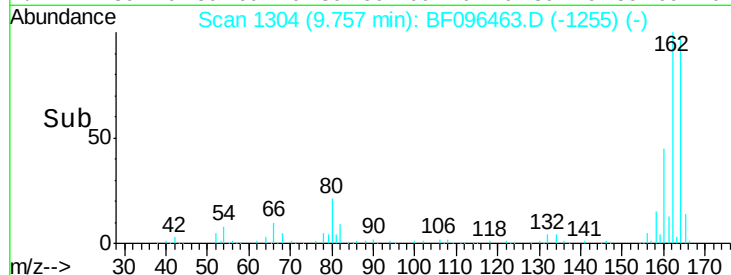

#41

2,4,6-Tribromophenol

Concen: 62.980 ng

RT: 10.55 min Scan# 1438

Delta R.T. -0.01 min

Lab File: BF096463.D

Acq: 4 Jul 2017 2:47


Tgt Ion:330 Resp: 68214

Ion Ratio Lower Upper

330 100

332 95.4 76.6 115.0



141 42.0 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

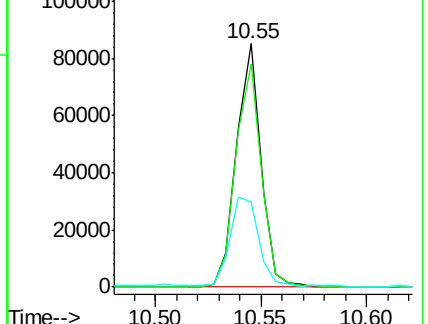







#44
 2-Fluorobiphenyl
 Concen: 65.247 ng
 RT: 9.09 min Scan# 1190
 Delta R.T. -0.01 min
 Lab File: BF096463.D
 Acq: 4 Jul 2017 2:47

Instrument :
 BNA_F
 ClientSampleId :
 E2-P4-WSW

Tgt Ion:172 Resp: 529140
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.6 44.4
 170 23.7 19.8 29.8

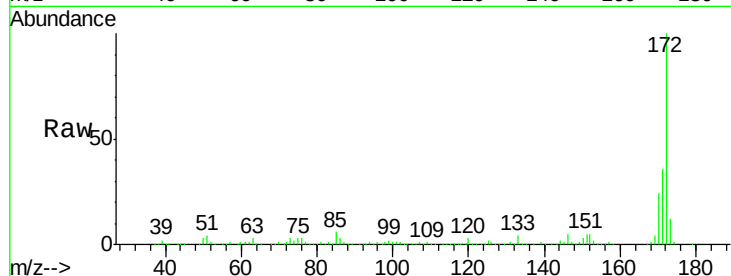


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


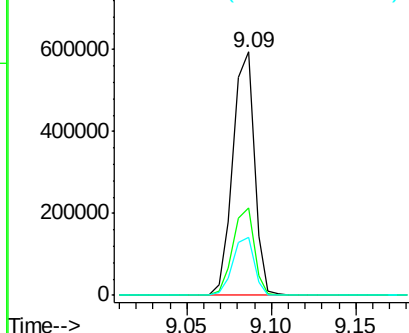



#49
 Dimethylphthalate
 Concen: 5.187 ng
 RT: 9.47 min Scan# 1256
 Delta R.T. -0.02 min
 Lab File: BF096463.D
 Acq: 4 Jul 2017 2:47

Tgt Ion:163 Resp: 53693
 Ion Ratio Lower Upper
 163 100
 194 3.7 2.6 4.0
 164 9.1 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

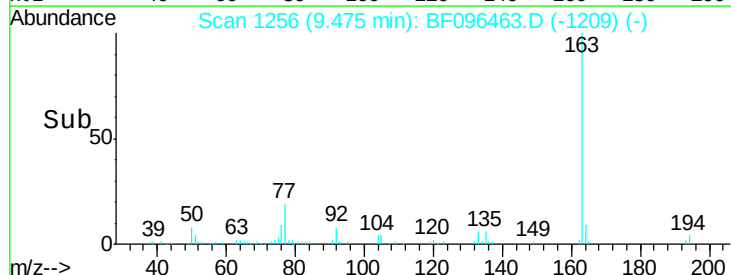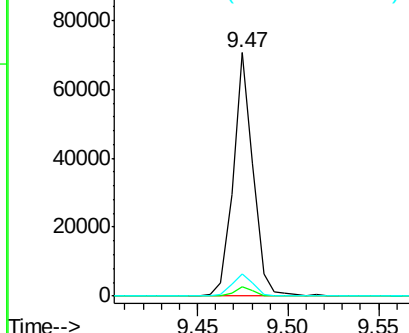


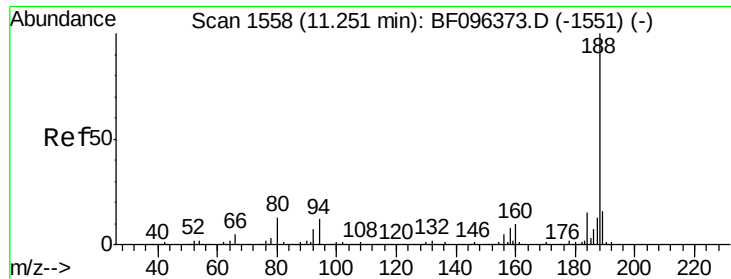


#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF096463.D
Acq: 4 Jul 2017 2:47

Instrument :
BNA_F
ClientSampleId :
E2-P4-WSW



Tgt Ion:188 Resp: 246823
Ion Ratio Lower Upper
188 100
94 11.8 9.4 14.2
80 12.1 10.2 15.2



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

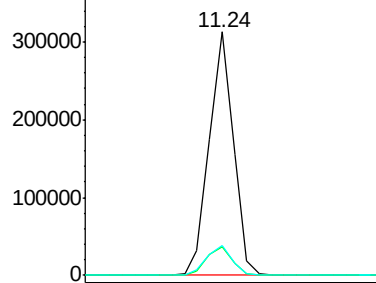


Time-->

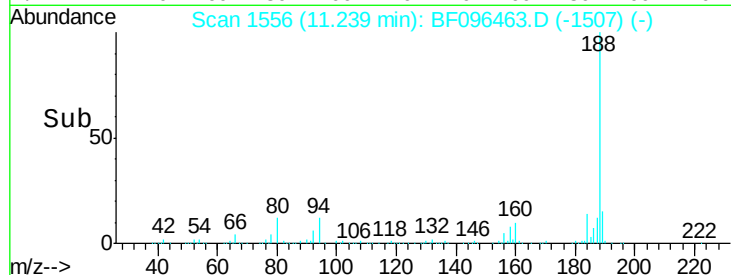


#70
Phenanthrene
Concen: 2.024 ng
RT: 11.26 min Scan# 1560
Delta R.T. -0.01 min
Lab File: BF096463.D
Acq: 4 Jul 2017 2:47


Tgt Ion:178 Resp: 27006
Ion Ratio Lower Upper
178 100
176 19.0 16.2 24.4
179 16.8 12.6 19.0




Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

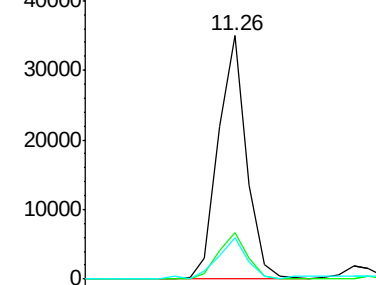

Time-->

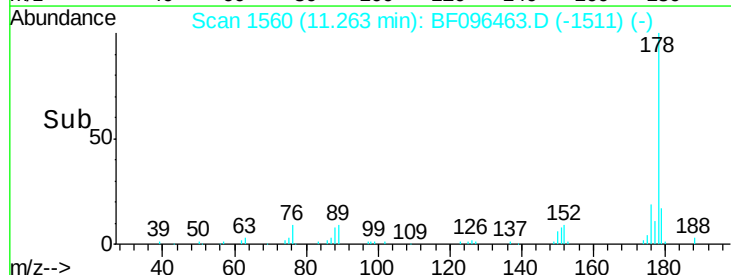

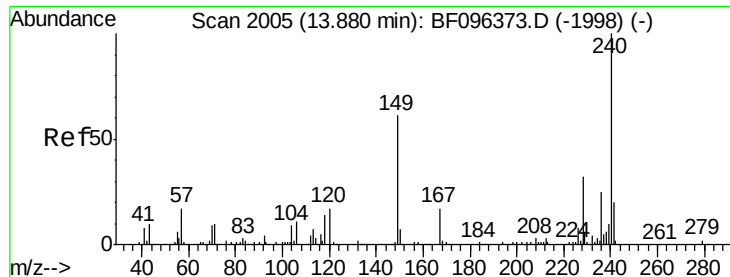

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 2003

Delta R.T. -0.01 min

Lab File: BF096463.D

Acq: 4 Jul 2017 2:47

Instrument :

BNA_F

ClientSampleId :

E2-P4-WSW


Tgt Ion:240 Resp: 183774

Ion Ratio Lower Upper

240 100

120 16.1 5.8 8.8#




236 25.8 20.5 30.7

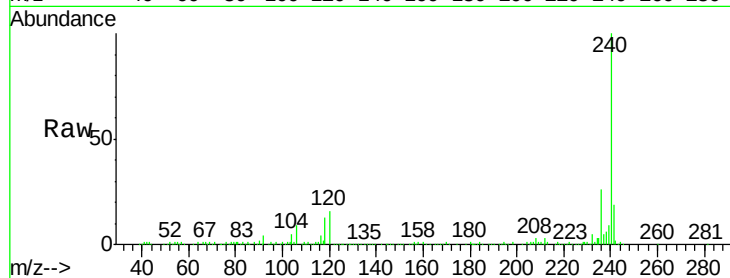

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

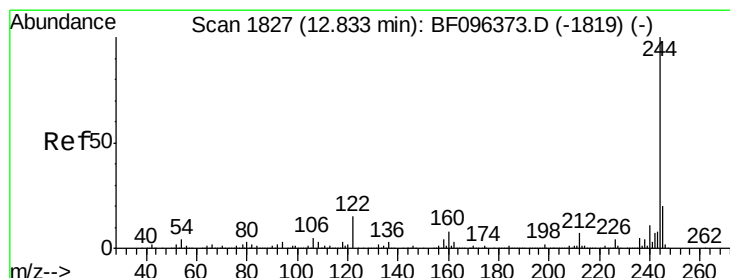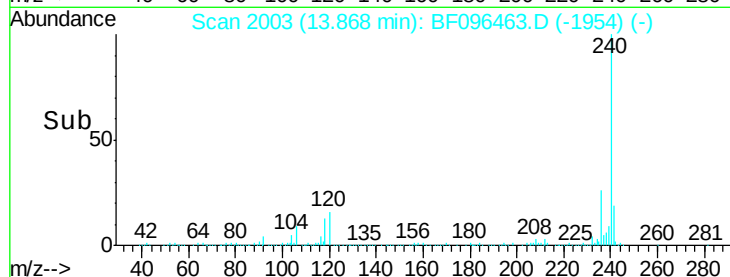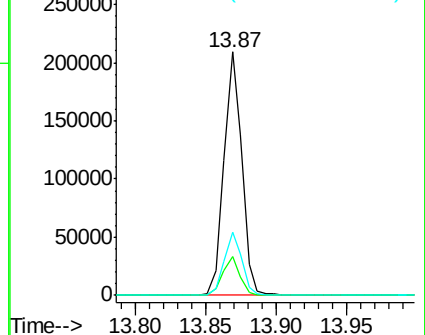

#78

Terphenyl-d14

Concen: 48.494 ng

RT: 12.82 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BF096463.D

Acq: 4 Jul 2017 2:47


Tgt Ion:244 Resp: 417065

Ion Ratio Lower Upper

244 100

212 6.5 6.0 9.0



122 15.4 10.3 15.5

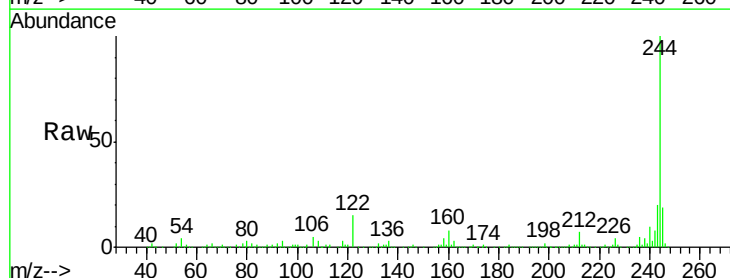


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

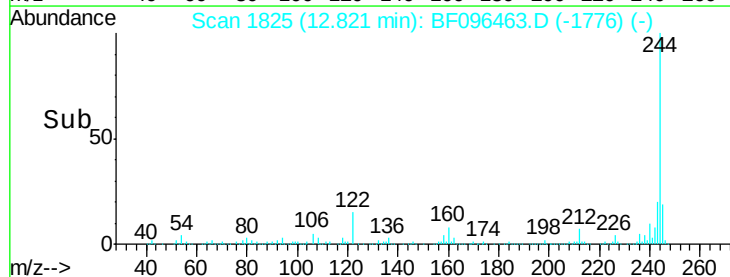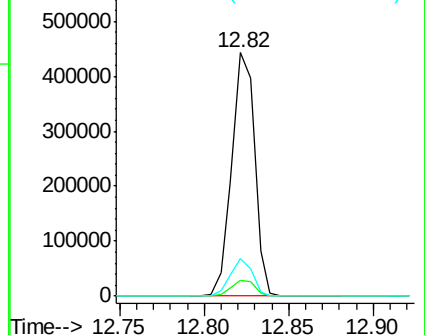

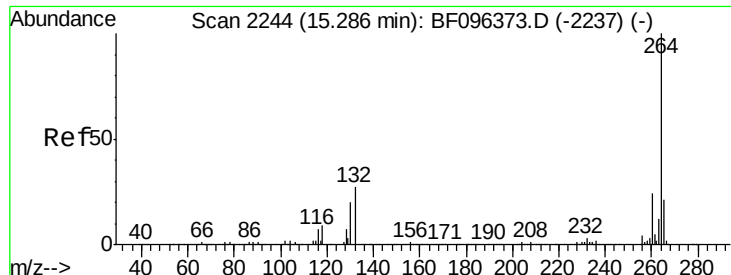

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.28 min Scan# 2243
Delta R.T. -0.01 min
Lab File: BF096463.D
Acq: 4 Jul 2017 2:47

Instrument :
BNA_F
ClientSampleId :
E2-P4-WSW

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.5	29.3
265	21.7	17.2	25.8

