

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070317\
 Data File : BF096435.D
 Acq On : 3 Jul 2017 12:28
 Operator : SJ/MA
 Sample : I3908-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-55-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	474	478	481	rBV	18270	19953	1.75%	0.291%
2	5.322	546	550	555	rBV	150043	131244	11.51%	1.913%
3	6.345	721	724	729	rBV	162149	141968	12.45%	2.070%
4	6.487	744	748	751	rBV	167671	145541	12.76%	2.122%
5	6.722	784	788	791	rBV	977950	814004	71.37%	11.867%
6	6.875	810	814	817	rBV	113674	91533	8.03%	1.334%
7	7.275	878	882	885	rBV	100304	82772	7.26%	1.207%
8	8.004	1001	1006	1009	rBV	1389417	1140505	100.00%	16.627%
9	9.010	1172	1177	1183	rBV5	6297	17283	1.52%	0.252%
10	9.080	1185	1189	1194	rVB	180418	162089	14.21%	2.363%
11	9.469	1253	1255	1260	rVB	26858	21073	1.85%	0.307%
12	9.616	1275	1280	1283	rBV4	11952	23628	2.07%	0.344%
13	9.663	1283	1288	1293	rVB4	16044	29476	2.58%	0.430%
14	9.757	1299	1304	1307	rBV	1308315	1136762	99.67%	16.573%
15	9.963	1329	1339	1341	rBV5	10572	16470	1.44%	0.240%
16	10.533	1433	1436	1440	rBV	83485	72475	6.35%	1.057%
17	11.110	1531	1534	1539	rVB4	8985	13619	1.19%	0.199%
18	11.233	1551	1555	1559	rBV	1262283	1079415	94.64%	15.737%
19	11.769	1642	1646	1655	rVV4	43812	59311	5.20%	0.865%
20	11.839	1655	1658	1661	rVB5	11796	14216	1.25%	0.207%
21	12.163	1710	1713	1716	rBV5	10486	14557	1.28%	0.212%
22	12.439	1757	1760	1763	rBV	31817	28976	2.54%	0.422%
23	12.557	1777	1780	1784	rBV2	53666	56719	4.97%	0.827%
24	12.663	1793	1798	1802	rBV2	25231	42740	3.75%	0.623%
25	12.816	1818	1824	1827	rBV	148827	132074	11.58%	1.925%
26	13.068	1863	1867	1871	rBV7	15531	25958	2.28%	0.378%
27	13.863	1998	2002	2006	rBV	801725	718196	62.97%	10.471%
28	15.274	2238	2242	2246	rBV	541617	626668	54.95%	9.136%


Sum of corrected areas: 6859225

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070317\
Data File : BF096435.D
Acq On : 3 Jul 2017 12:28
Operator : SJ/MA
Sample : I3908-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-55-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

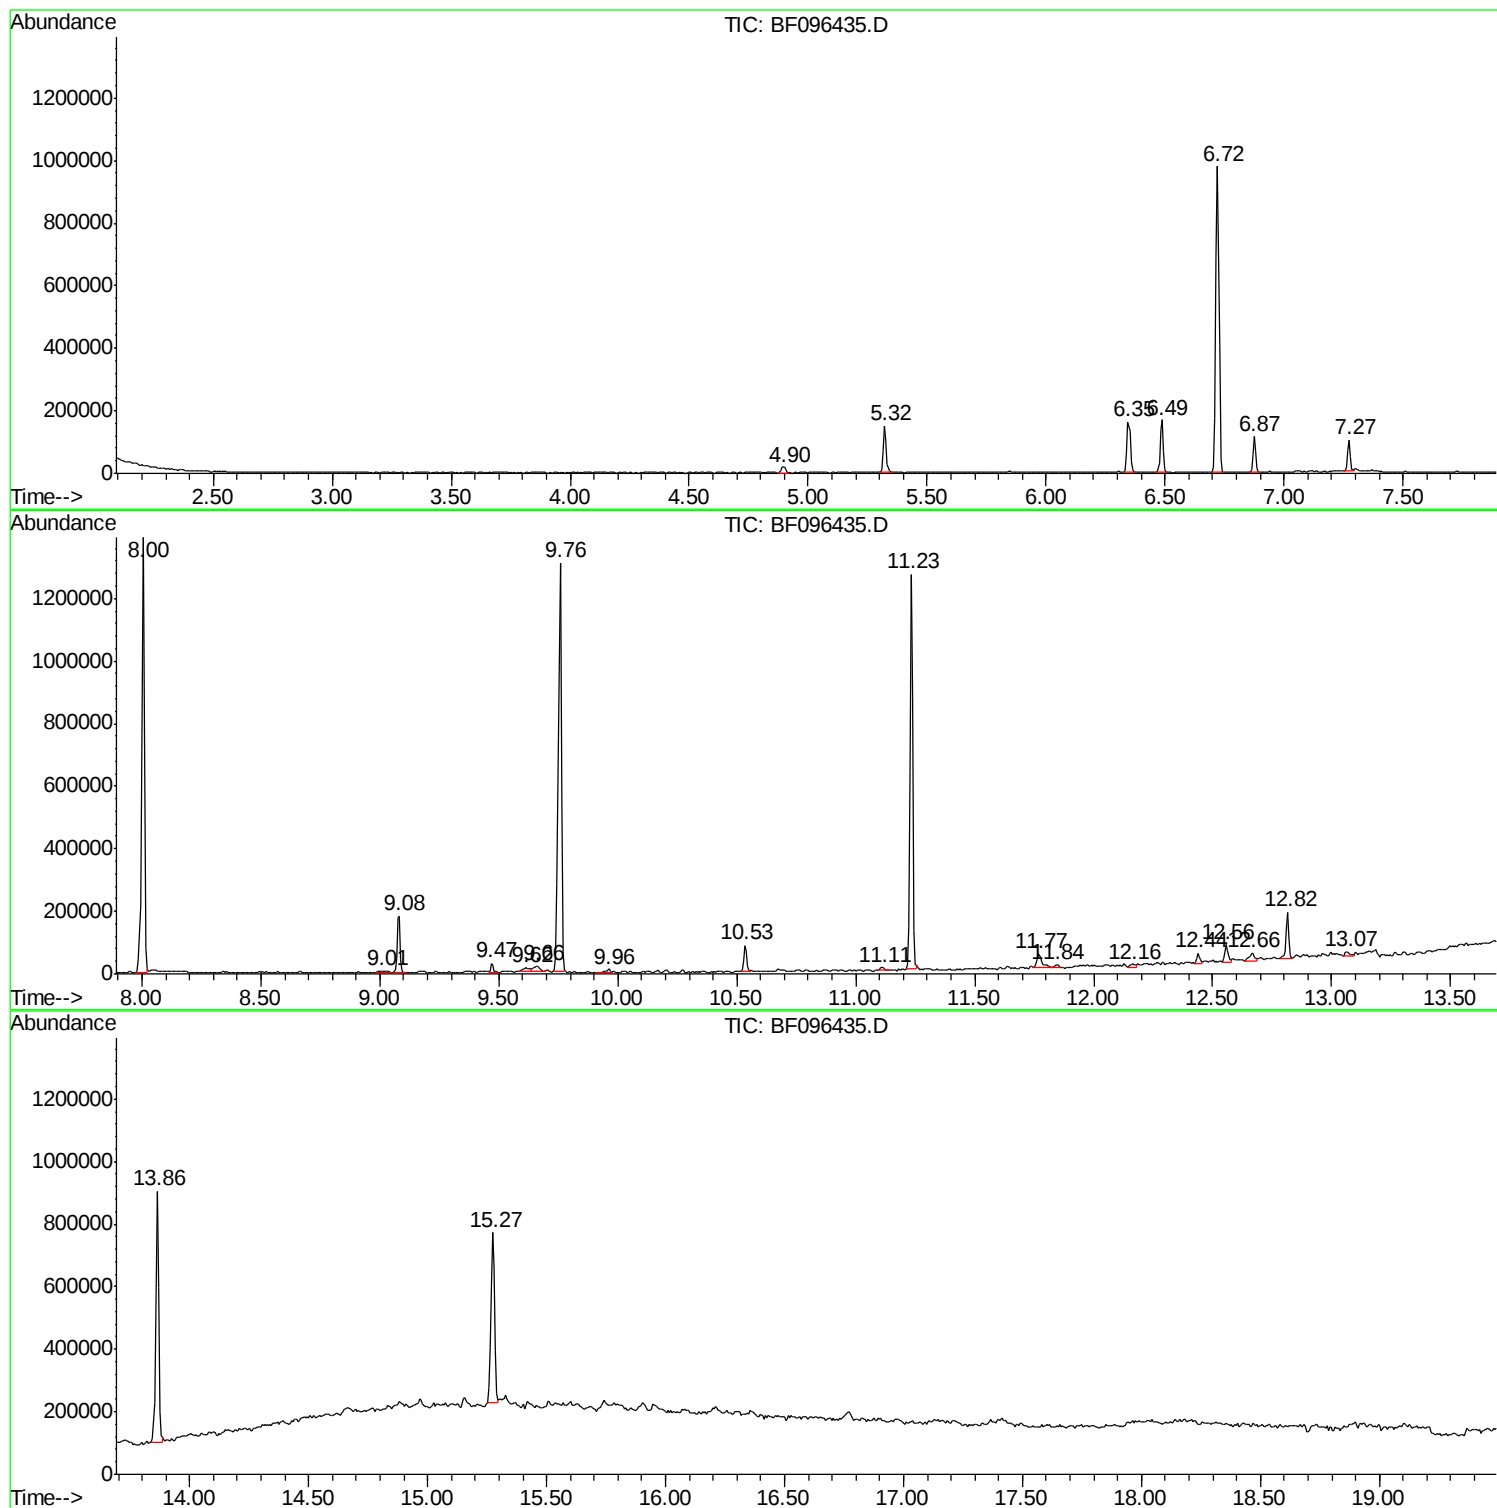

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070317\
Data File : BF096435.D
Acq On : 3 Jul 2017 12:28
Operator : SJ/MA
Sample : I3908-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-55-0-1.5










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.49 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.49	3.58 ng	145541	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	9
3		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		Xenon	132	Xe	007440-63-3	9

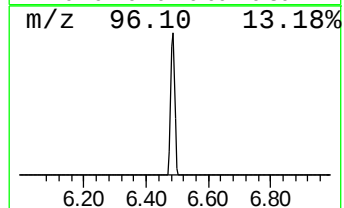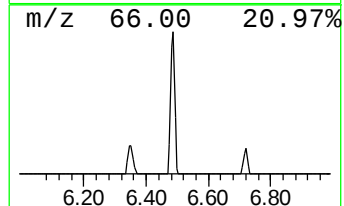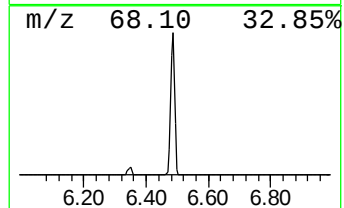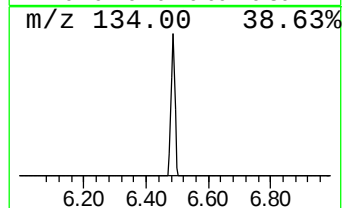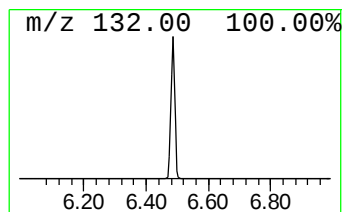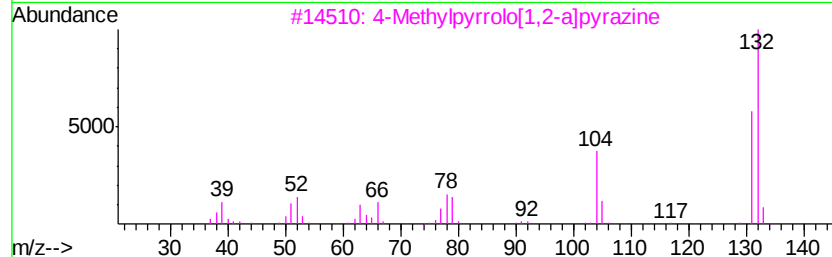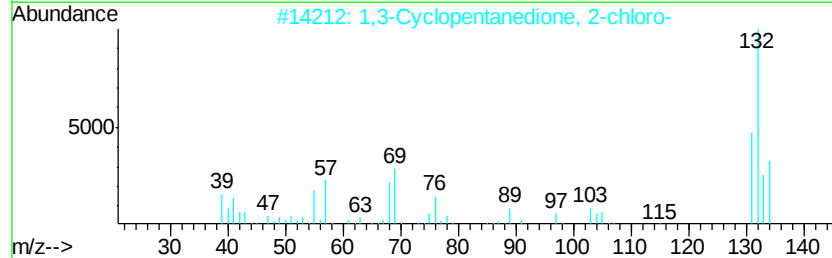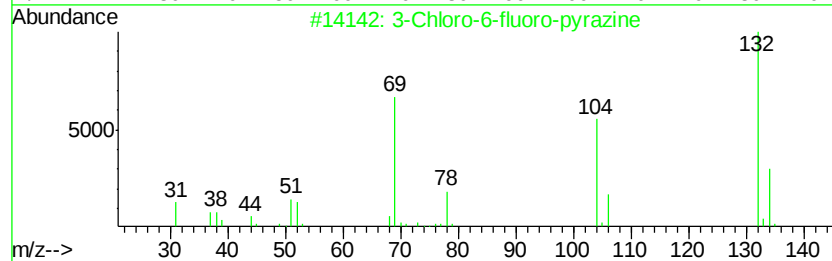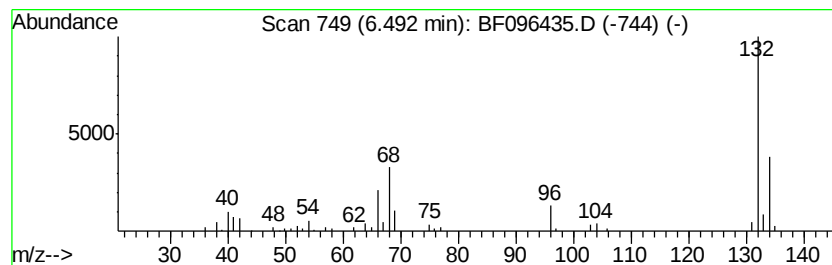

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070317\
Data File : BF096435.D
Acq On : 3 Jul 2017 12:28
Operator : SJ/MA
Sample : I3908-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-55-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.49	6.49	3.6	ng	145541	1	6.72	814004	20.0