


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070317\
 Data File : BF096430.D
 Acq On : 3 Jul 2017 10:01
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 01:43:12 2017

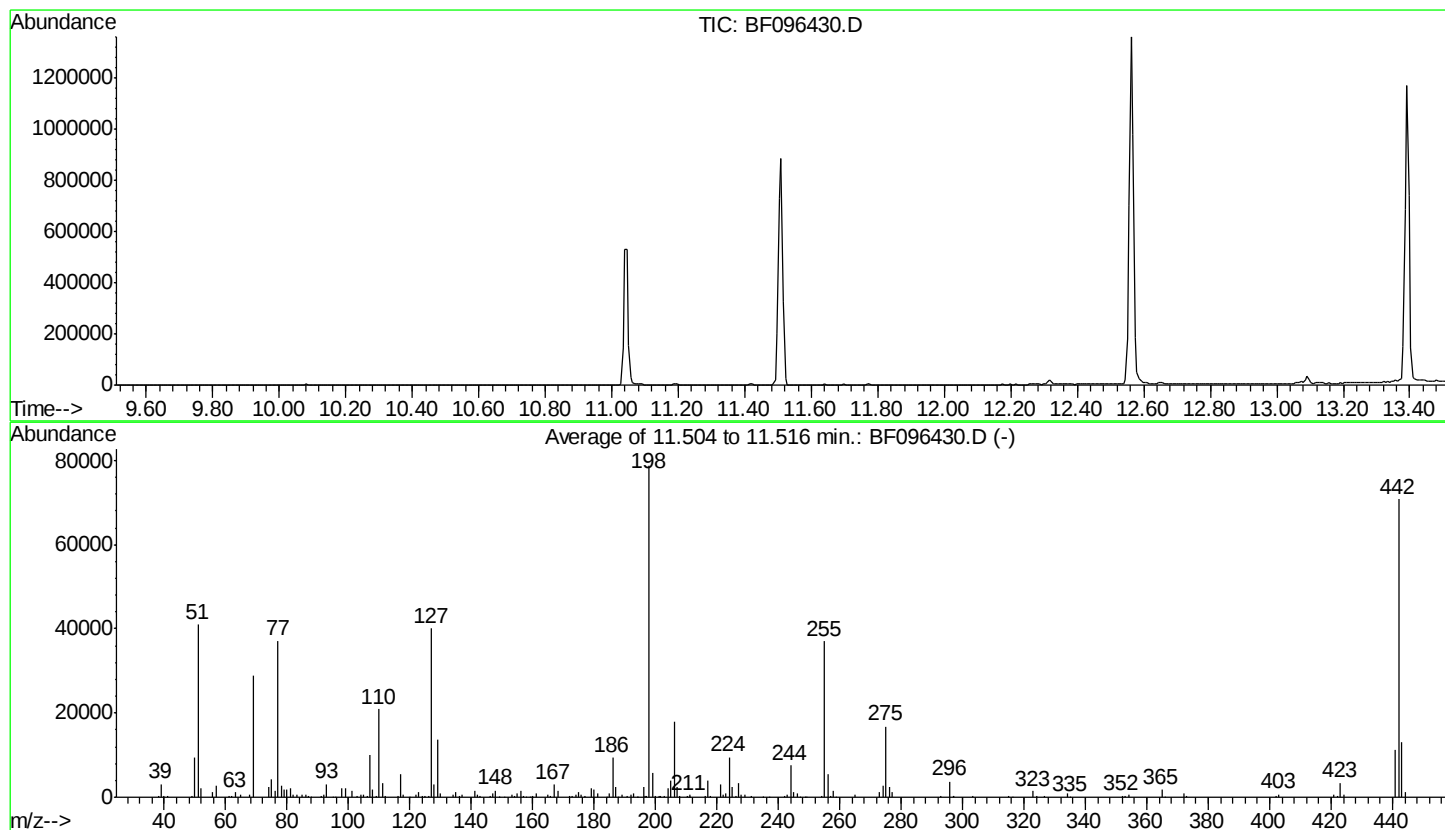

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.1	41011	PASS
68	69	0.00	2	1.8	508	PASS
69	198	0.00	100	36.7	28891	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	40088	PASS
197	198	0.00	2	0.5	362	PASS
198	198	100	100	100.0	78773	PASS
199	198	5	9	7.3	5714	PASS
275	198	10	60	21.4	16844	PASS
365	198	1	100	2.3	1787	PASS
441	442	0.01	24	16.0	11351	PASS
442	198	50	100	89.8	70752	PASS
443	442	15	24	18.3	12958	PASS