


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070317\
Data File : BF096455.D
Acq On : 3 Jul 2017 23:06
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 03 01:43:12 2017

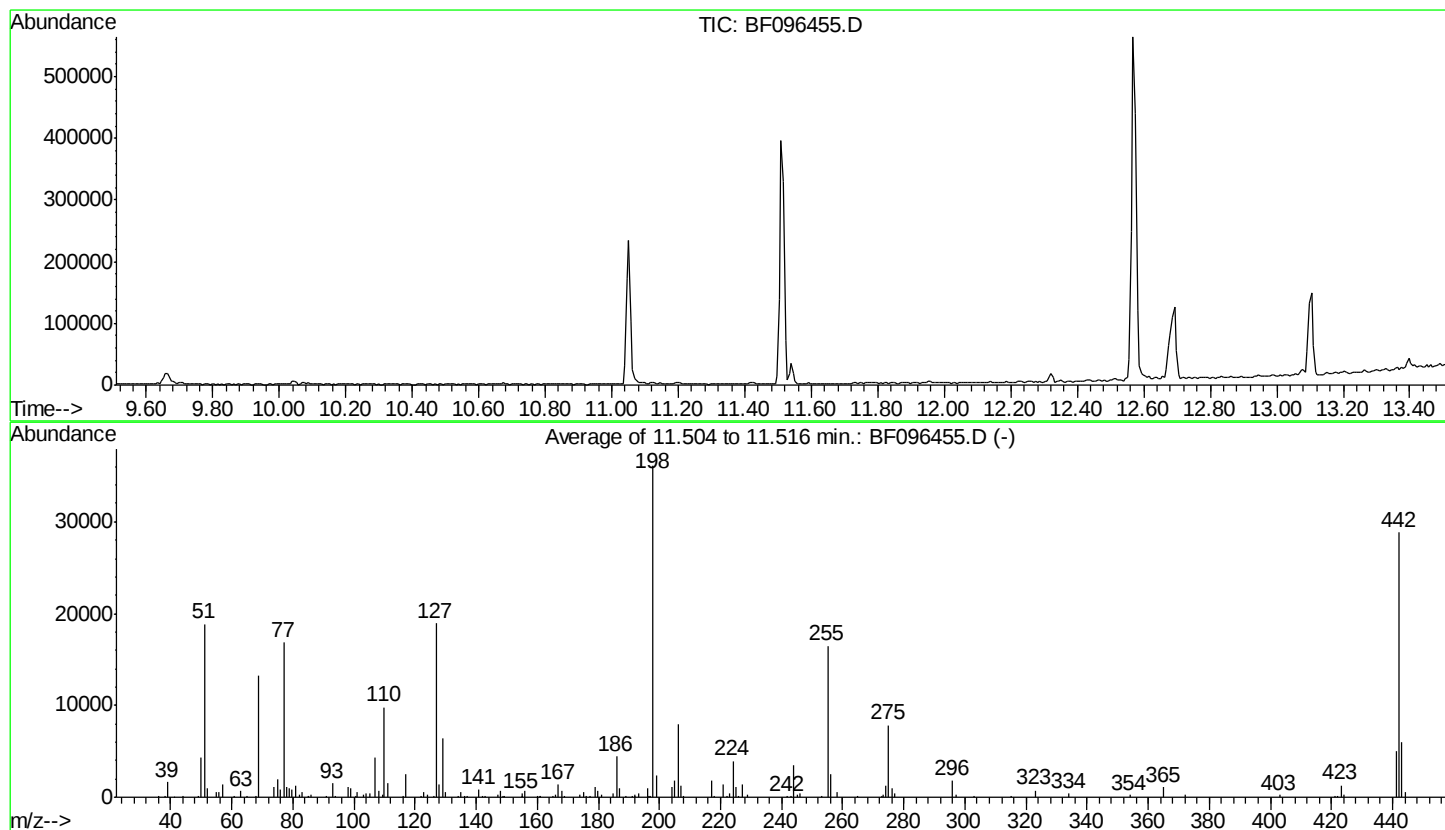

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	18892	PASS
68	69	0.00	2	0.8	100	PASS
69	198	0.00	100	36.8	13272	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	18897	PASS
197	198	0.00	2	0.4	134	PASS
198	198	100	100	100.0	36113	PASS
199	198	5	9	6.6	2401	PASS
275	198	10	60	21.7	7833	PASS
365	198	1	100	2.9	1056	PASS
441	442	0.01	24	17.3	4977	PASS
442	198	50	100	79.9	28839	PASS
443	442	15	24	20.6	5945	PASS