
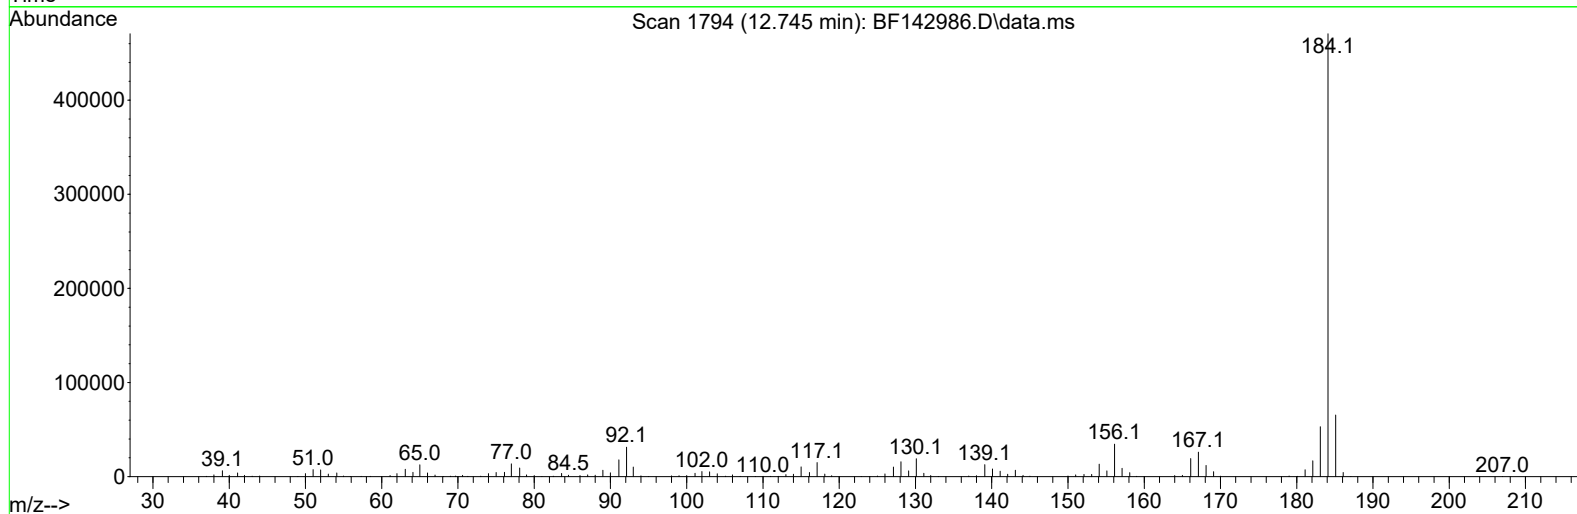


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070325\
Data File : BF142986.D
Acq On : 03 Jul 2025 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 11:16:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

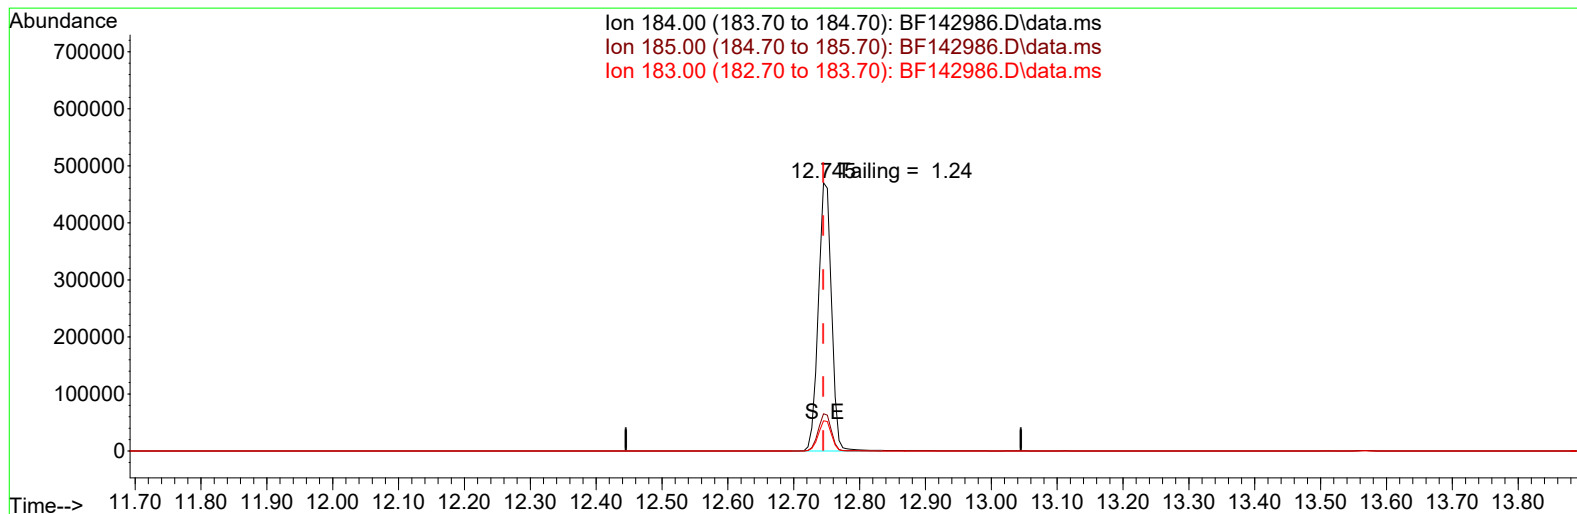

TIC: BF142986.D\data.ms

(77) Benzidine



12.745min (+ 0.000) 0.00 ng

response 654353

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.91
183.00	11.20	11.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070325\
Data File : BF142986.D
Acq On : 03 Jul 2025 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 11:16:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

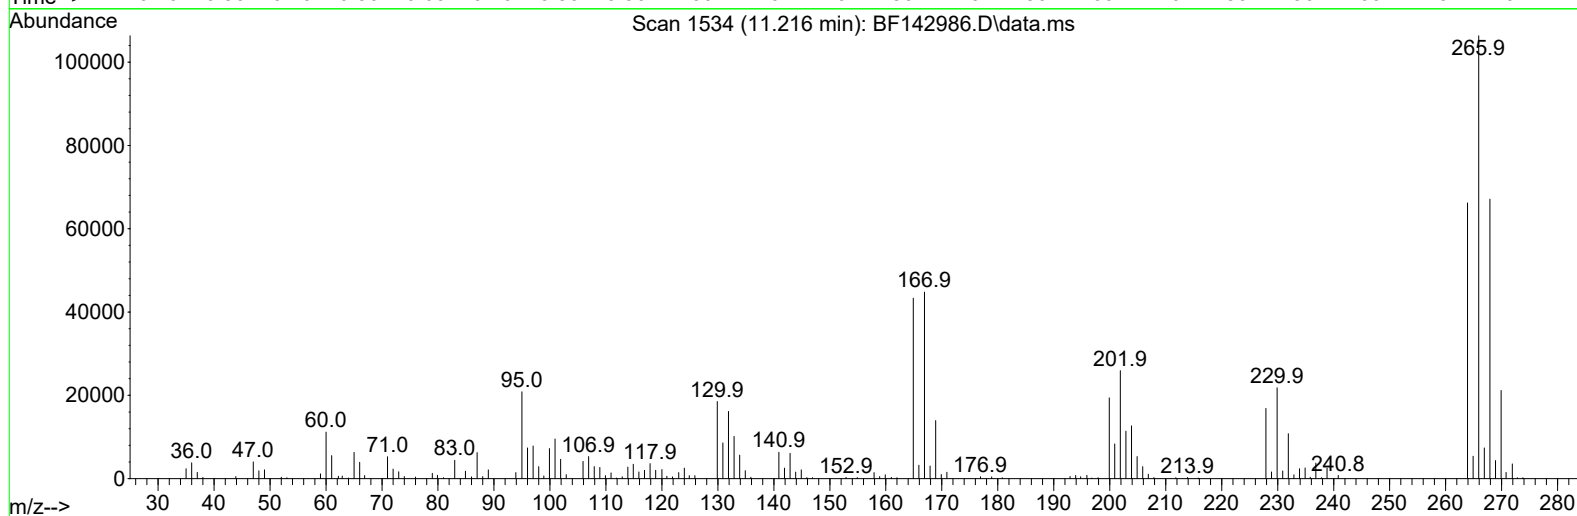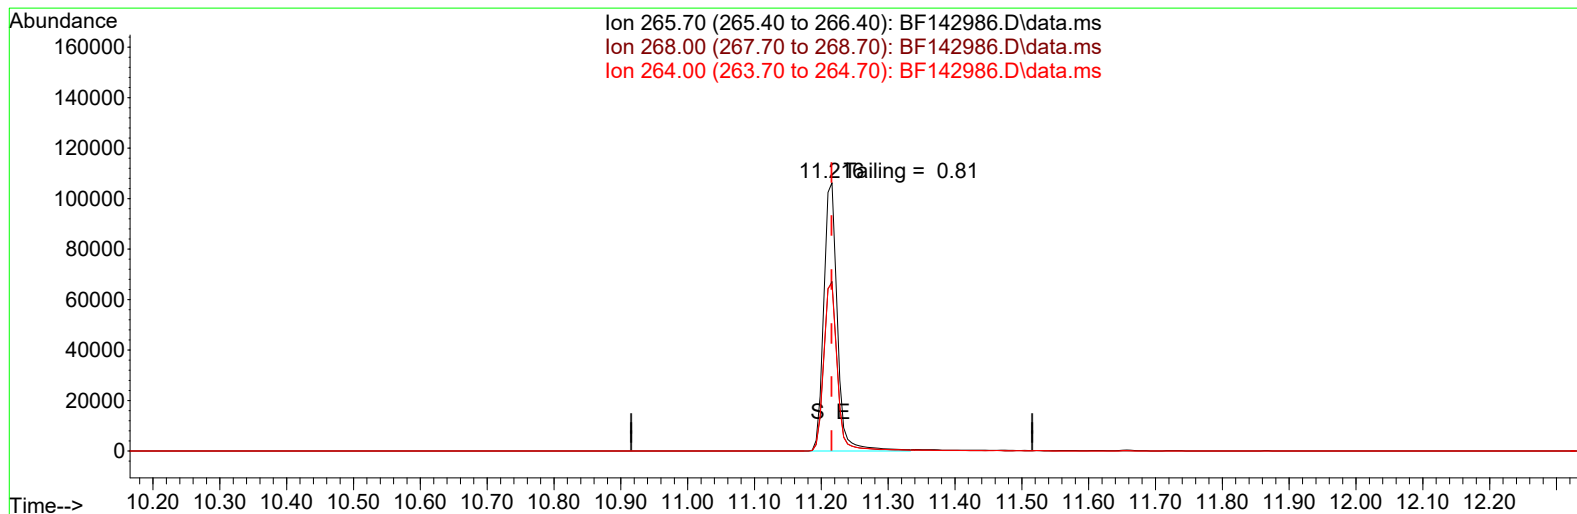

TIC: BF142986.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 44040.02 ng

response 150694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.11
264.00	62.40	62.24
0.00	0.00	0.00