

#57

Fluorene

Concen: 24.63 ng

RT: 10.35 min Scan# 767

Delta R.T. -0.01 min

Lab File: BF088701.D

Acq: 5 Jul 2016 14:17

Instrument :

BNA_F

ClientSampleId :


Tot Ion:166 Resp: 348945

Ion Ratio Lower Upper

166 100

165 98.8 77.8 116.8

167 14.0 11.2 16.8



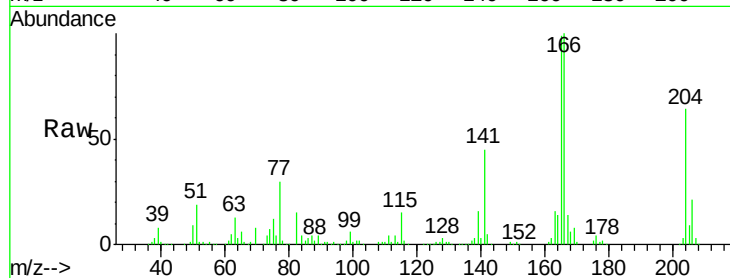


Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

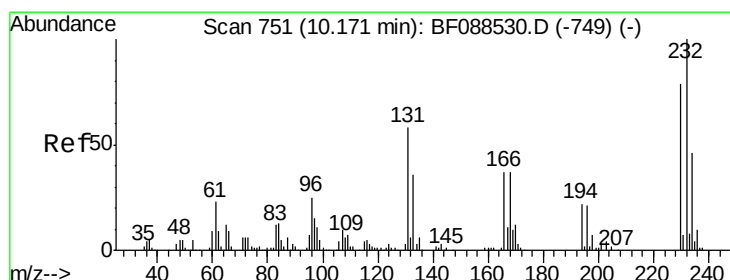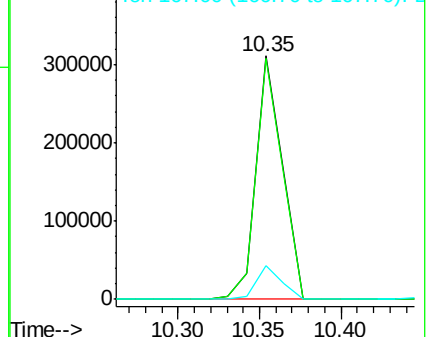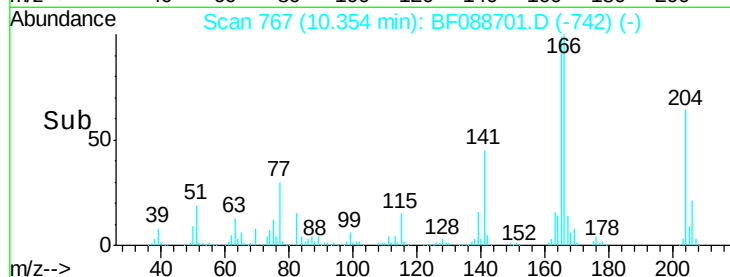

#58

2,3,4,6-Tetrachlorophenol

Concen: 33.09 ng

RT: 10.14 min Scan# 748

Delta R.T. 0.00 min

Lab File: BF088701.D

Acq: 5 Jul 2016 14:17

Tgt Ion:232 Resp: 107016


Ion Ratio Lower Upper

232 100

131 54.4 0.9 1.3#

130 2.6 1.5 2.3#

166 35.3 0.5 0.7#

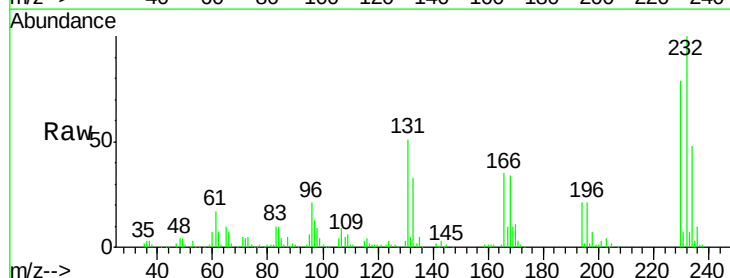

Abundance

Ion 232.00 (231.70 to 232.70): E

Ion 131.00 (130.70 to 131.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 166.00 (165.70 to 166.70): E

