

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070517\
 Data File : BF096474.D
 Acq On : 5 Jul 2017 10:45
 Operator : SJ/MA
 Sample : PB100369BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB100369BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.916	473	481	489	rBV	370500	584932	17.19%	2.018%
2	5.334	547	552	555	rBV	3128581	3208374	94.31%	11.071%
3	6.351	719	725	728	rBV	2813192	3192407	93.84%	11.016%
4	6.481	742	747	751	rBV	2921844	3130641	92.03%	10.803%
5	6.710	782	786	789	rBV	871401	691685	20.33%	2.387%
6	6.869	808	813	816	rBV	2639952	2357543	69.30%	8.135%
7	7.269	875	881	884	rBV	1793845	2026331	59.56%	6.992%
8	7.716	948	957	964	rBV	81361	146516	4.31%	0.506%
9	7.992	999	1004	1007	rBV	1097206	972308	28.58%	3.355%
10	9.075	1181	1188	1191	rBV	3280086	3401928	100.00%	11.739%
11	9.745	1297	1302	1306	rBV2	1164724	1049122	30.84%	3.620%
12	10.533	1430	1436	1440	rBV	1898672	2052790	60.34%	7.084%
13	11.227	1549	1554	1557	rBV	1203954	1045330	30.73%	3.607%
14	12.821	1818	1825	1828	rBV	2784802	3262386	95.90%	11.258%
15	13.857	1997	2001	2005	rBV	1111310	1013224	29.78%	3.496%
16	15.268	2235	2241	2246	rBV	697154	805936	23.69%	2.781%
17	16.192	2395	2398	2404	rVB6	21219	37383	1.10%	0.129%


Sum of corrected areas: 28978836

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070517\
Data File : BF096474.D
Acq On : 5 Jul 2017 10:45
Operator : SJ/MA
Sample : PB100369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100369BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

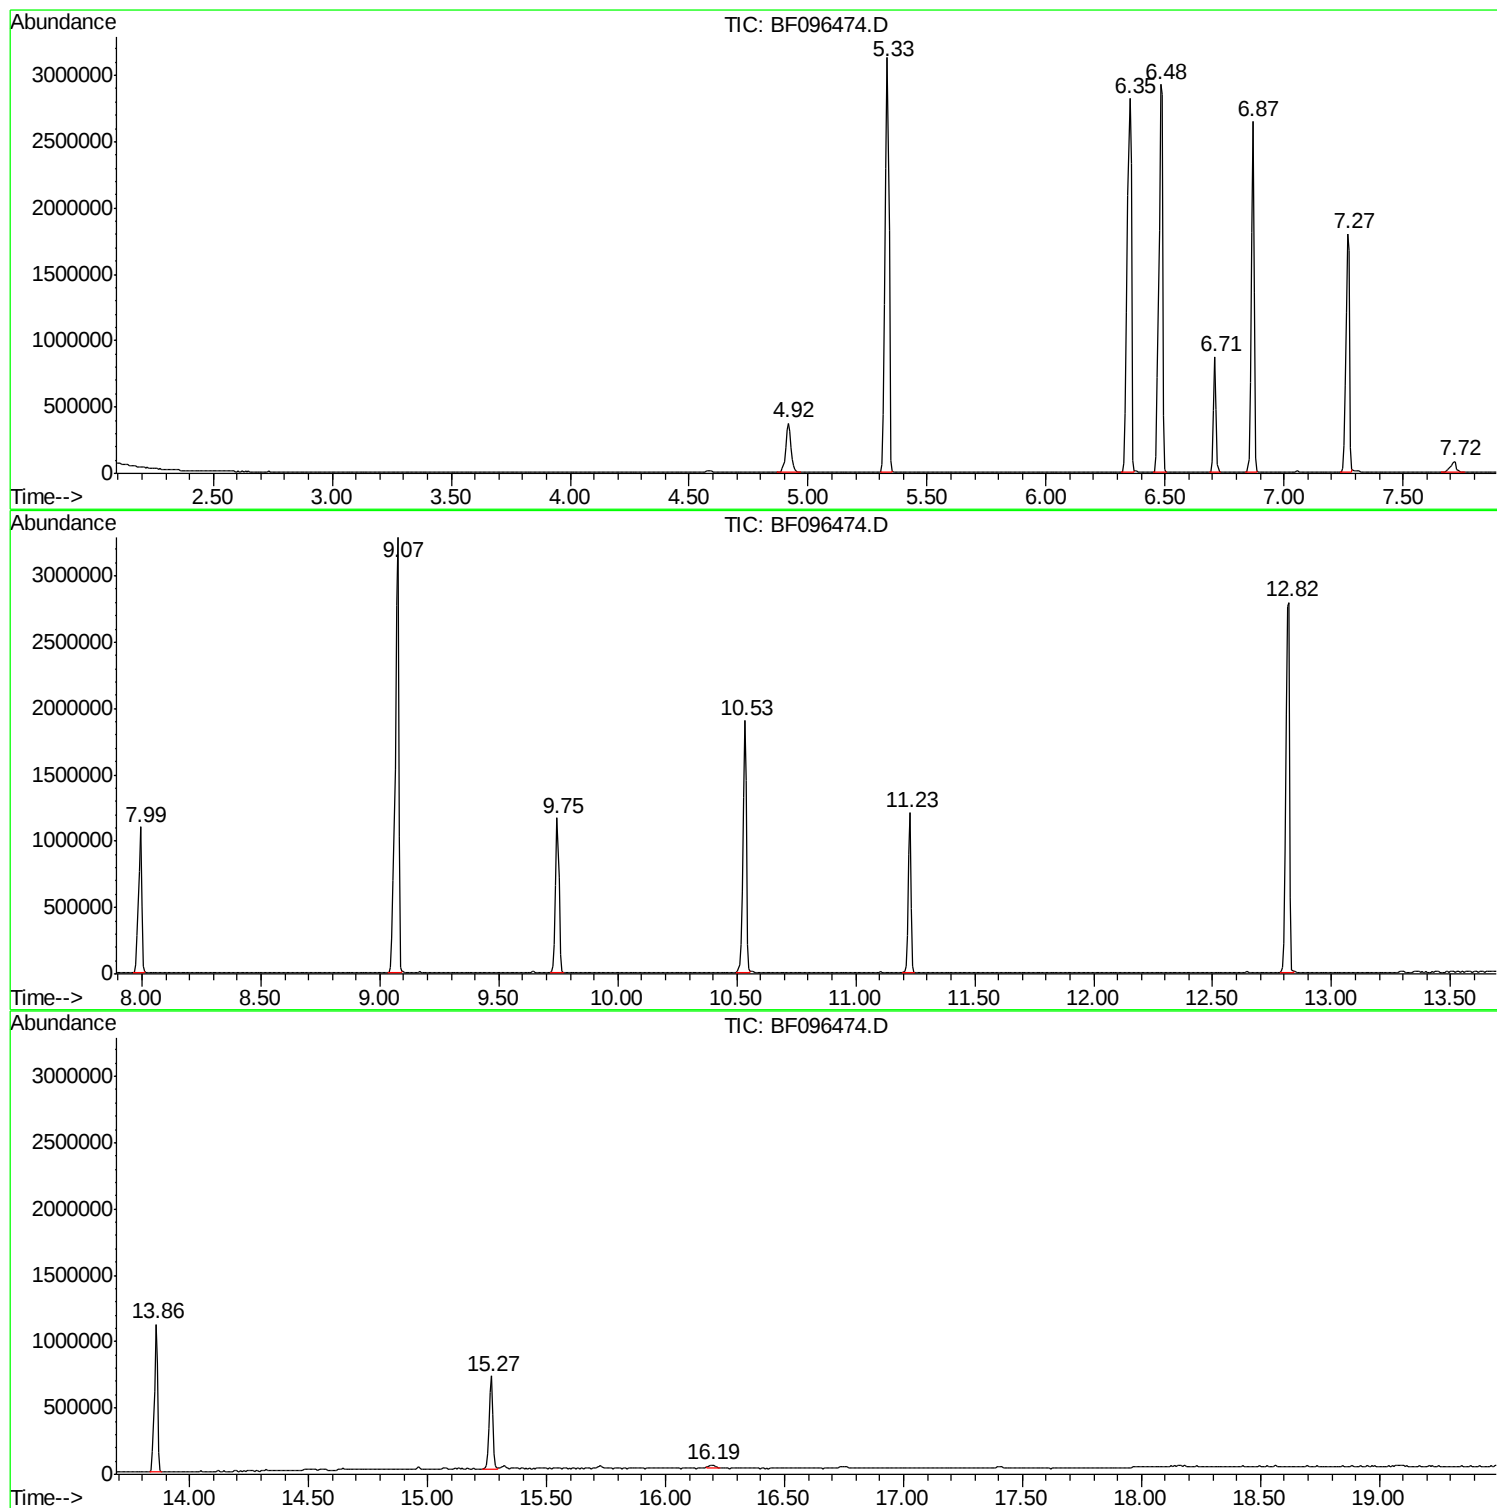

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070517\
Data File : BF096474.D
Acq On : 5 Jul 2017 10:45
Operator : SJ/MA
Sample : PB100369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100369BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown4.92 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.92	16.91 ng	584932	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38
2		Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
3		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4		3-Hexanol	102	C6H14O	000623-37-0	33
5		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25

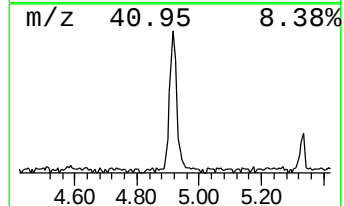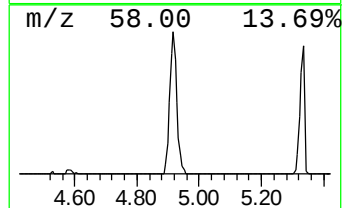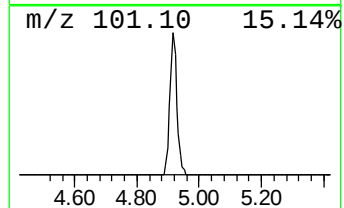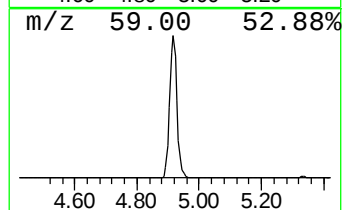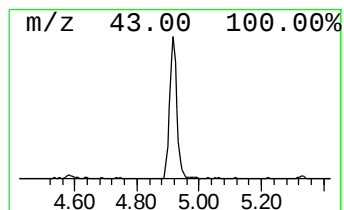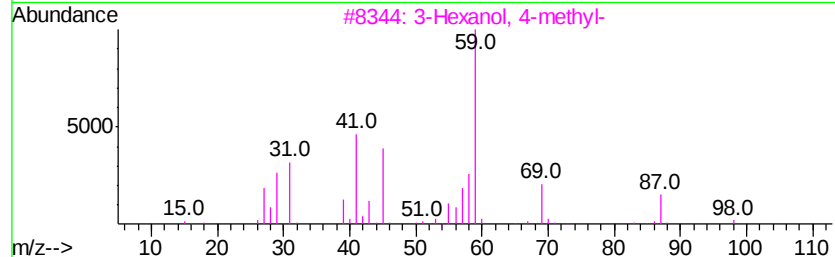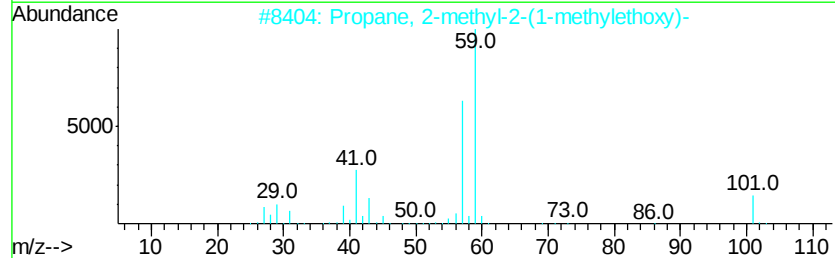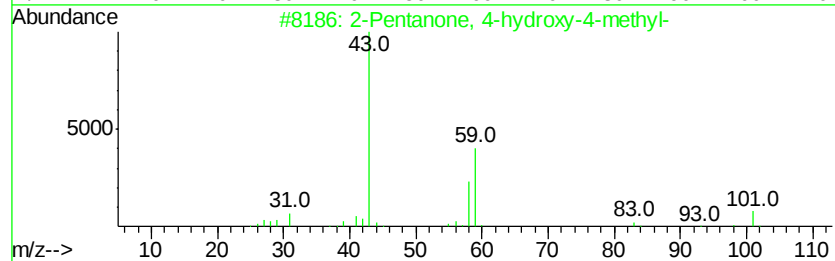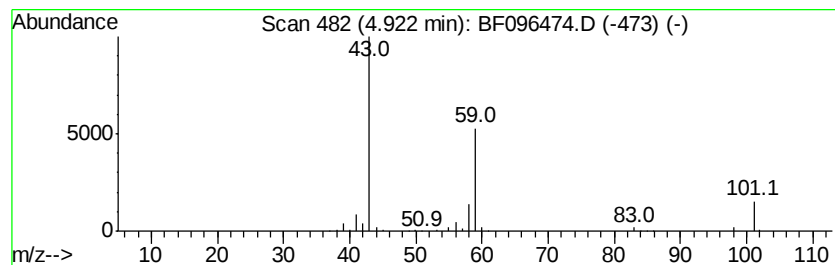

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070517\
Data File : BF096474.D
Acq On : 5 Jul 2017 10:45
Operator : SJ/MA
Sample : PB100369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100369BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	90.52 ng	3130640	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

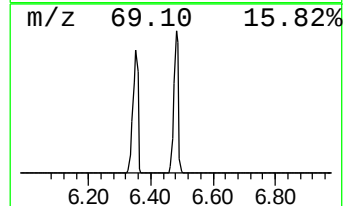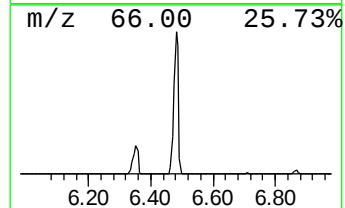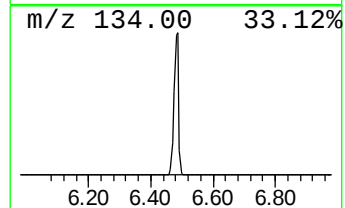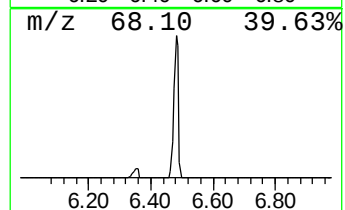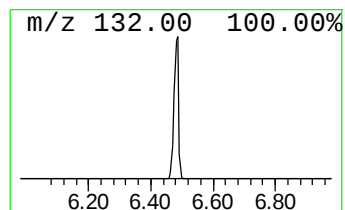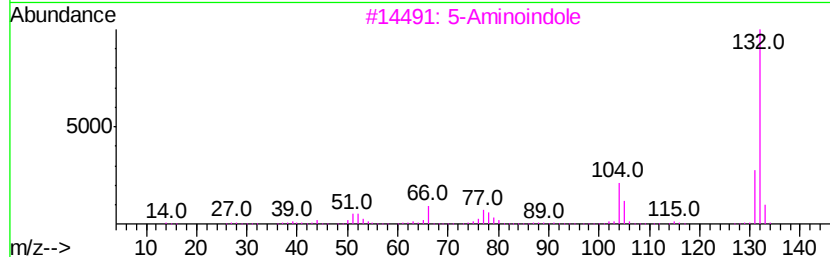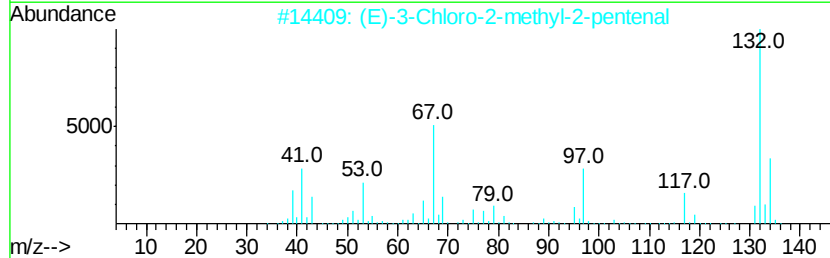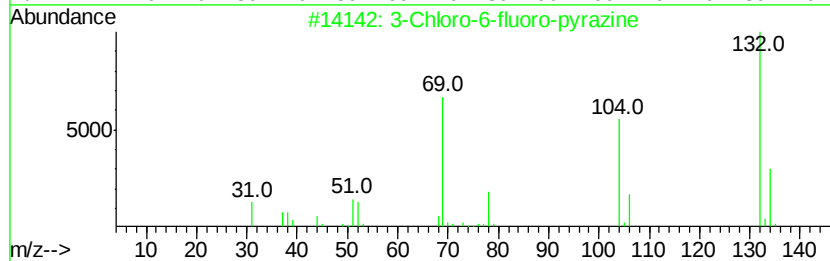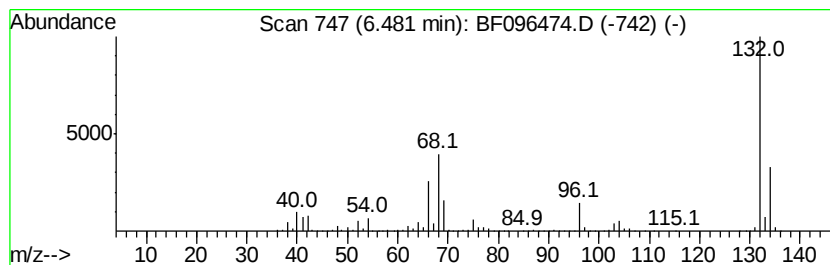

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070517\
Data File : BF096474.D
Acq On : 5 Jul 2017 10:45
Operator : SJ/MA
Sample : PB100369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB100369BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown4.92	4.92	16.9	ng	584932	1	6.71	691685	20.0
unknown6.48	6.48	90.5	ng	3130640	1	6.71	691685	20.0