

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070517\
 Data File : BF096482.D
 Acq On : 5 Jul 2017 14:26
 Operator : SJ/MA
 Sample : I3908-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-55-0-1.5RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.881	472	475	480	rBV	13477	16342	1.42%	0.253%
2	5.310	544	548	553	rBV	134882	115961	10.09%	1.798%
3	6.339	719	723	728	rBV	142798	131196	11.42%	2.034%
4	6.475	742	746	749	rBV	166754	129805	11.30%	2.012%
5	6.710	782	786	789	rBV	1054034	859555	74.82%	13.325%
6	6.863	809	812	816	rVB	110791	91088	7.93%	1.412%
7	7.263	877	880	884	rBV	86298	69122	6.02%	1.072%
8	7.992	1000	1004	1008	rBV	1422590	1148867	100.00%	17.810%
9	9.069	1184	1187	1190	rBV	183849	130077	11.32%	2.017%
10	9.463	1251	1254	1257	rBV	22101	16862	1.47%	0.261%
11	9.645	1276	1285	1287	rBV4	8626	17173	1.49%	0.266%
12	9.745	1298	1302	1306	rBV2	1229179	1102388	95.95%	17.090%
13	10.527	1432	1435	1439	rBV	67882	56071	4.88%	0.869%
14	11.227	1550	1554	1557	rBV	1086800	909745	79.19%	14.103%
15	12.433	1756	1759	1762	rVB	24424	17187	1.50%	0.266%
16	12.645	1792	1795	1803	rBV2	76826	86291	7.51%	1.338%
17	12.721	1806	1808	1812	rVB4	17290	15644	1.36%	0.243%
18	12.810	1819	1823	1826	rBV	114707	101201	8.81%	1.569%
19	13.351	1912	1915	1918	rBV	44962	42872	3.73%	0.665%
20	13.857	1997	2001	2005	rBV	848927	779565	67.86%	12.085%
21	15.268	2236	2241	2245	rBV	521009	613518	53.40%	9.511%


Sum of corrected areas: 6450530

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070517\
Data File : BF096482.D
Acq On : 5 Jul 2017 14:26
Operator : SJ/MA
Sample : I3908-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-55-0-1.5RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

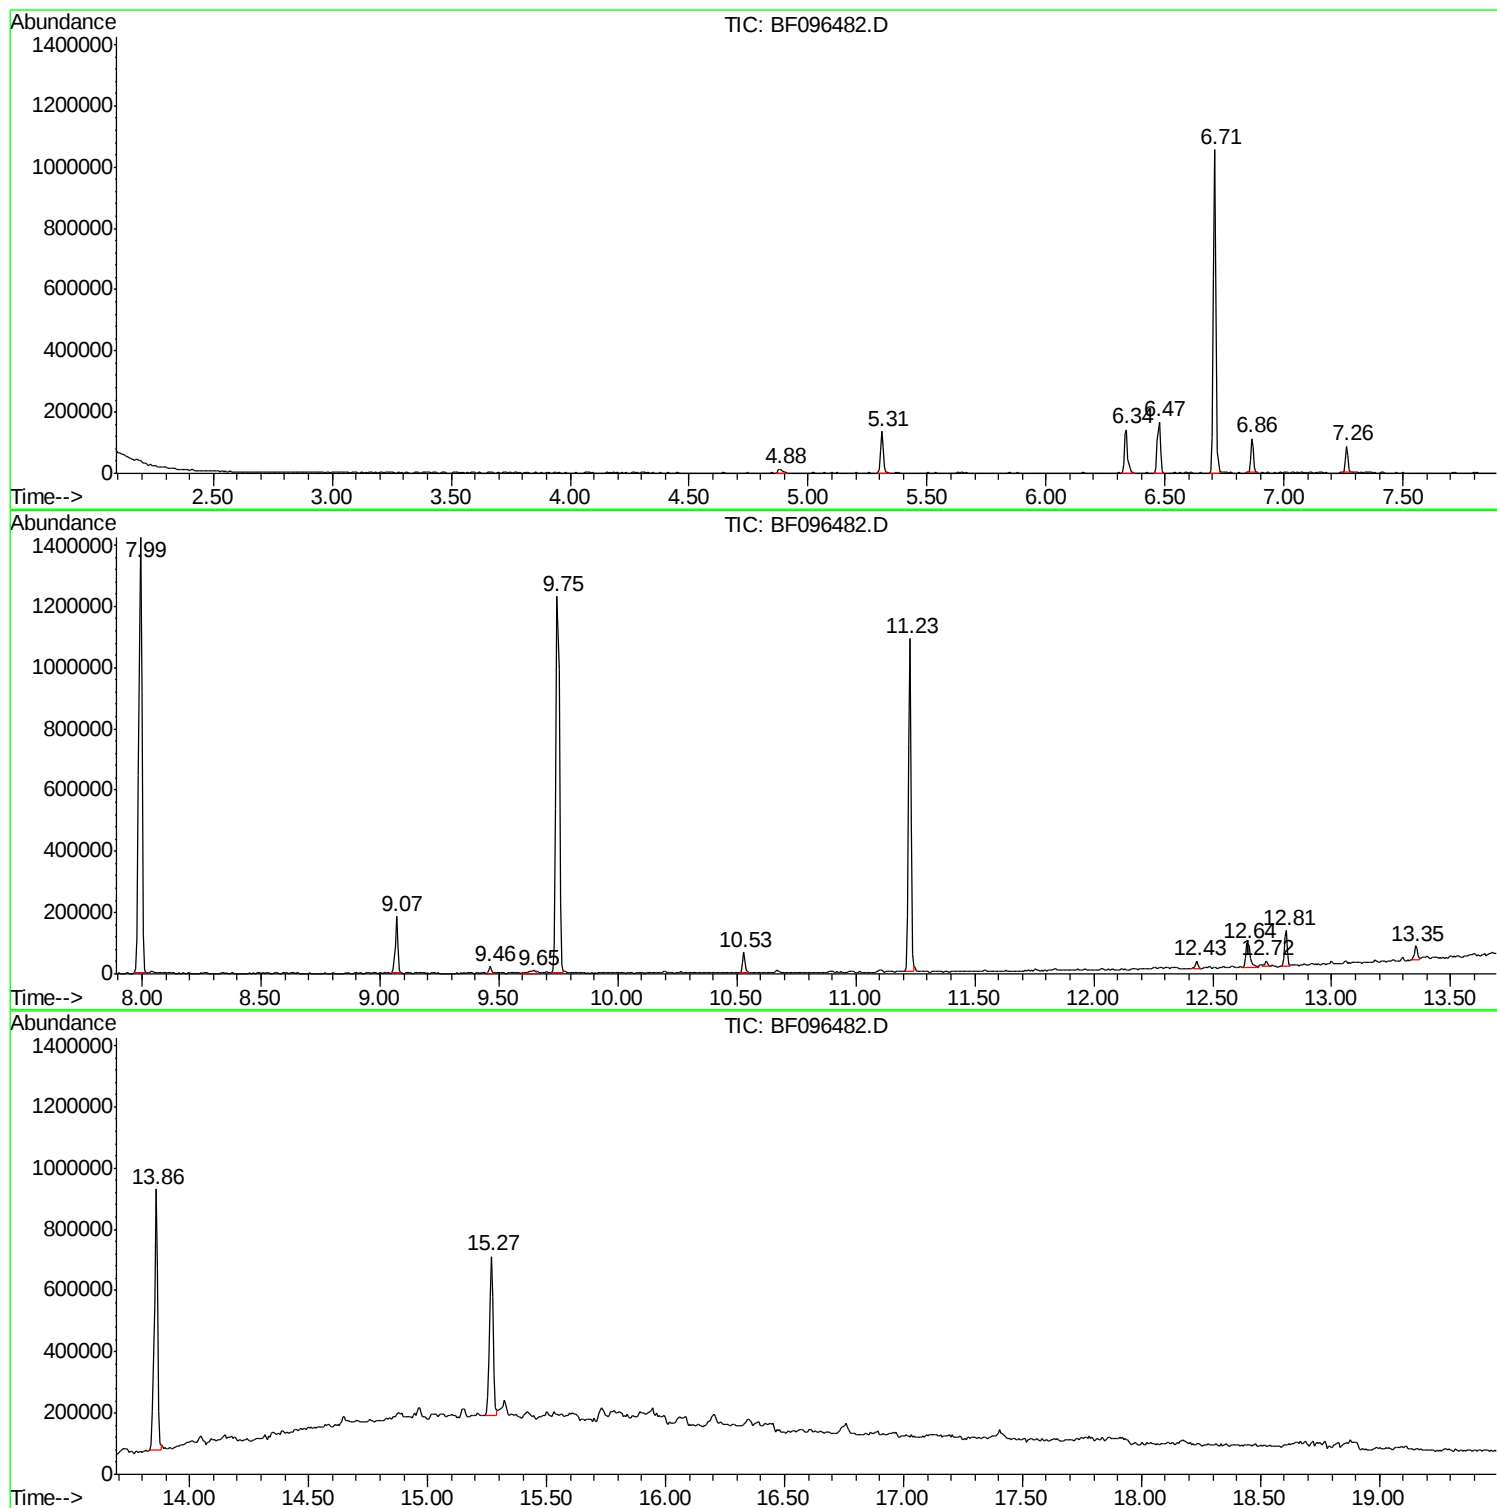

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF070517\
Data_File : BF096482.D
Acq_On : 5_Jul_2017. 14:266
Operator : SJ/MAA
Sample : I3908-01REE
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-55-0-1.5RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
