


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070517\
 Data File : BF096471.D
 Acq On : 5 Jul 2017 9:19
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 05 13:27:10 2017

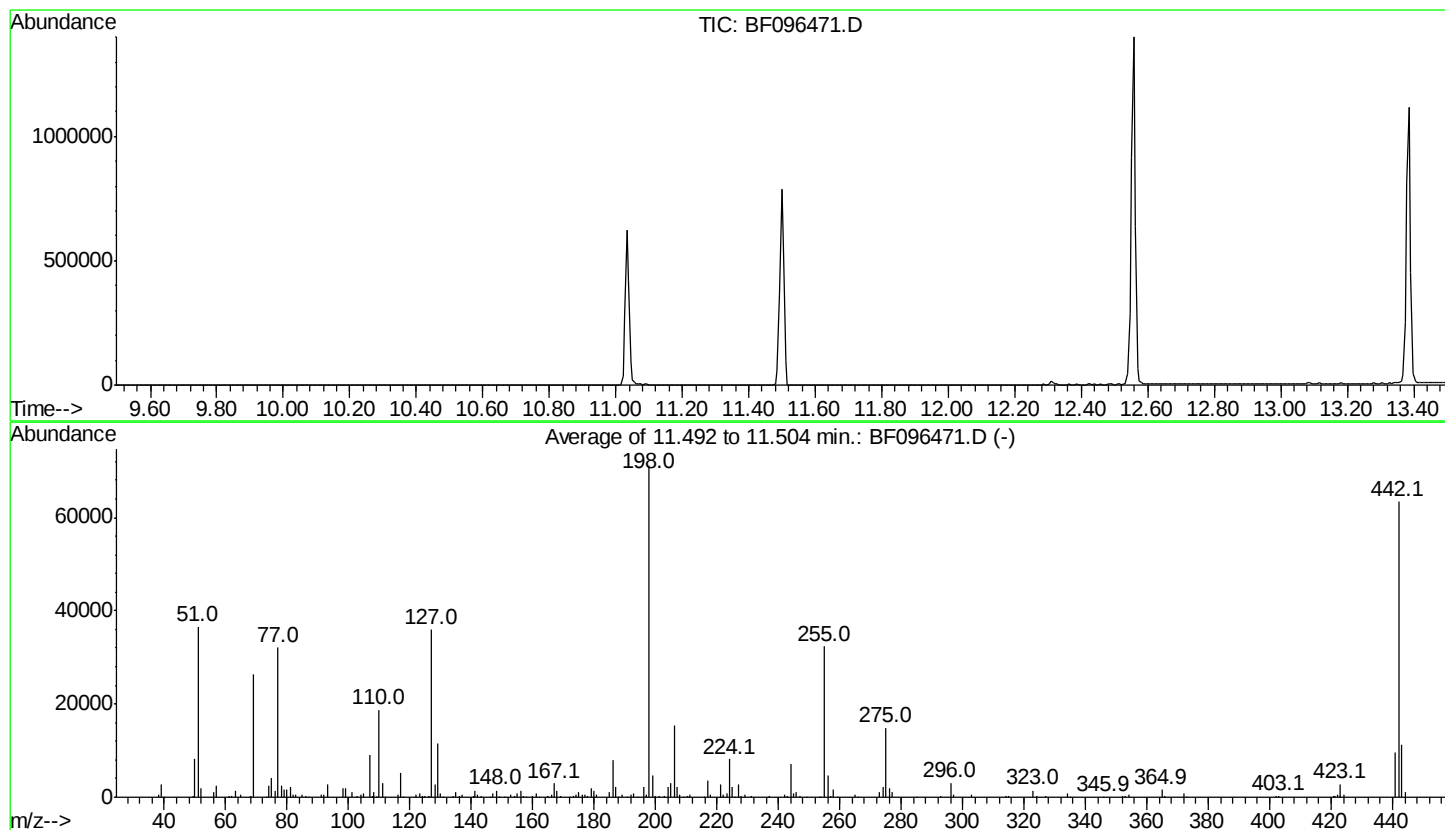

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	36658	PASS
68	69	0.00	2	1.3	346	PASS
69	198	0.00	100	37.1	26362	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	35954	PASS
197	198	0.00	2	0.6	461	PASS
198	198	100	100	100.0	71133	PASS
199	198	5	9	6.5	4637	PASS
275	198	10	60	21.1	14974	PASS
365	198	1	100	2.3	1607	PASS
441	442	0.01	24	15.4	9741	PASS
442	198	50	100	89.0	63320	PASS
443	442	15	24	17.9	11331	PASS