


Data Path : Z:\HPCHEM1\BNA F\Data\BF070517\
 Data File : BF096497.D
 Acq On : 5 Jul 2017 21:50
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 05 13:27:10 2017

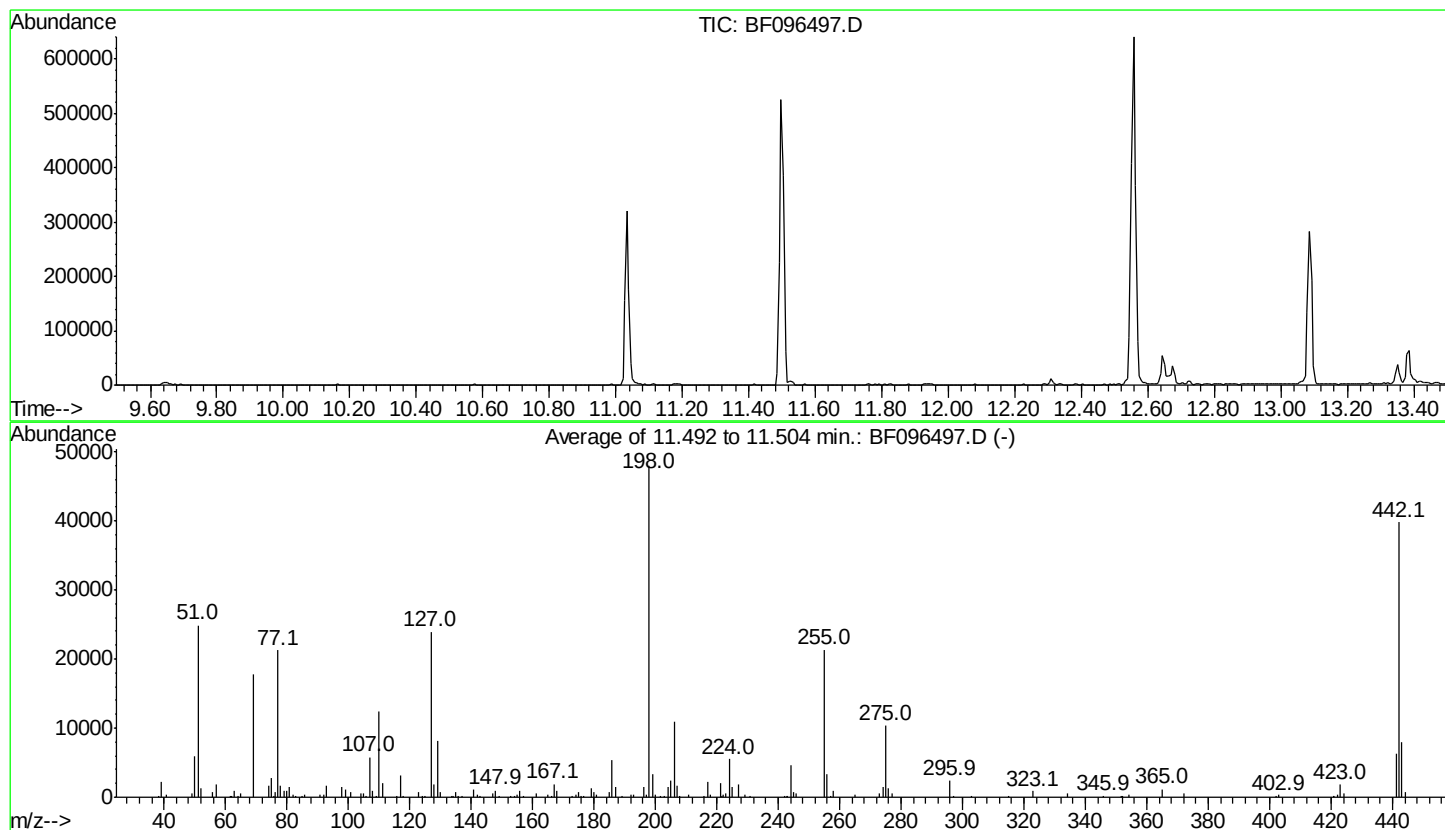

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	24885	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.1	17776	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	23957	PASS
197	198	0.00	2	0.8	392	PASS
198	198	100	100	100.0	47968	PASS
199	198	5	9	6.9	3290	PASS
275	198	10	60	21.5	10308	PASS
365	198	1	100	2.4	1152	PASS
441	442	0.01	24	16.0	6350	PASS
442	198	50	100	83.0	39791	PASS
443	442	15	24	20.0	7941	PASS