

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070518\
 Data File : BF107151.D
 Acq On : 6 Jul 2018 4:37
 Operator : JU/SJ
 Sample : J3805-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062818-TIPC-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.178	479	483	491	rBV	24044	28653	1.76%	0.292%
2	5.590	549	553	569	rBV	430828	467197	28.66%	4.754%
3	6.590	720	723	738	rBV	307675	326889	20.05%	3.326%
4	6.725	742	746	755	rBV	899533	830055	50.91%	8.445%
5	6.943	780	783	787	rBV	403841	354381	21.74%	3.606%
6	7.101	806	810	814	rBV	1266685	1178821	72.30%	11.994%
7	7.513	875	880	883	rBV	932324	918067	56.31%	9.341%
8	8.231	997	1002	1016	rBV	453961	438073	26.87%	4.457%
9	8.572	1050	1060	1066	rBV5	6931	19252	1.18%	0.196%
10	9.301	1179	1184	1187	rBV	1714155	1630361	100.00%	16.588%
11	9.695	1248	1251	1260	rVB	58190	51753	3.17%	0.527%
12	9.989	1297	1301	1311	rVB	487490	445434	27.32%	4.532%
13	10.395	1367	1370	1373	rVB	19480	16374	1.00%	0.167%
14	10.648	1410	1413	1418	rVB	33238	30680	1.88%	0.312%
15	10.783	1432	1436	1445	rBV	604878	556697	34.15%	5.664%
16	10.866	1447	1450	1456	rVB	22981	21432	1.31%	0.218%
17	11.483	1551	1555	1562	rBV	414164	378493	23.22%	3.851%
18	13.066	1819	1824	1827	rBV	1530047	1364303	83.68%	13.881%
19	13.960	1970	1976	1984	rBV4	9302	17534	1.08%	0.178%
20	14.136	2002	2006	2012	rBV	422840	398332	24.43%	4.053%
21	14.877	2129	2132	2135	rBV	17546	16365	1.00%	0.167%
22	15.230	2188	2192	2196	rVB	19596	21671	1.33%	0.220%
23	15.624	2255	2259	2262	rBV2	18304	22606	1.39%	0.230%
24	15.666	2262	2266	2273	rVB	205533	272078	16.69%	2.768%
25	16.083	2333	2337	2341	rVB	16024	22971	1.41%	0.234%


Sum of corrected areas: 9828472

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070518\
Data File : BF107151.D
Acq On : 6 Jul 2018 4:37
Operator : JU/SJ
Sample : J3805-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062818-TIPC-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

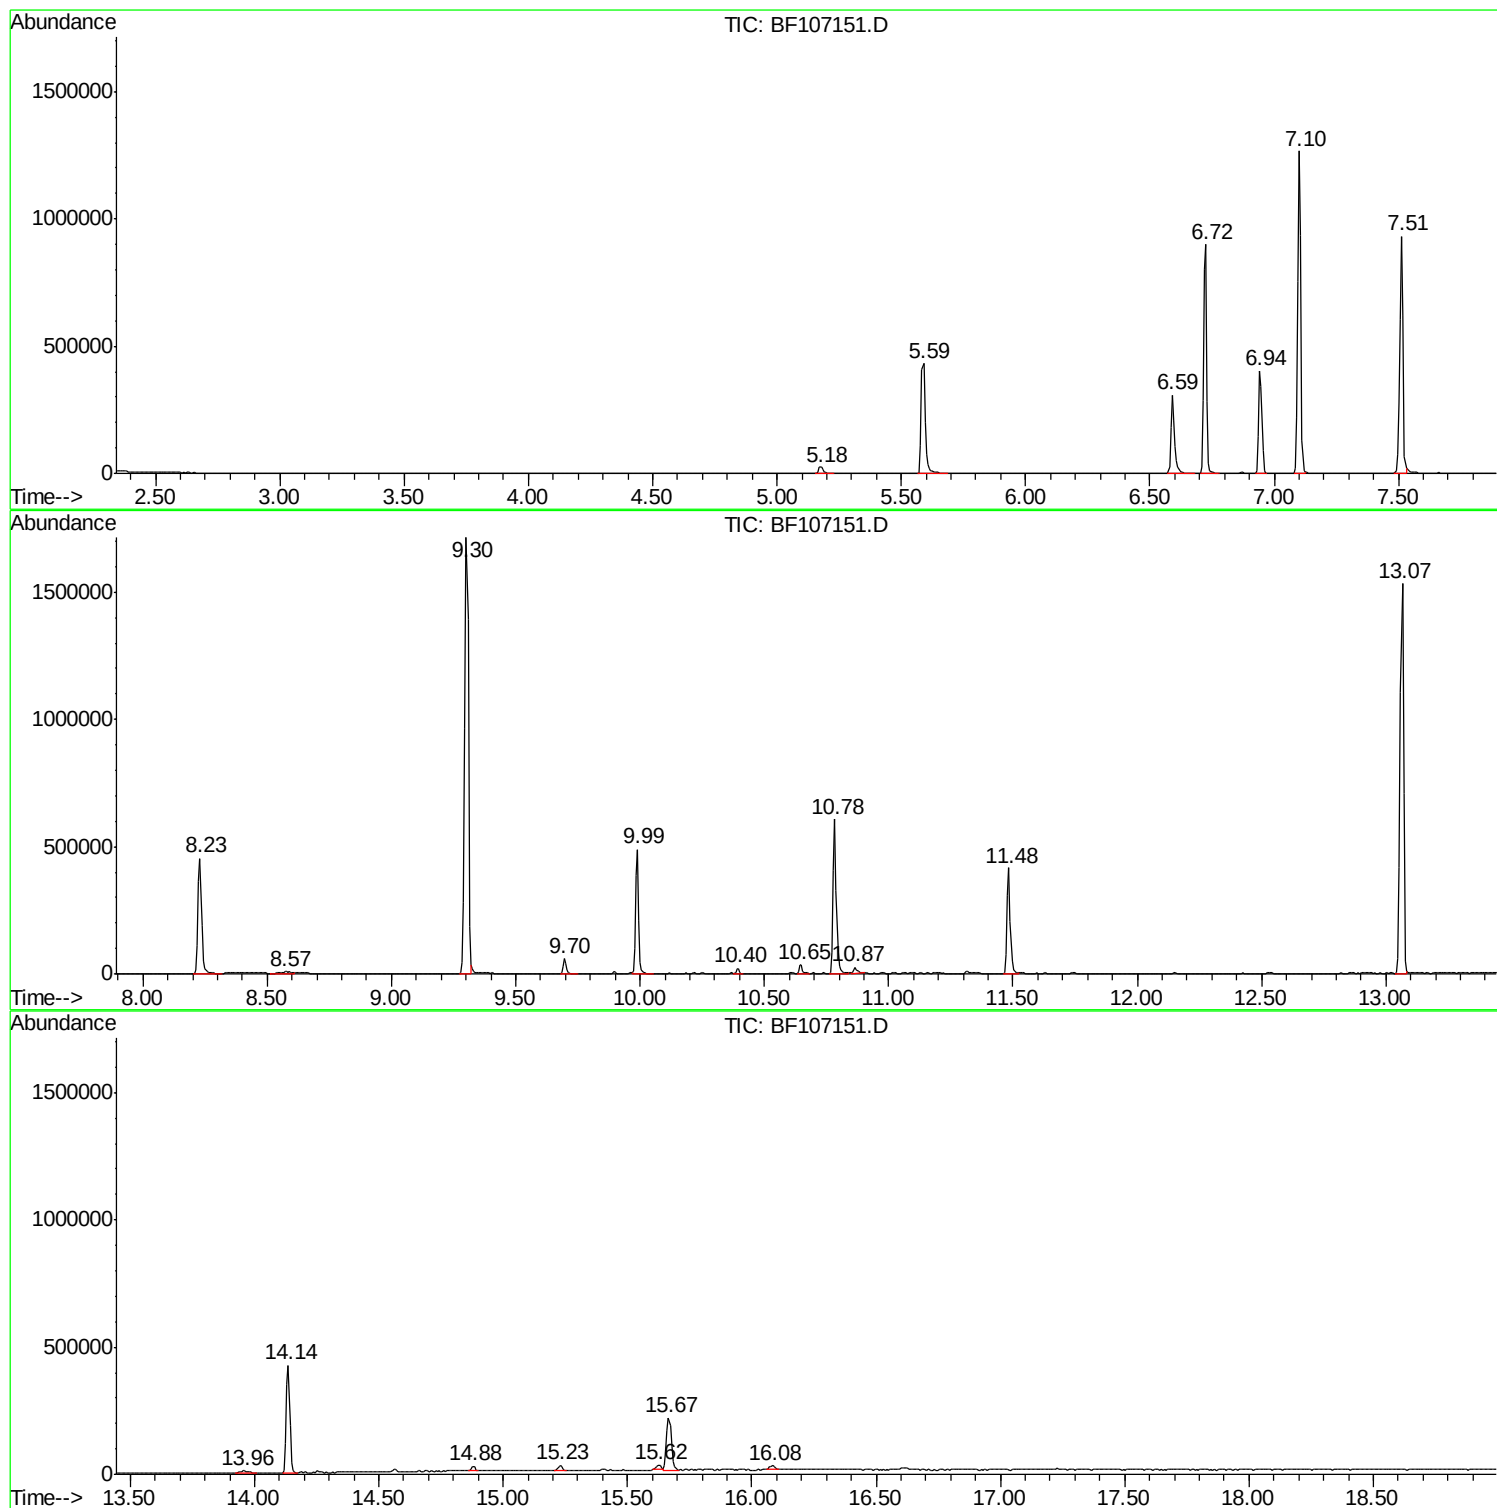

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070518\
Data File : BF107151.D
Acq On : 6 Jul 2018 4:37
Operator : JU/SJ
Sample : J3805-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062818-TIPC-F-U-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.72 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.72	46.85 ng	830055	1,4-Dichlorobenzene-d4	6.94

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

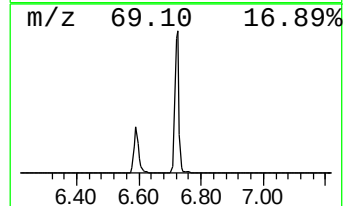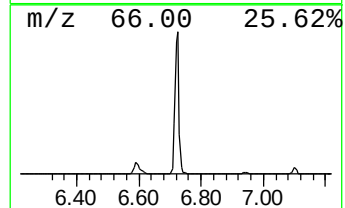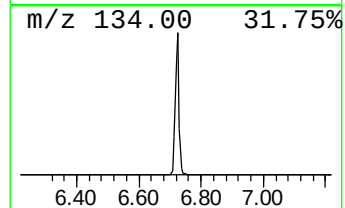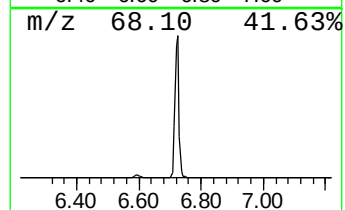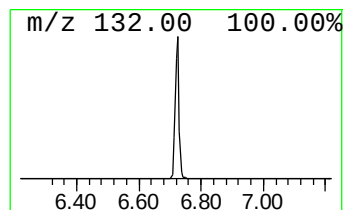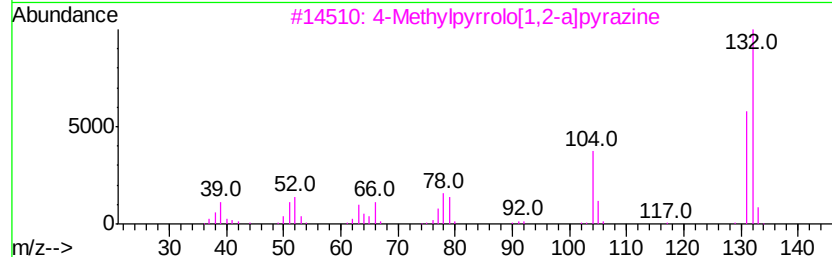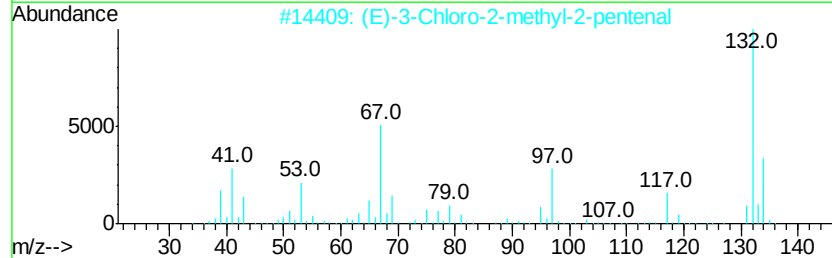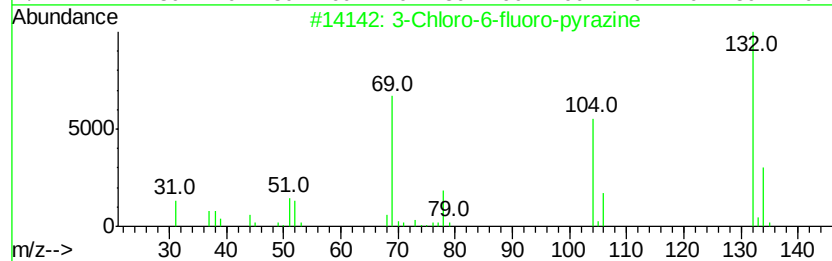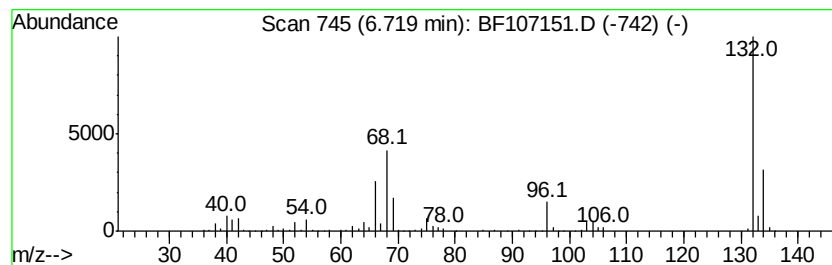

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070518\
Data File : BF107151.D
Acq On : 6 Jul 2018 4:37
Operator : JU/SJ
Sample : J3805-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062818-TIPC-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.72	6.72	46.9	ng	830055	1	6.94	354381	20.0