


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070518\
 Data File : BF107115.D
 Acq On : 5 Jul 2018 9:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

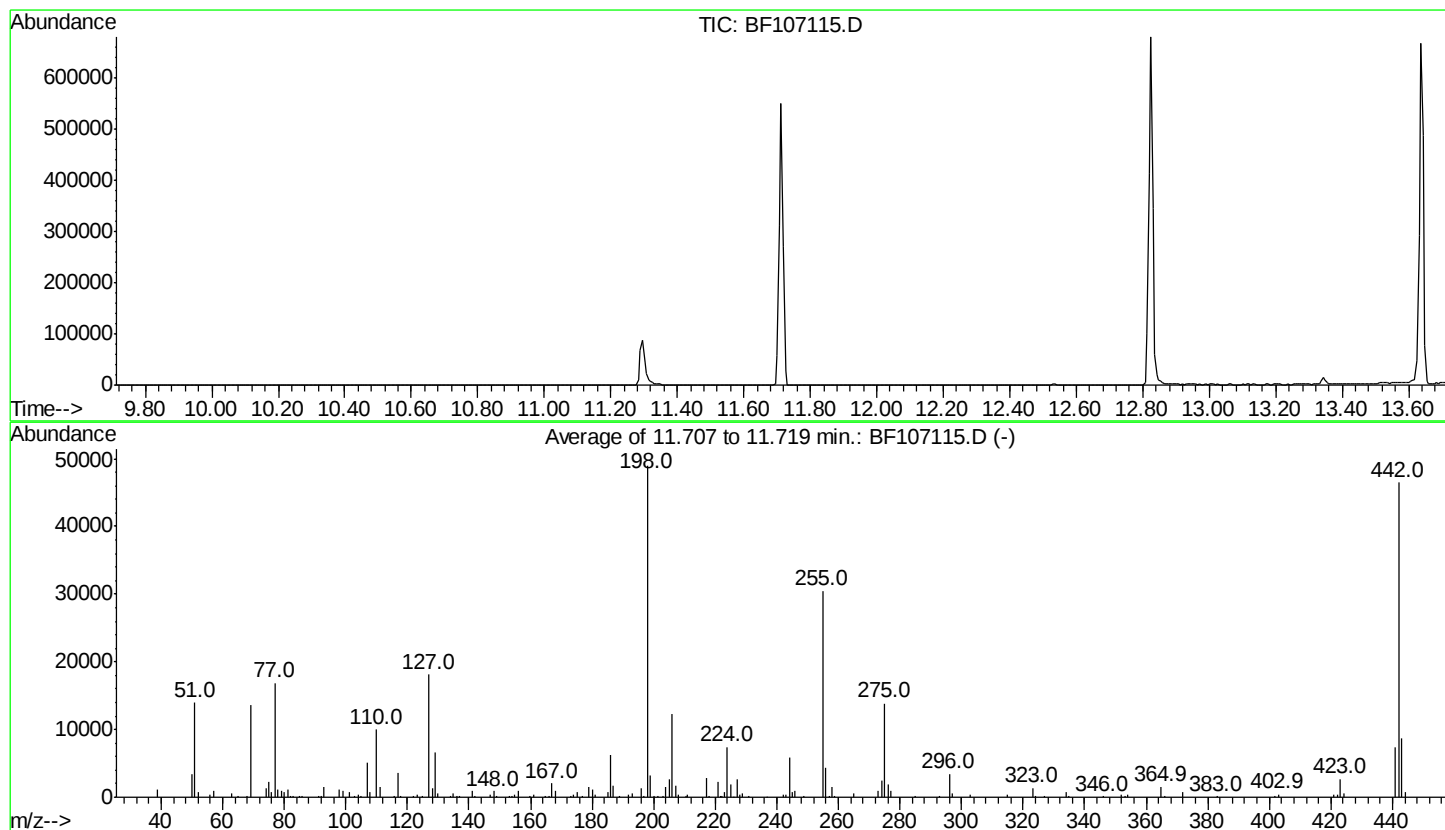

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	13970	PASS
68	69	0.00	2	0.8	103	PASS
69	198	0.00	100	27.8	13609	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.9	18081	PASS
197	198	0.00	2	0.5	257	PASS
198	198	100	100	100.0	48978	PASS
199	198	5	9	6.5	3198	PASS
275	198	10	60	28.2	13802	PASS
365	198	1	100	3.3	1610	PASS
441	198	0.01	100	15.1	7408	PASS
442	198	50	100	94.9	46474	PASS
443	442	15	24	18.9	8790	PASS