
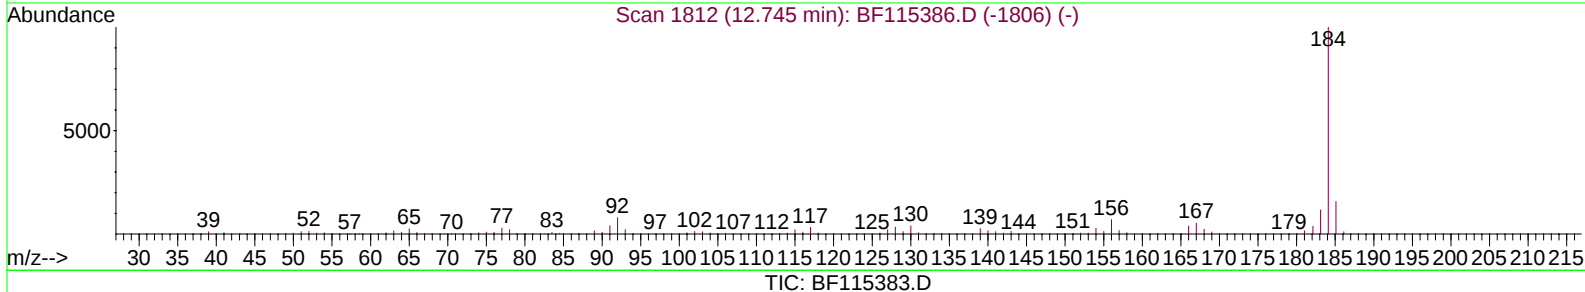
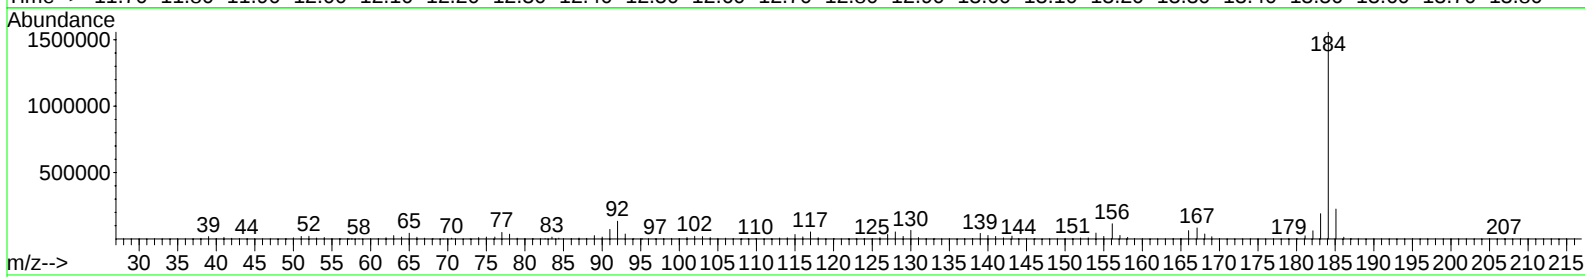


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070519\
Data File : BF115383.D
Acq On : 5 Jul 2019 8:04
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 05 17:42:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 14:57:35 2019
Response via : Initial Calibration

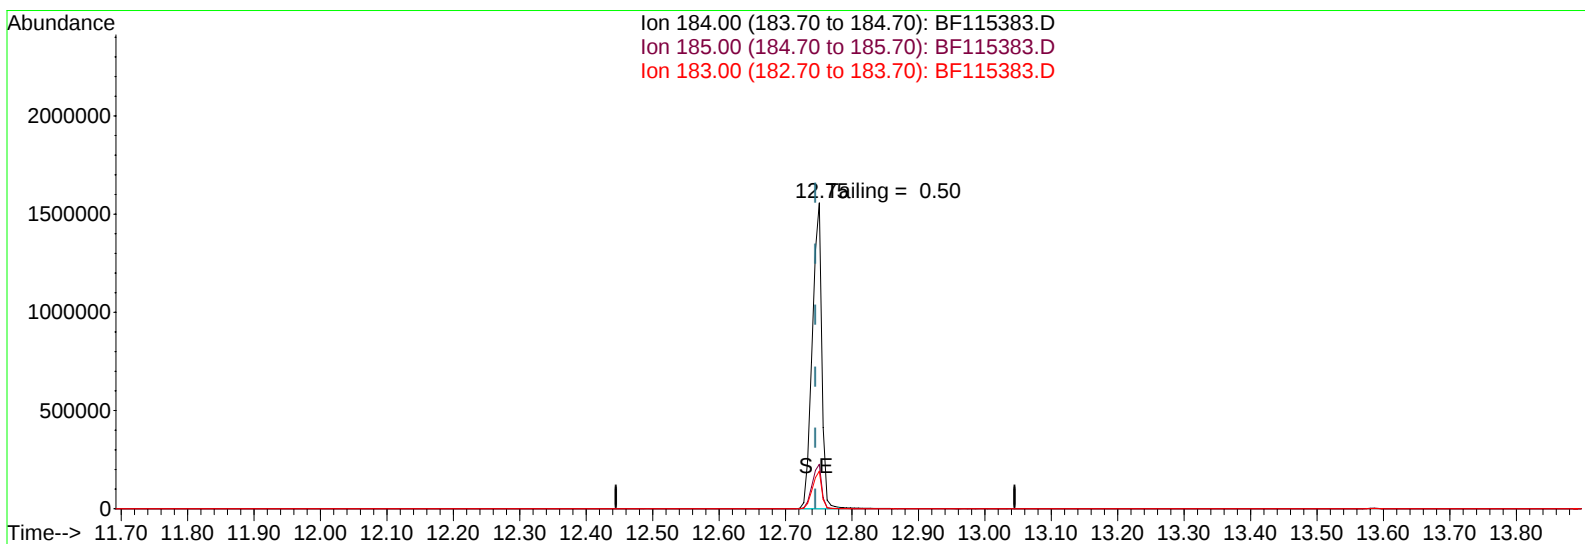

(77) Benzidine




12.751min (+0.006) 0.00ng

response 1565389

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.53
183.00	11.70	12.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070519\
Data File : BF115383.D
Acq On : 5 Jul 2019 8:04
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 05 17:42:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 14:57:35 2019
Response via : Initial Calibration

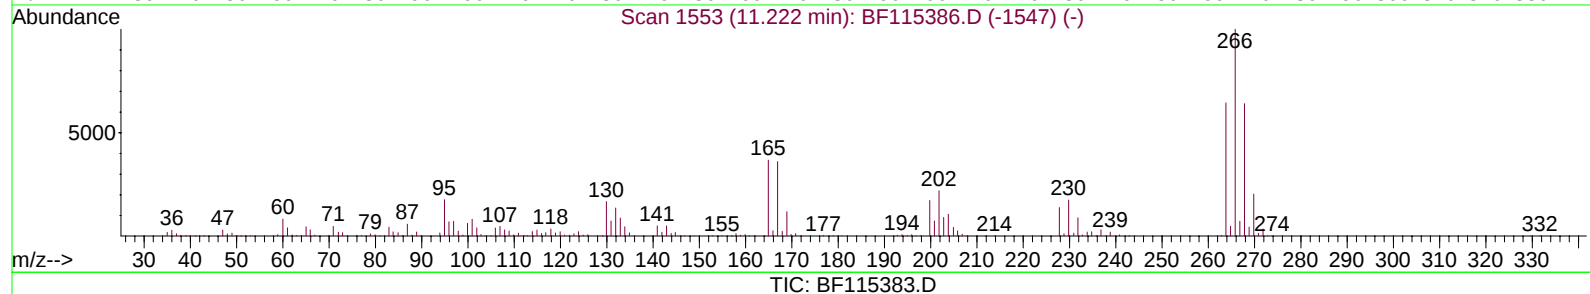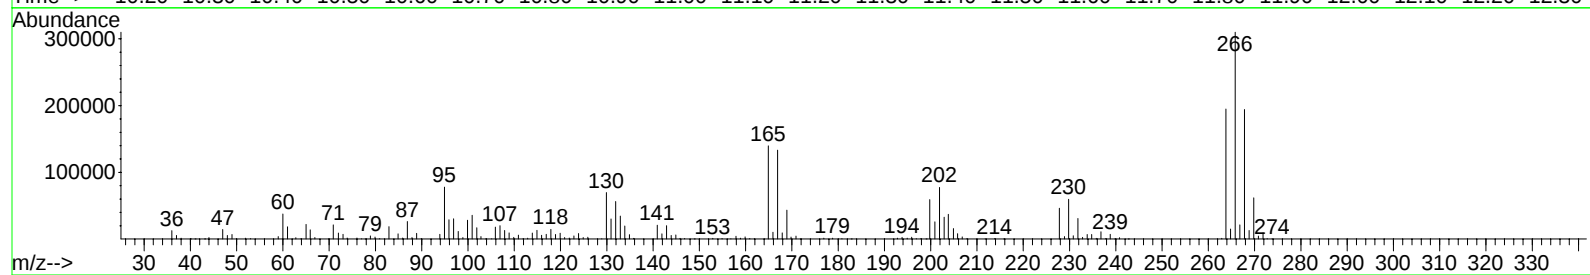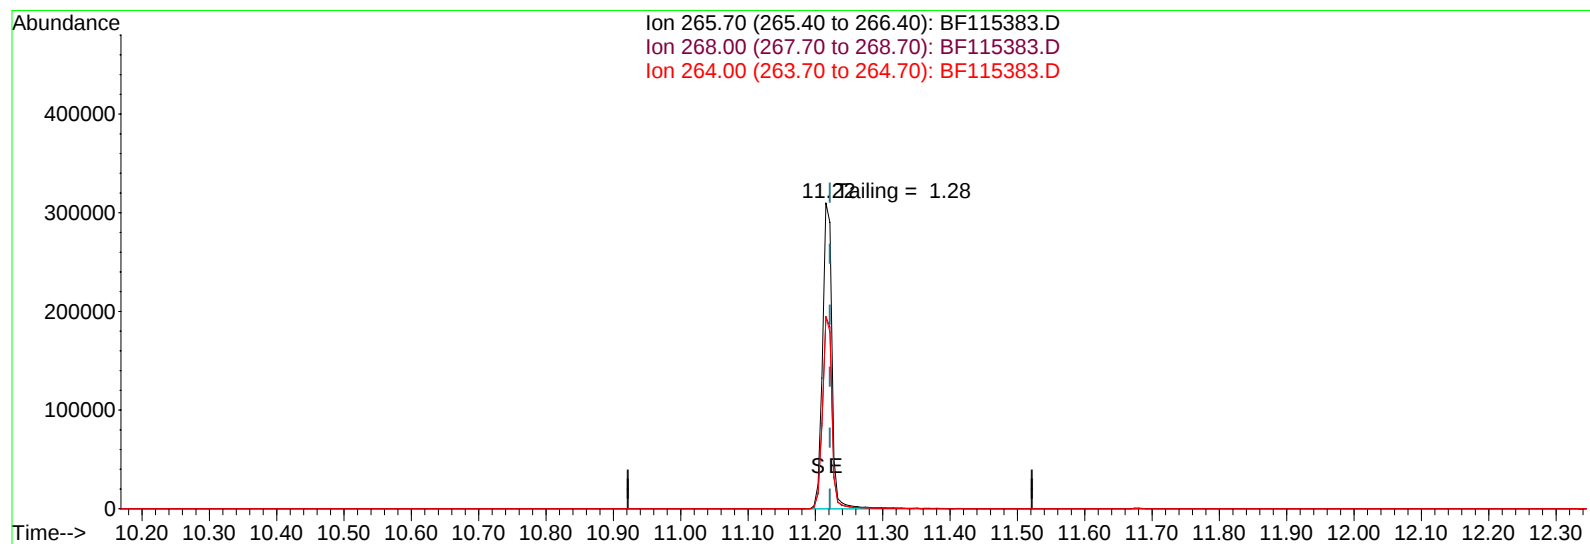

(70) Pentachlorophenol (C)

11.216min (-0.006) 47146.87ng

response 300636

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	62.68
264.00	64.50	62.91
0.00	0.00	0.00