


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070519\
 Data File : BF115383.D
 Acq On : 5 Jul 2019 8:04
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 05 14:57:35 2019

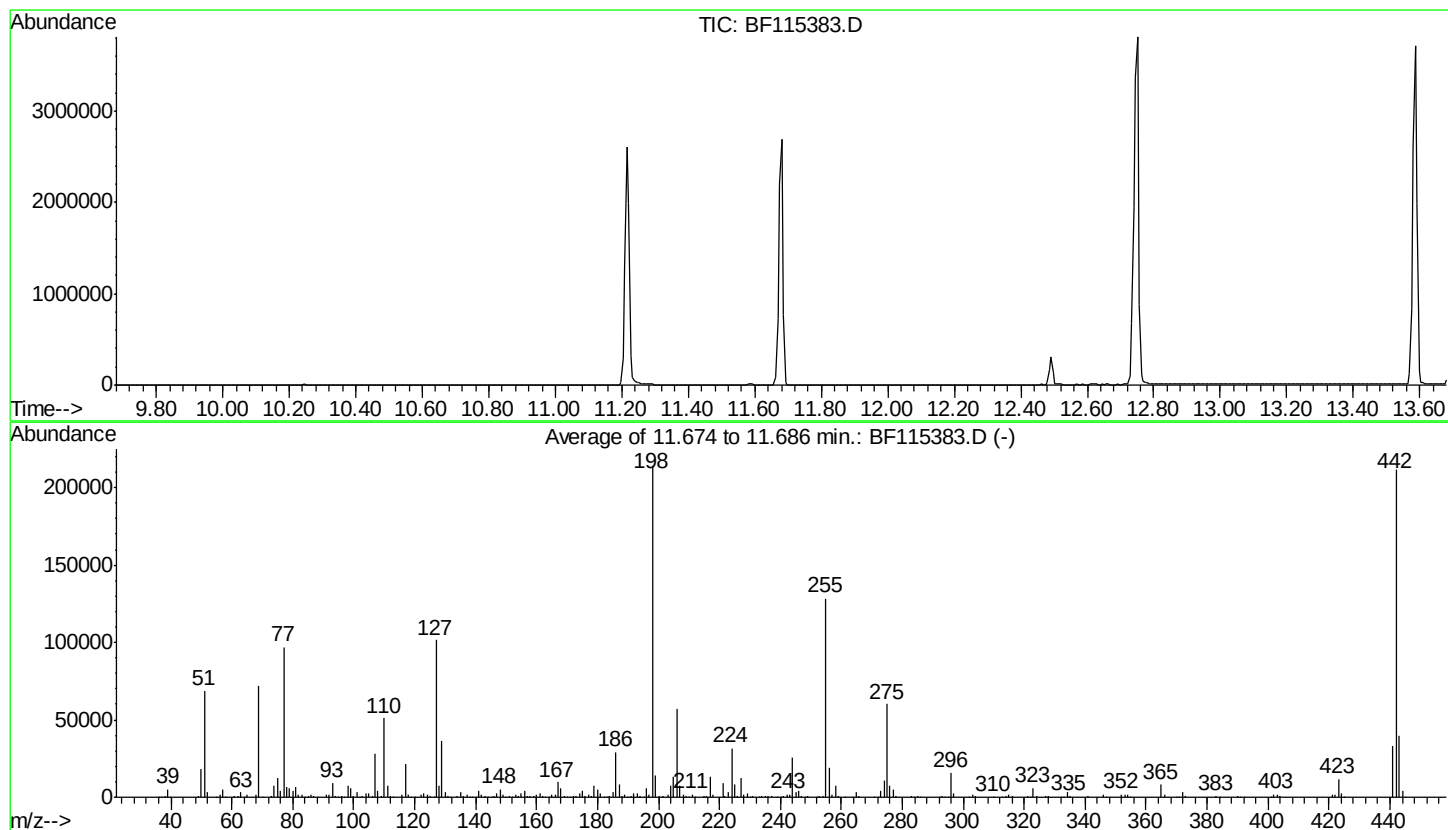

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	68965	PASS
68	69	0.00	2	1.8	1287	PASS
69	198	0.00	100	33.6	72020	PASS
70	69	0.00	2	0.6	414	PASS
127	198	10	80	47.4	101485	PASS
197	198	0.00	2	0.6	1316	PASS
198	198	100	100	100.0	214202	PASS
199	198	5	9	6.6	14243	PASS
275	198	10	60	28.0	60050	PASS
365	198	1	100	3.7	8010	PASS
441	198	0.01	100	15.4	32922	PASS
442	198	50	100	99.0	211968	PASS
443	442	15	24	18.8	39944	PASS