
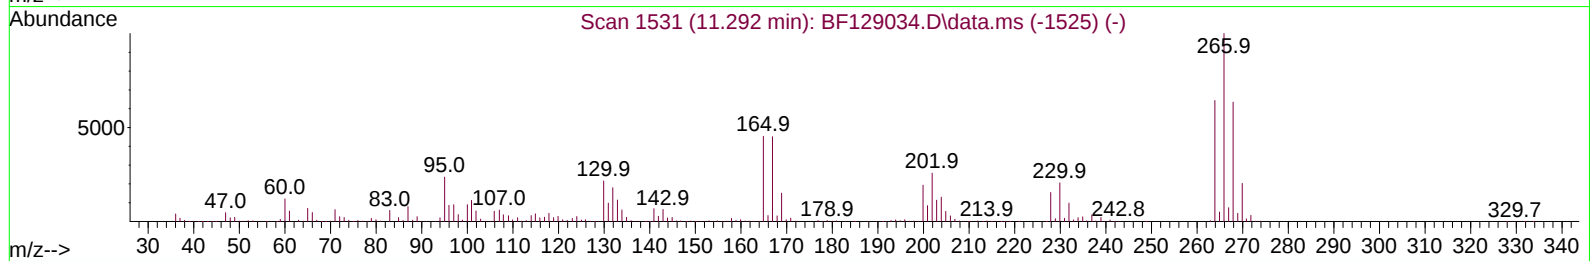
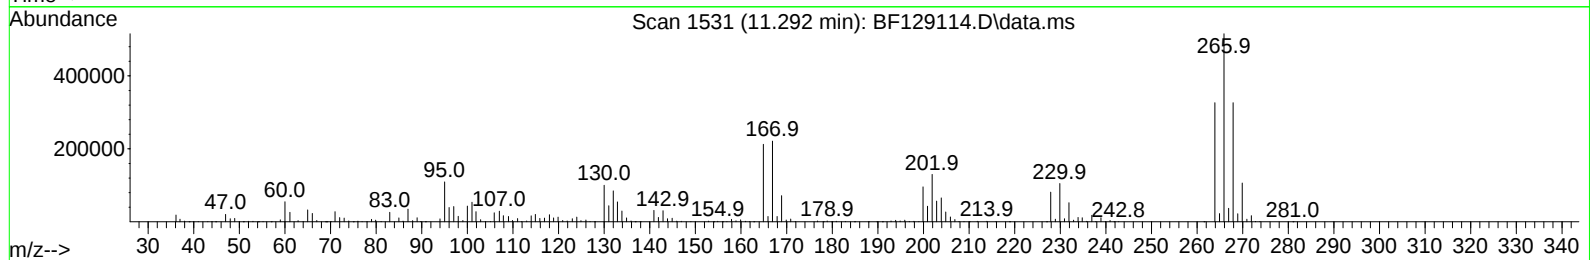


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
Data File : BF129114.D
Acq On : 05 Jul 2022 09:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 05 16:33:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

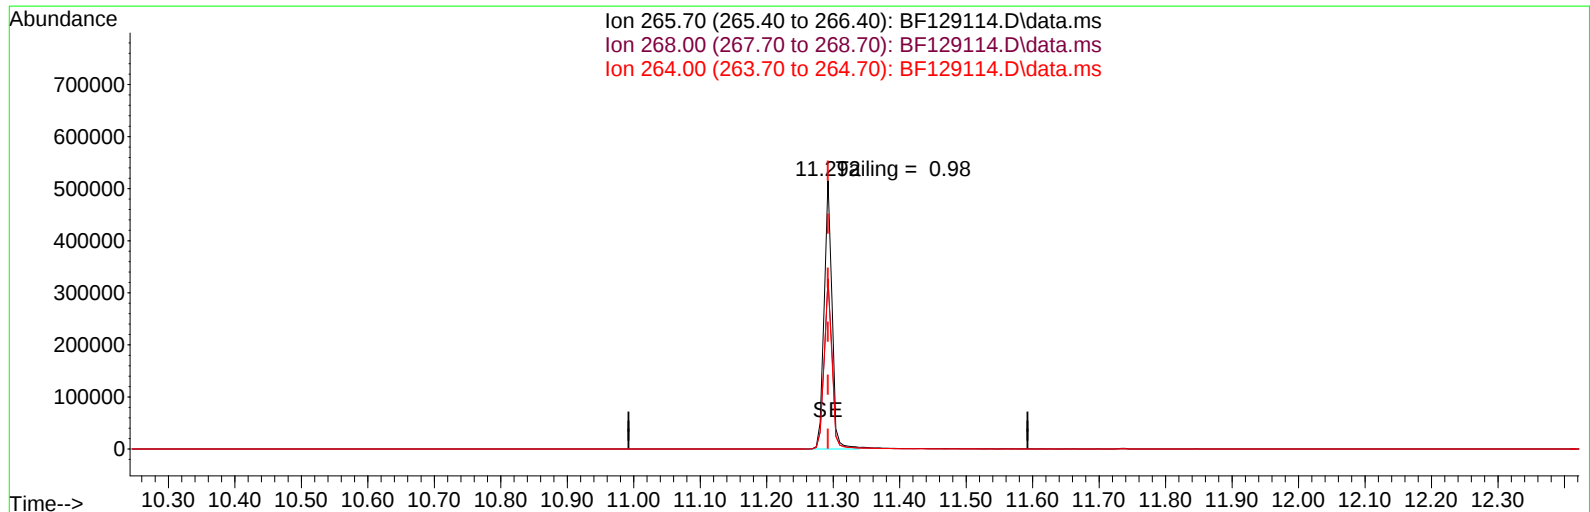

TIC: BF129114.D\data.ms

(70) Pentachlorophenol (C)




11.292min (-0.000) 128514.68 ng

response 434298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.32
264.00	61.80	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
Data File : BF129114.D
Acq On : 05 Jul 2022 09:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 05 16:33:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

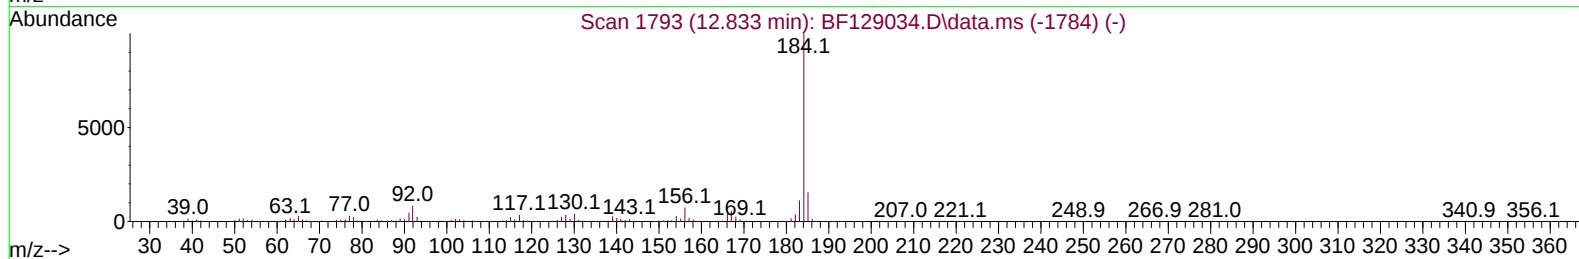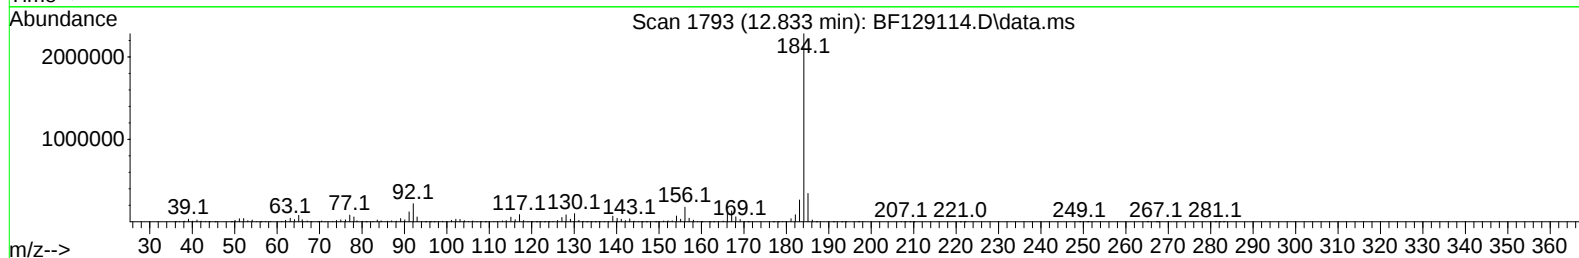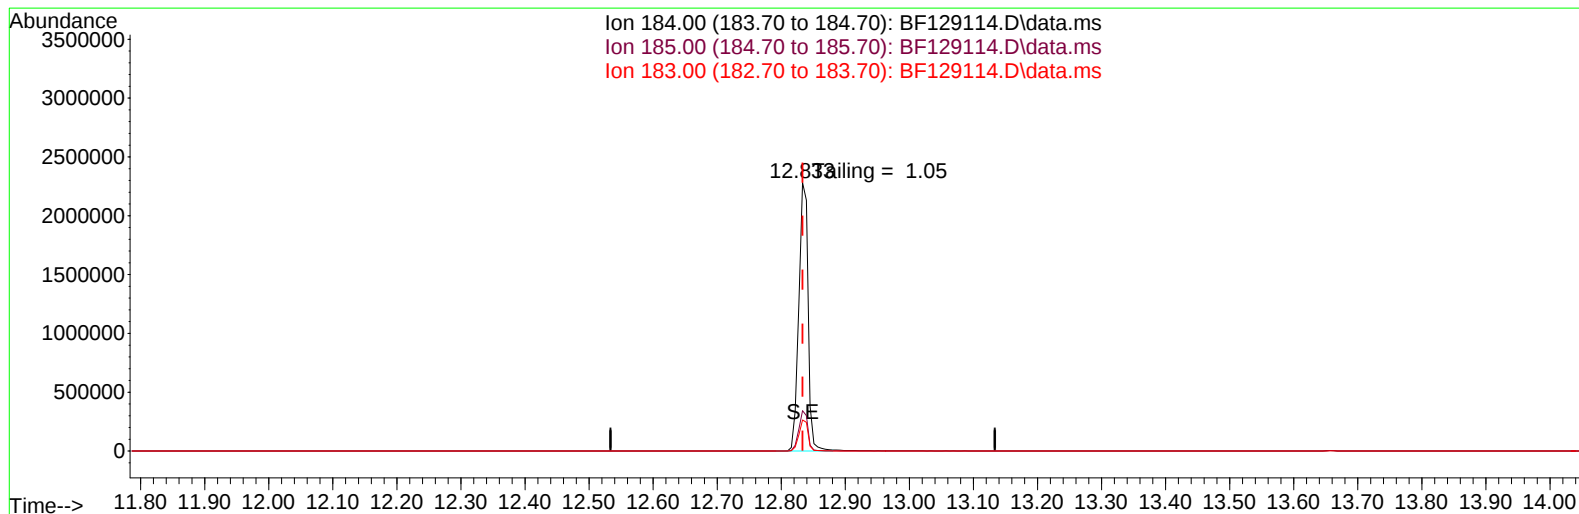

TIC: BF129114.D\data.ms

(77) Benzidine

12.833min (-0.000) 161318.11 ng

response 2346820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.06
183.00	11.60	11.57
0.00	0.00	0.00