

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
 Data File : BF129116.D
 Acq On : 05 Jul 2022 11:03
 Operator : CG\JU
 Sample : PB145999BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145999BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.369	6	14	22	rVB	211790	303560	2.68%	0.439%
2	5.592	556	562	565	rBV	8353970	8593563	75.83%	12.436%
3	6.581	724	730	733	rBV	7431052	8544336	75.40%	12.364%
4	6.957	790	794	797	rBV	2721568	2104694	18.57%	3.046%
5	7.522	884	890	893	rBV	5741680	5803576	51.21%	8.398%
6	8.239	1007	1012	1015	rBV	3219081	2853012	25.17%	4.129%
7	9.316	1189	1195	1198	rBV	10864950	10811435	95.40%	15.645%
8	9.998	1305	1311	1315	rBV	3771370	3195184	28.19%	4.624%
9	10.792	1439	1446	1449	rBV	7580783	6863774	60.57%	9.932%
10	11.492	1561	1565	1568	rBV	3980158	3272533	28.88%	4.736%
11	13.086	1830	1836	1839	rBV	11470461	11332726	100.00%	16.399%
12	14.139	2011	2015	2019	rBV	2958135	2772139	24.46%	4.012%
13	14.233	2026	2031	2036	rBV	88250	120867	1.07%	0.175%
14	15.668	2269	2275	2287	rBV	1842119	2410820	21.27%	3.489%
15	16.133	2351	2354	2360	rVB	78568	122260	1.08%	0.177%




Sum of corrected areas: 69104479

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
Data File : BF129116.D
Acq On : 05 Jul 2022 11:03
Operator : CG\JU
Sample : PB145999BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145999BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

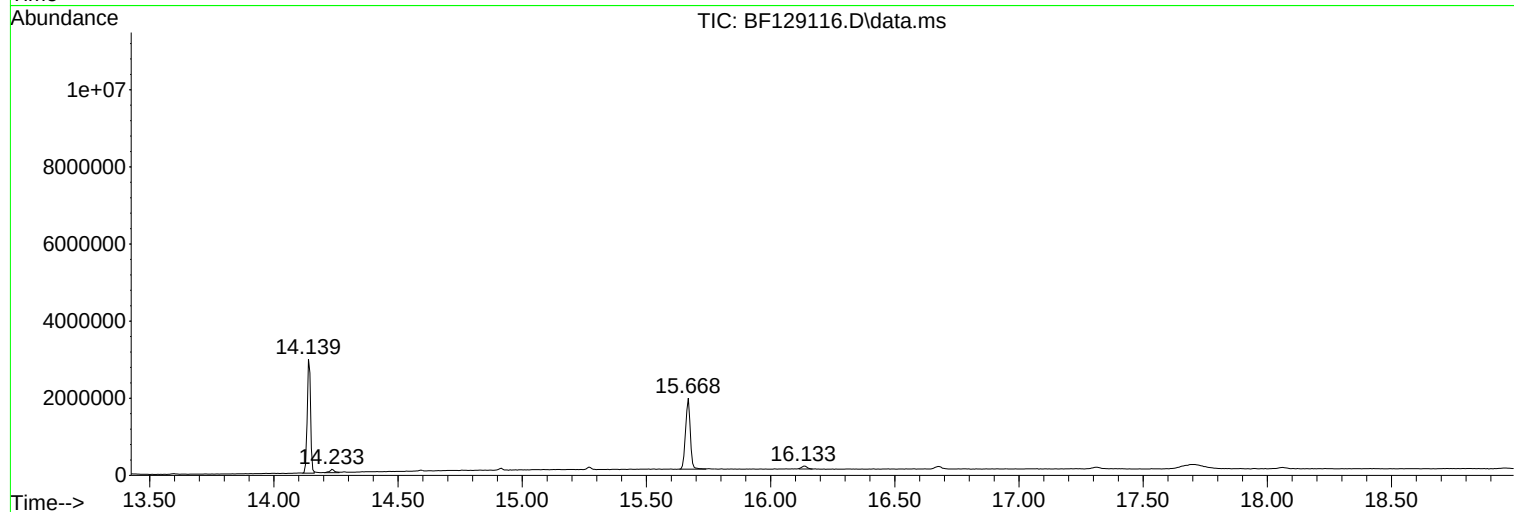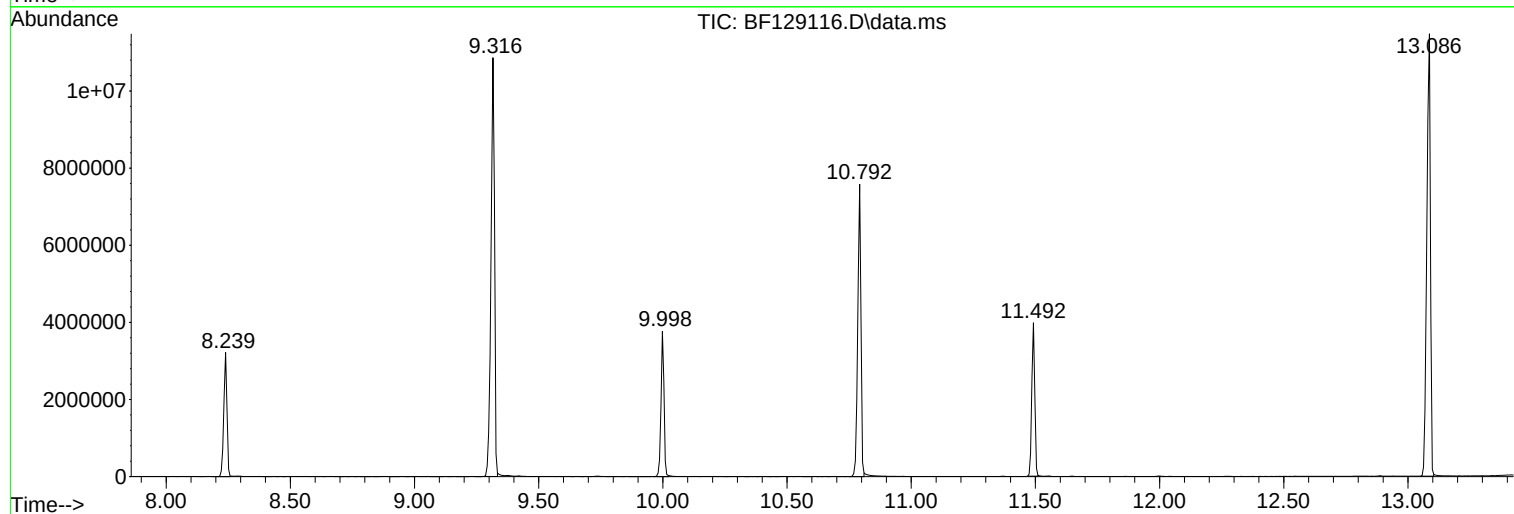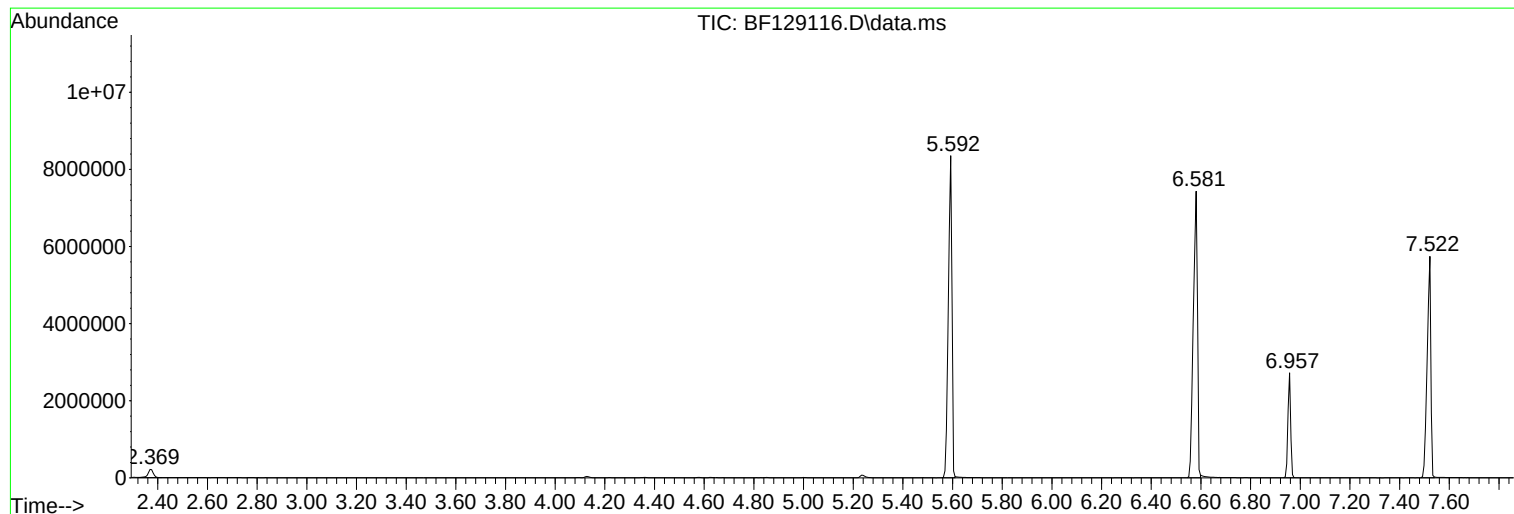

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
Data File : BF129116.D
Acq On : 05 Jul 2022 11:03
Operator : CG\JU
Sample : PB145999BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145999BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.369	2.88 ng	303560	1,4-Dichlorobenzene-d4	6.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12

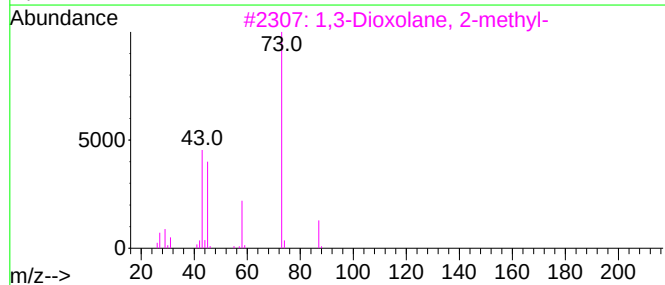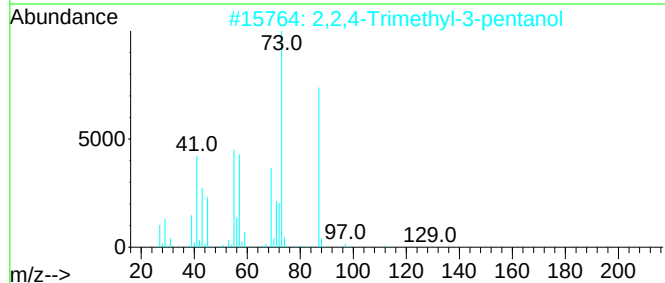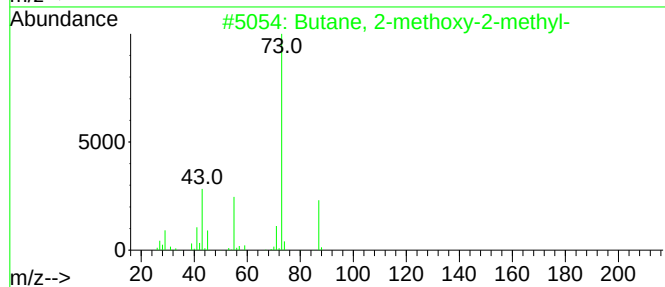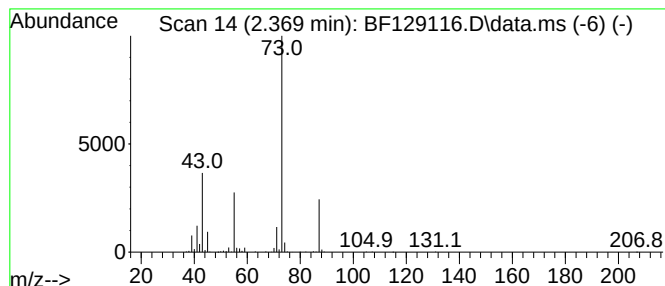

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
Data File : BF129116.D
Acq On : 05 Jul 2022 11:03
Operator : CG\JU
Sample : PB145999BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145999BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.369	2.9	ng	303560	1	6.957	2104690	20.0