


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
 Data File : BF129114.D
 Acq On : 05 Jul 2022 09:32
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

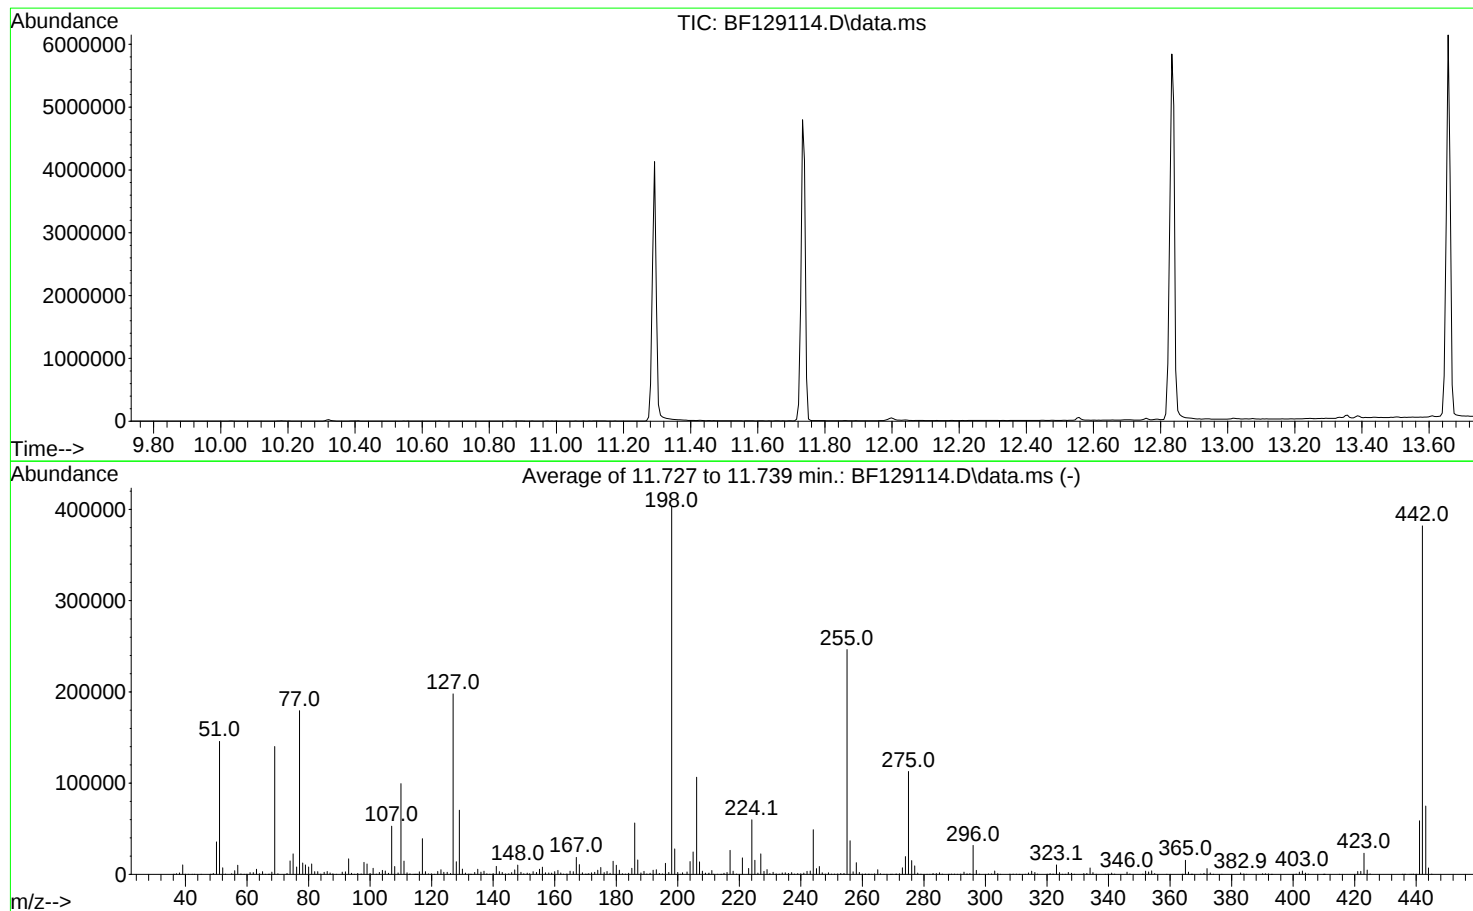




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	145789	PASS
68	69	0.00	2	1.8	2492	PASS
69	198	0.00	100	34.8	140152	PASS
70	69	0.00	2	0.6	779	PASS
127	198	10	80	49.1	197893	PASS
197	198	0.00	2	0.5	2104	PASS
198	198	100	100	100.0	403221	PASS
199	198	5	9	6.9	27870	PASS
275	198	10	60	28.0	112771	PASS
365	198	1	100	3.8	15375	PASS
441	198	0.01	100	14.6	58813	PASS
442	442	50	100	100.0	381920	PASS
443	442	15	24	19.6	74843	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
Data File : BF129114.D
Acq On : 05 Jul 2022 09:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 05 16:33:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

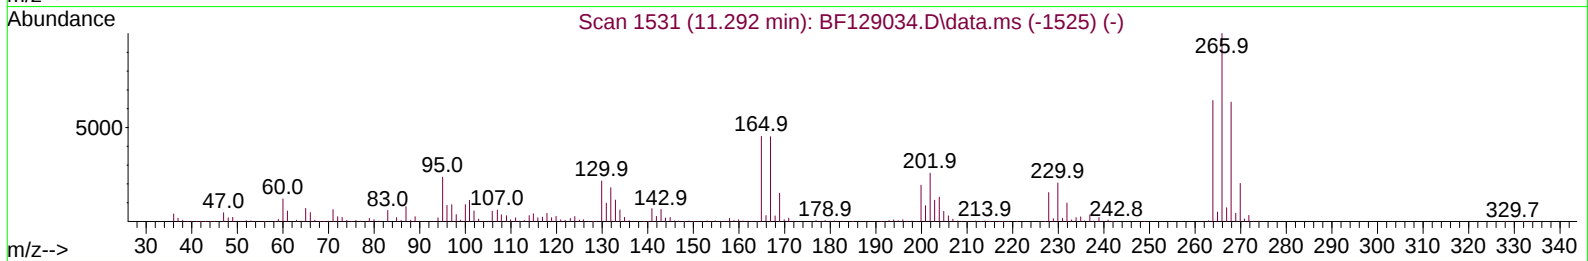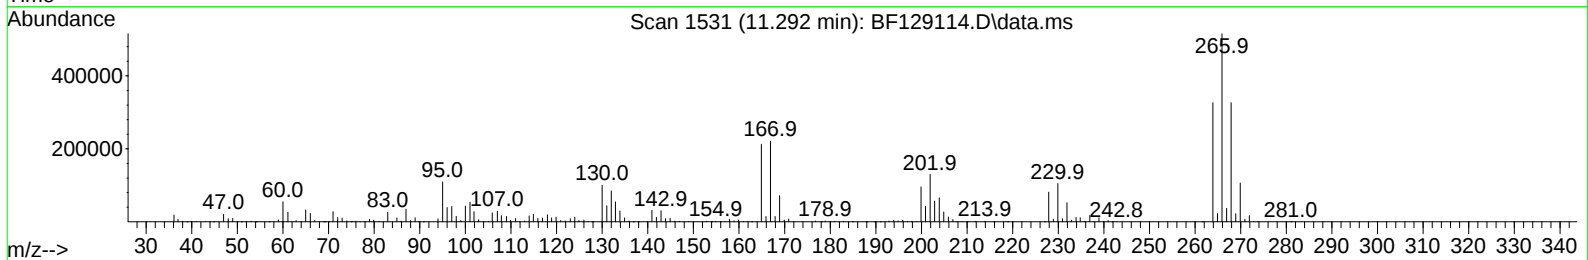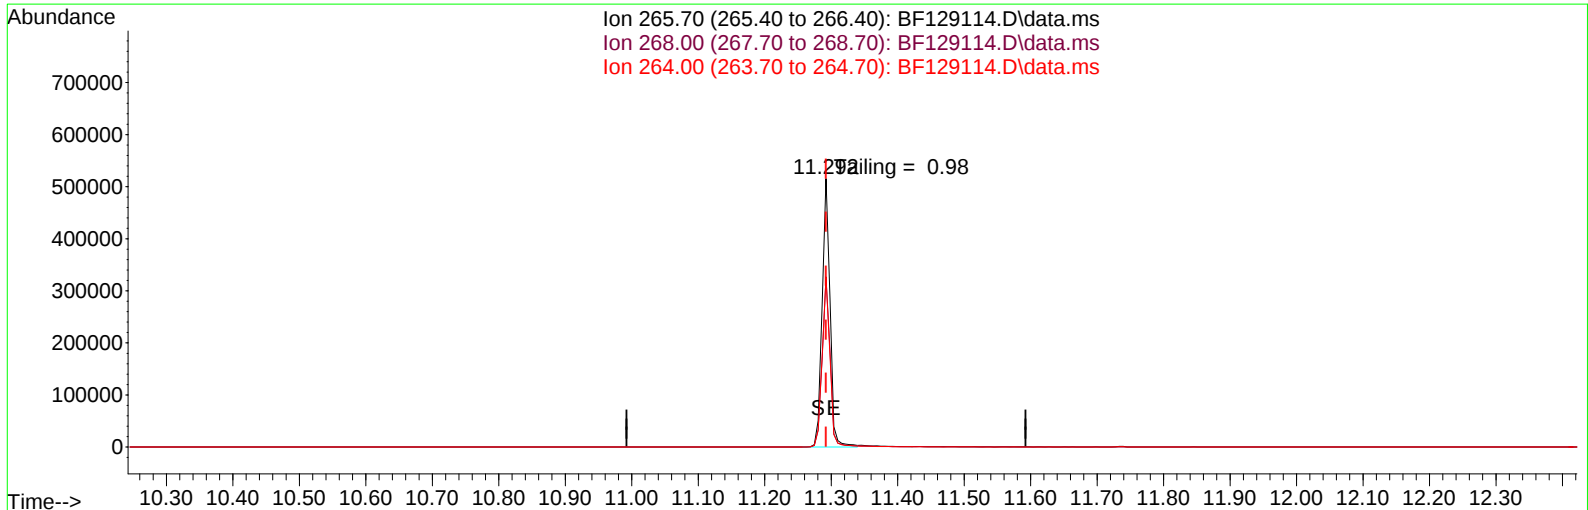

TIC: BF129114.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 128514.68 ng




response 434298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.32
264.00	61.80	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070522\
 Data File : BF129114.D
 Acq On : 05 Jul 2022 09:32
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 05 16:33:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

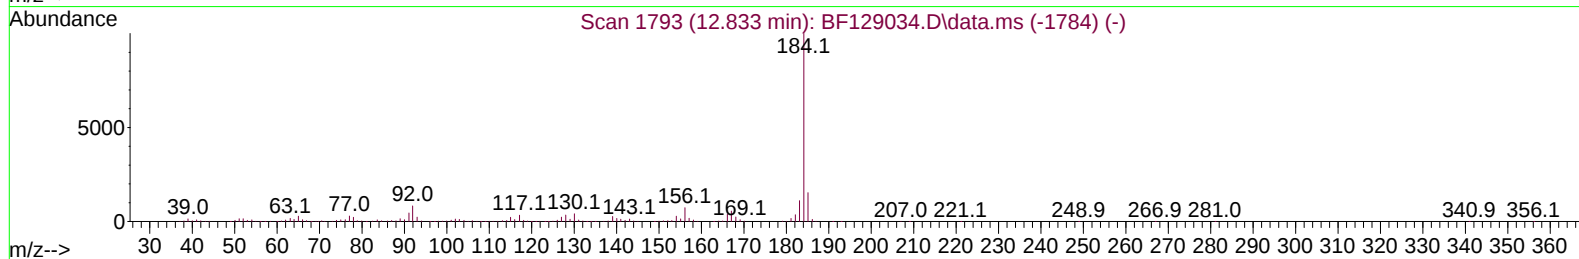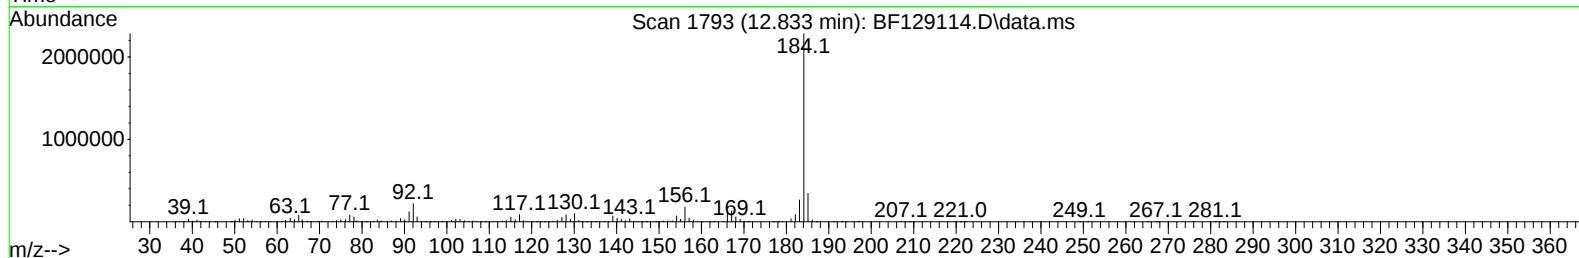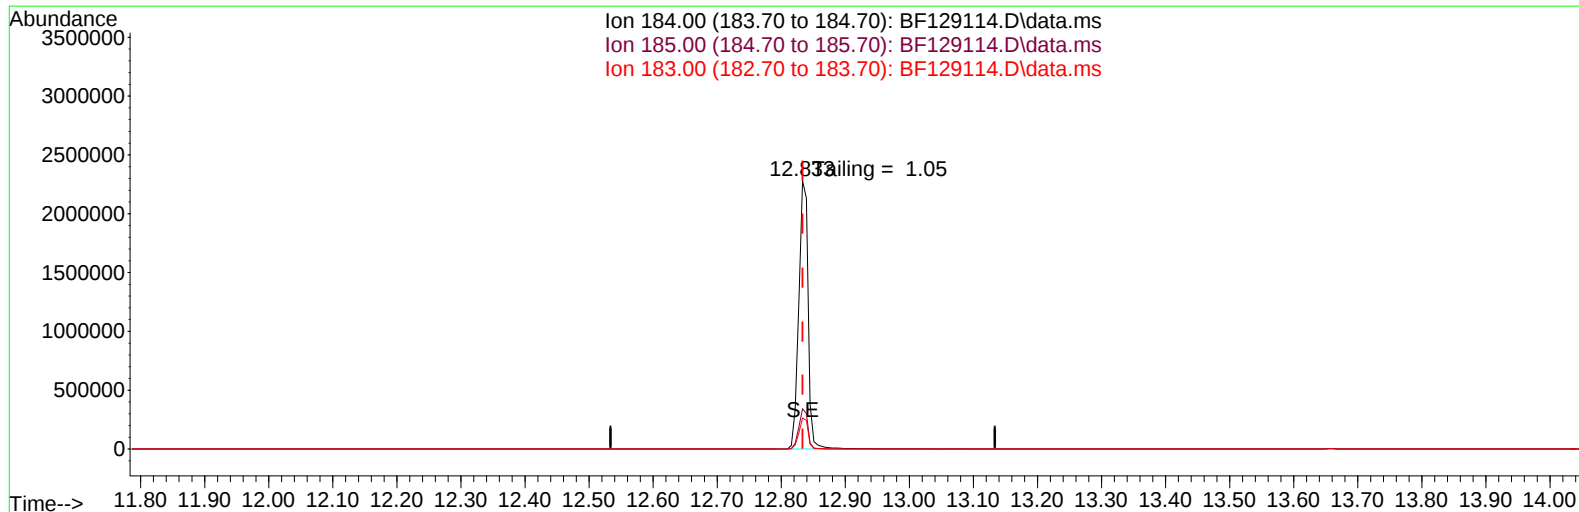

TIC: BF129114.D\data.ms

(77) Benzidine

12.833min (-0.000) 161318.11 ng

response 2346820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.06
183.00	11.60	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/5/2022	BNA_F	<u>BF129114.D</u>
Compound Name	Response	Retention Time
DDT	979565	13.65
DDD	8186	13.35
DDE	2756	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10942	990507	1.10

Instrument :
BNA_F
ClientSampleId :
DFTPP