
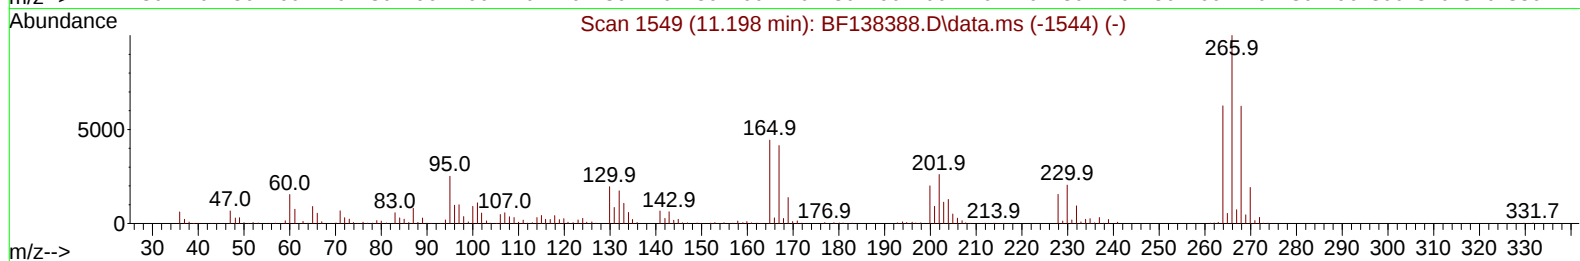
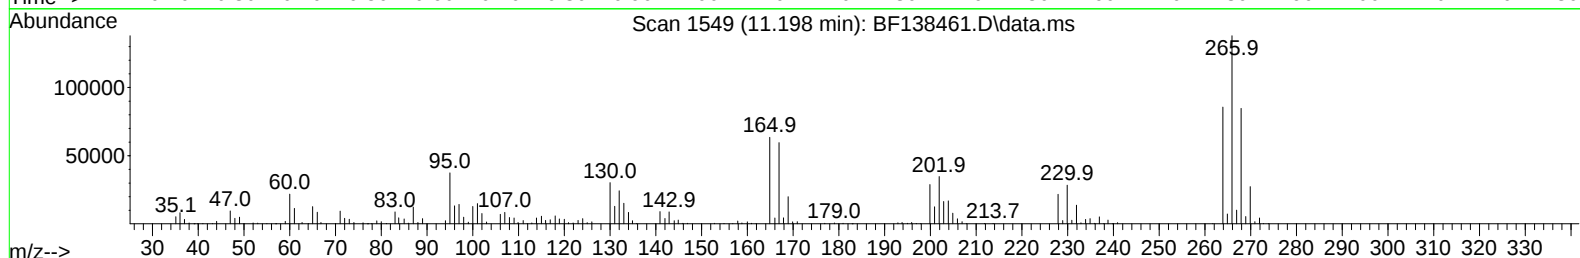


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070524\  
Data File : BF138461.D  
Acq On    : 05 Jul 2024  11:17  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 05 12:55:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

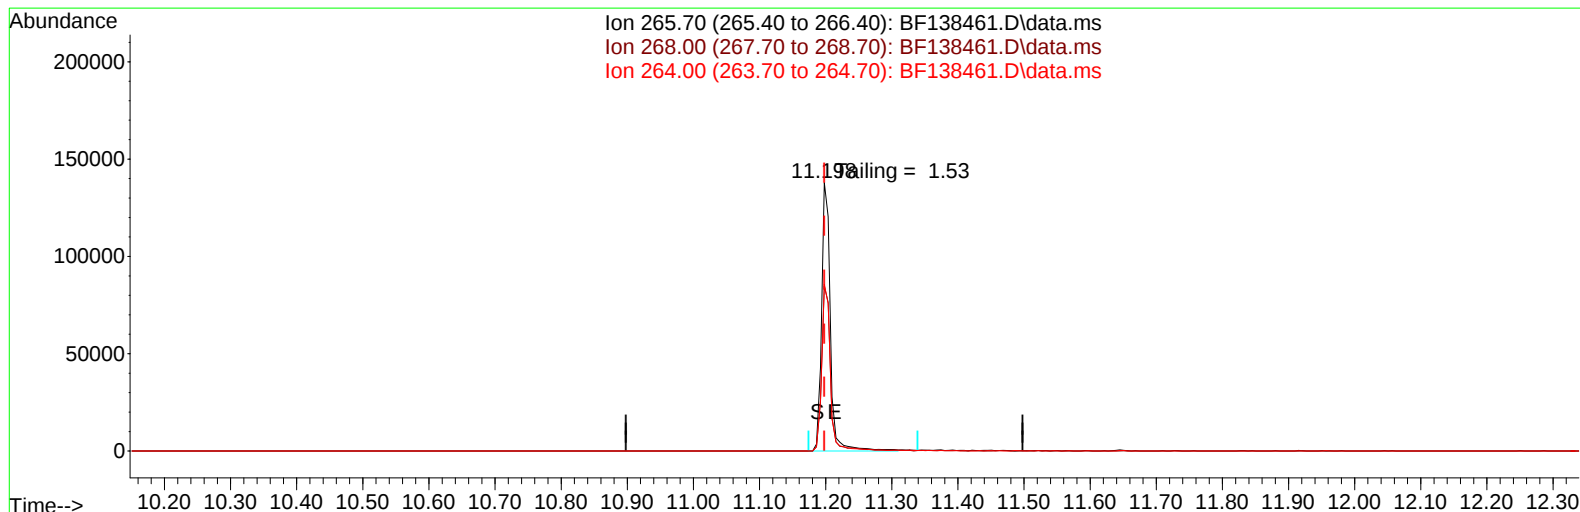

TIC: BF138461.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 26457.56 ng

response **129022**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	62.40	61.40
--------	-------	-------

264.00	62.50	62.11
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070524\
Data File : BF138461.D
Acq On : 05 Jul 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 05 12:55:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

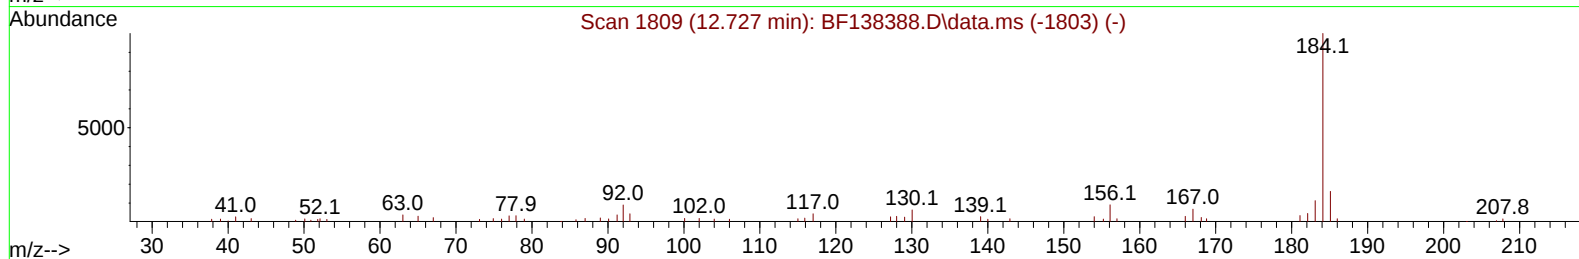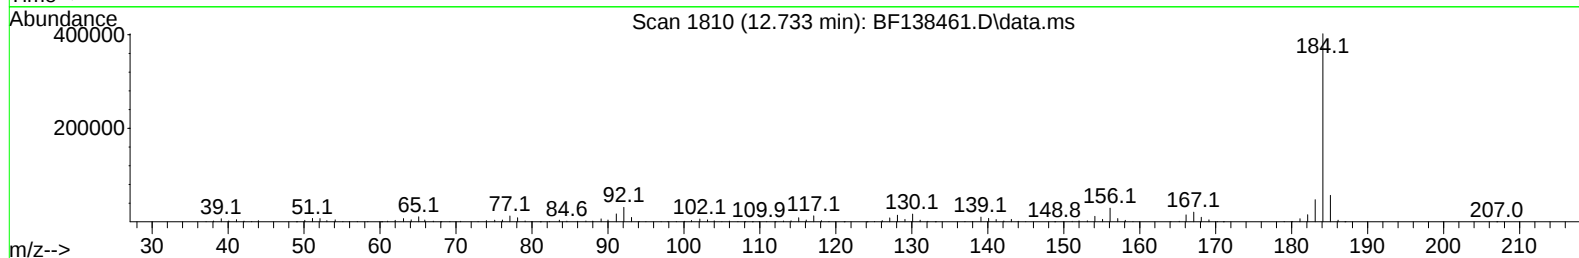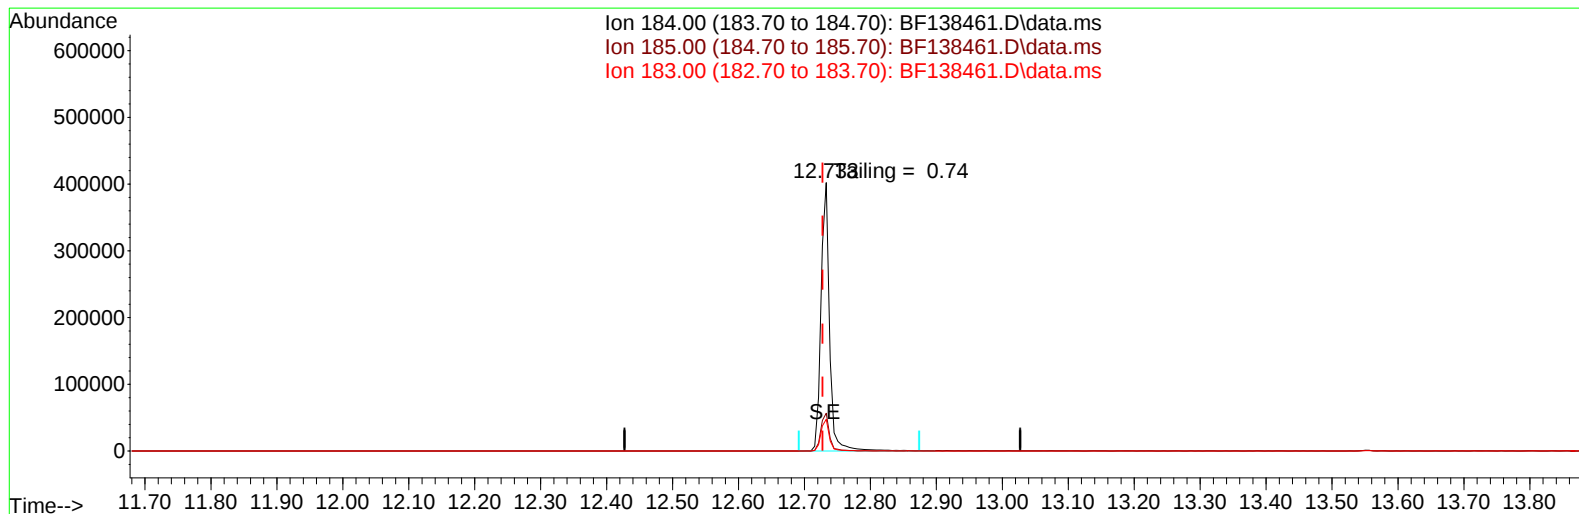

TIC: BF138461.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 80493.02 ng

response 362377

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.09
183.00	11.30	11.82
0.00	0.00	0.00