


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070524\
Data File : BF138461.D
Acq On : 05 Jul 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

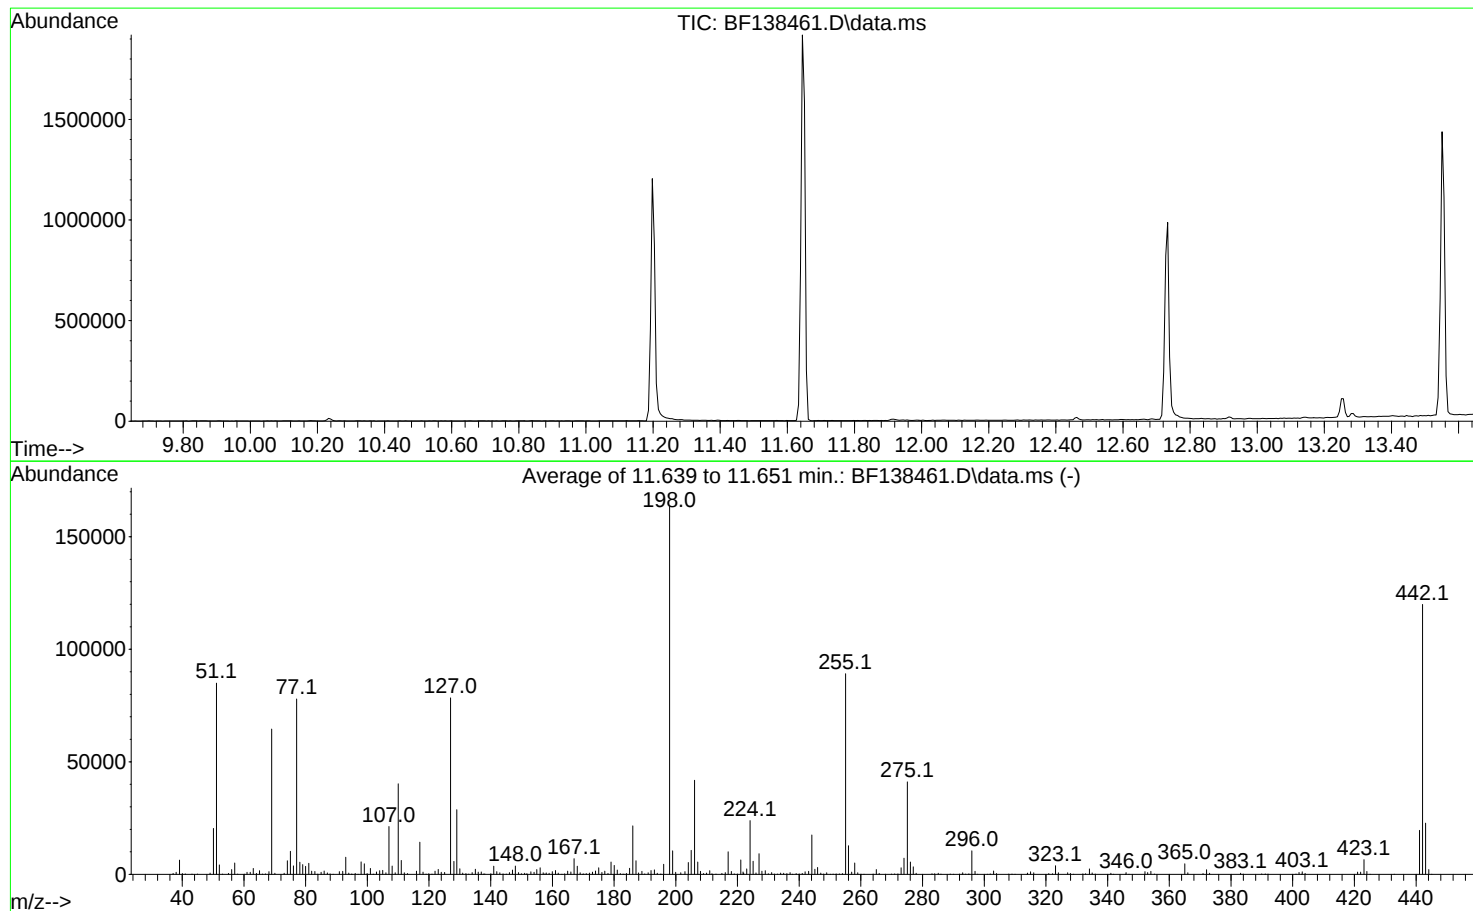

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	84965	PASS
68	69	0.00	2	1.8	1184	PASS
69	198	0.00	100	39.5	64520	PASS
70	69	0.00	2	0.8	488	PASS
127	198	10	80	48.0	78429	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	163437	PASS
199	198	5	9	6.4	10481	PASS
275	198	10	60	25.1	41061	PASS
365	198	1	100	2.9	4683	PASS
441	198	0.01	100	12.0	19561	PASS
442	442	50	100	100.0	119899	PASS
443	442	15	24	19.0	22791	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/5/2024	BNA_F	<u>BF138461.D</u>
Compound Name	Response	Retention Time
DDT	230197	13.551
DDD	19563	13.257
DDE	1101	12.915
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20664	250861	8.24

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070524\
Data File : BF138461.D
Acq On : 05 Jul 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 05 12:55:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

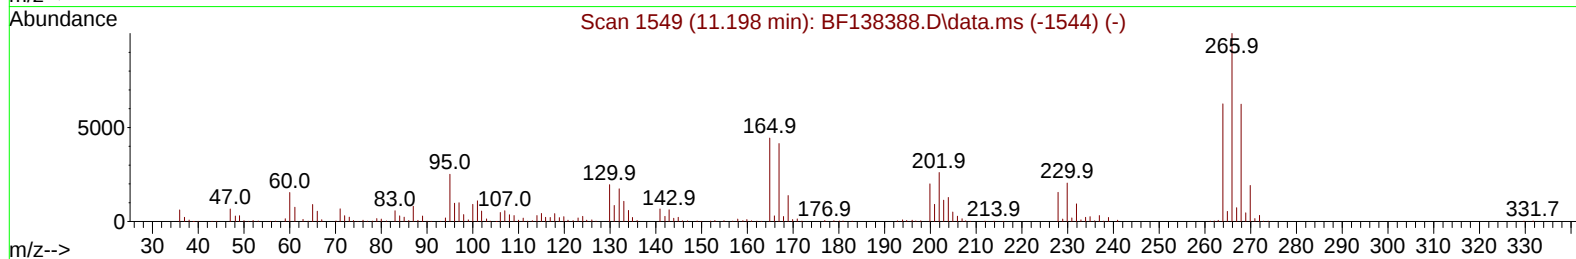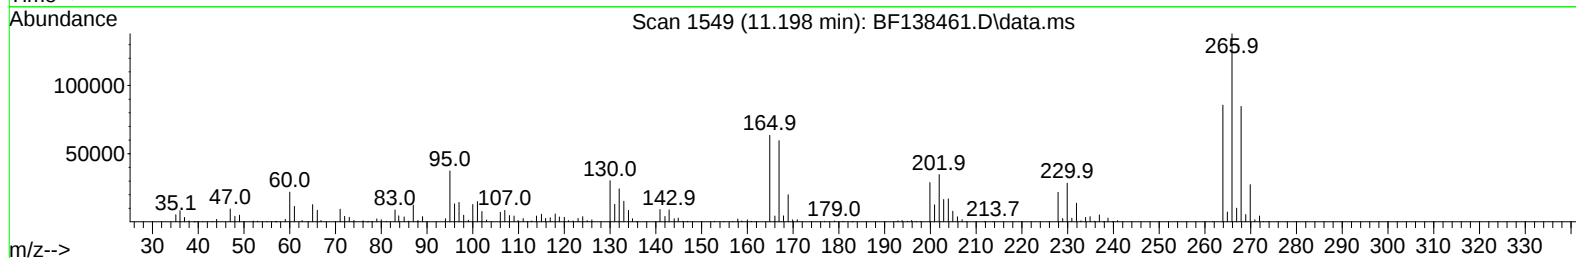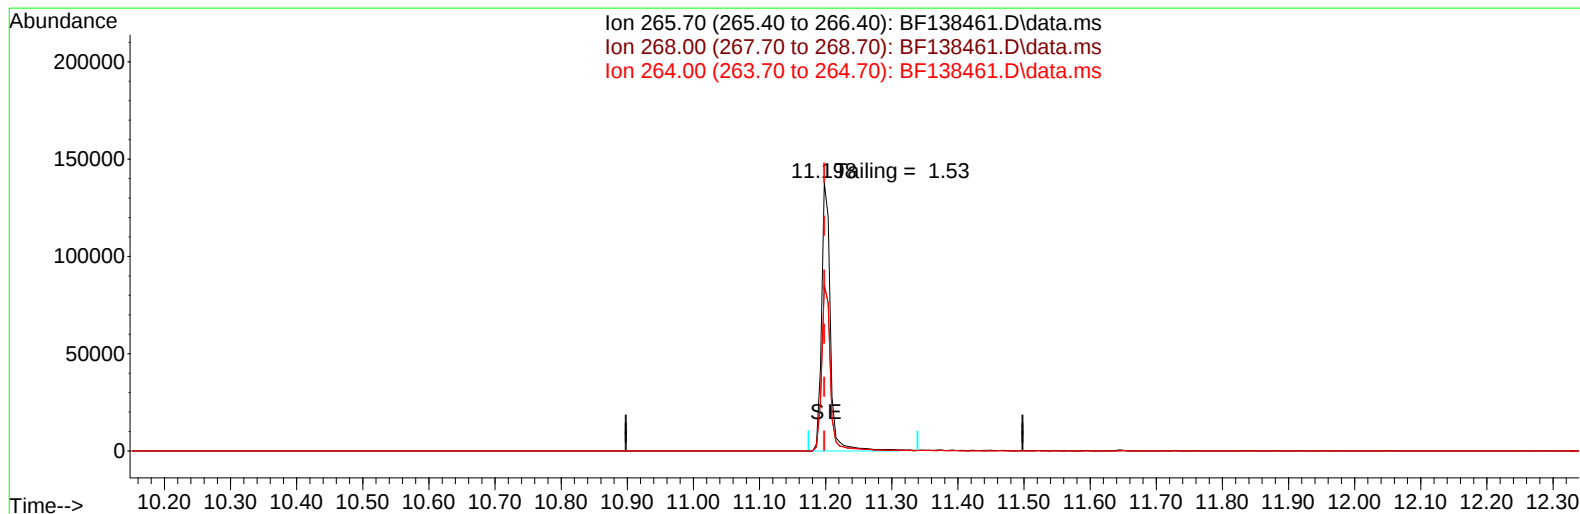

TIC: BF138461.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 26457.56 ng




response 129022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	61.40
264.00	62.50	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070524\
Data File : BF138461.D
Acq On : 05 Jul 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 05 12:55:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

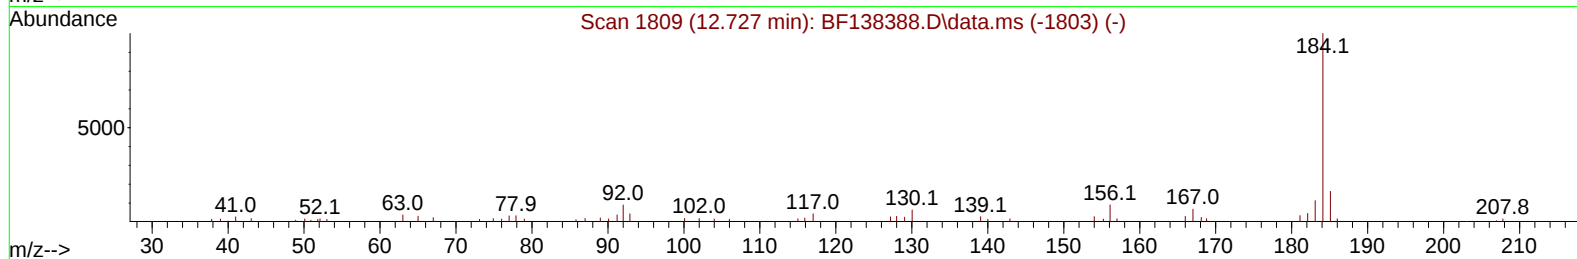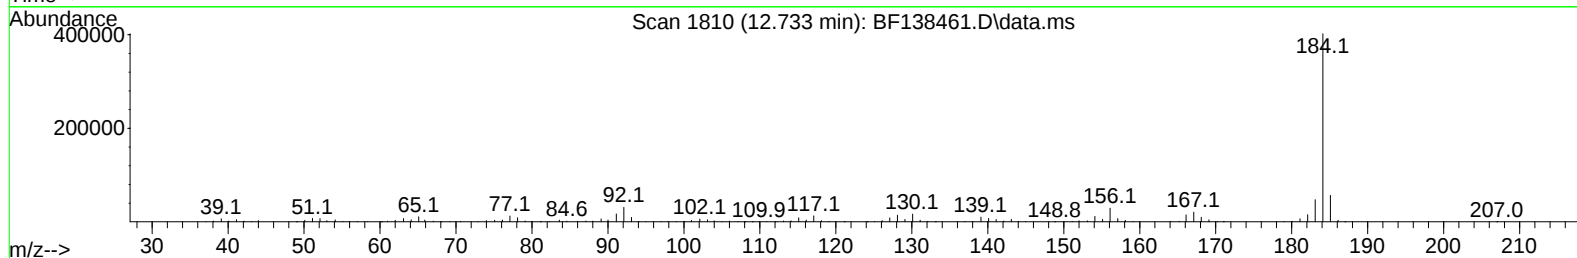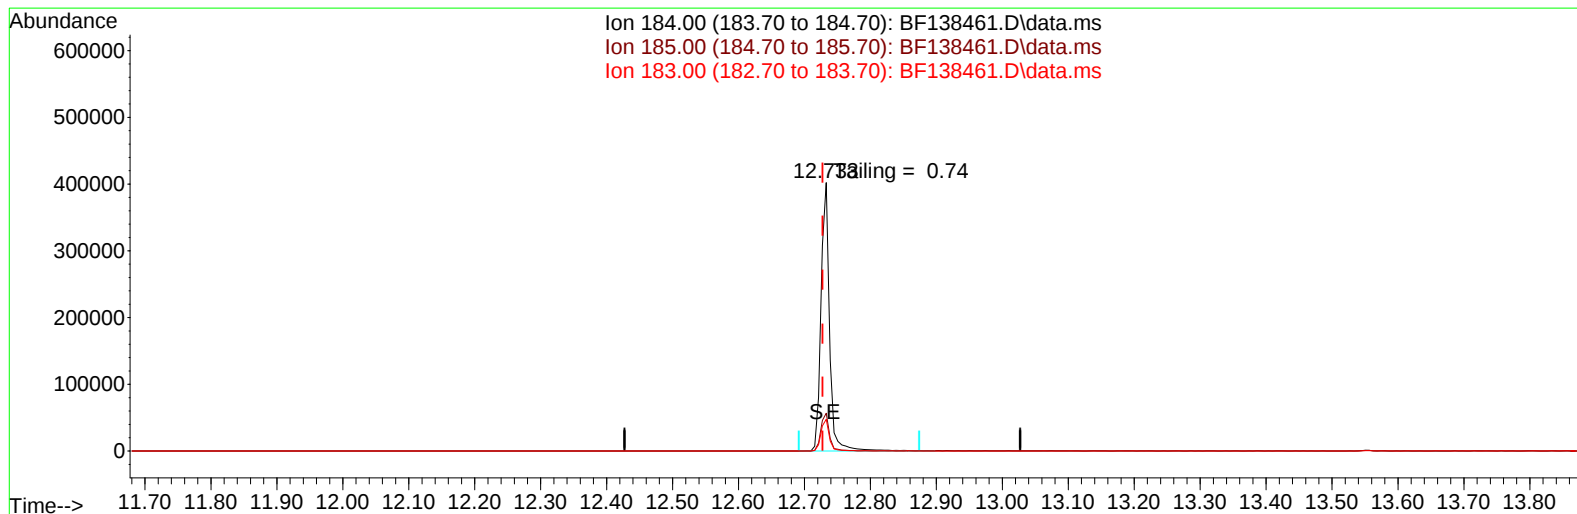

TIC: BF138461.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 80493.02 ng

response 362377

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.09
183.00	11.30	11.82
0.00	0.00	0.00