

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070615\
 Data File : BF080356.D
 Acq On : 6 Jul 2015 20:52
 Operator : TP/IZ
 Sample : G2877-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-152-7215

Quant Time: Jul 07 05:14:25 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 03:05:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.23	152	34663	20.00	ng	0.00
21) Naphthalene-d8	8.52	136	125625	20.00	ng	0.00
38) Acenaphthene-d10	10.29	164	59724	20.00	ng	0.00
63) Phenanthrene-d10	11.80	188	128189	20.00	ng	0.01
75) Chrysene-d12	14.84	240	141100	20.00	ng	0.10
86) Perylene-d12	16.75	264	129558	20.00	ng	0.19
System Monitoring Compounds						
5) 2-Fluorophenol	5.84	112	113023	59.72	ng	0.00
7) Phenol-d6	6.83	99	94081	37.50	ng	0.00
23) Nitrobenzene-d5	7.79	82	209670	97.35	ng	0.00
41) 2,4,6-Tribromophenol	11.08	330	100049	160.10	ng	0.00
44) 2-Fluorobiphenyl	9.60	172	484917	109.57	ng	0.00
78) Terphenyl-d14	13.53	244	608310	100.56	ng	0.06


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070615\
Data File : BF080356.D
Acq On : 6 Jul 2015 20:52
Operator : TP/IZ
Sample : G2877-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-152-7215

Quant Time: Jul 07 05:14:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 03:05:40 2015
Response via : Initial Calibration




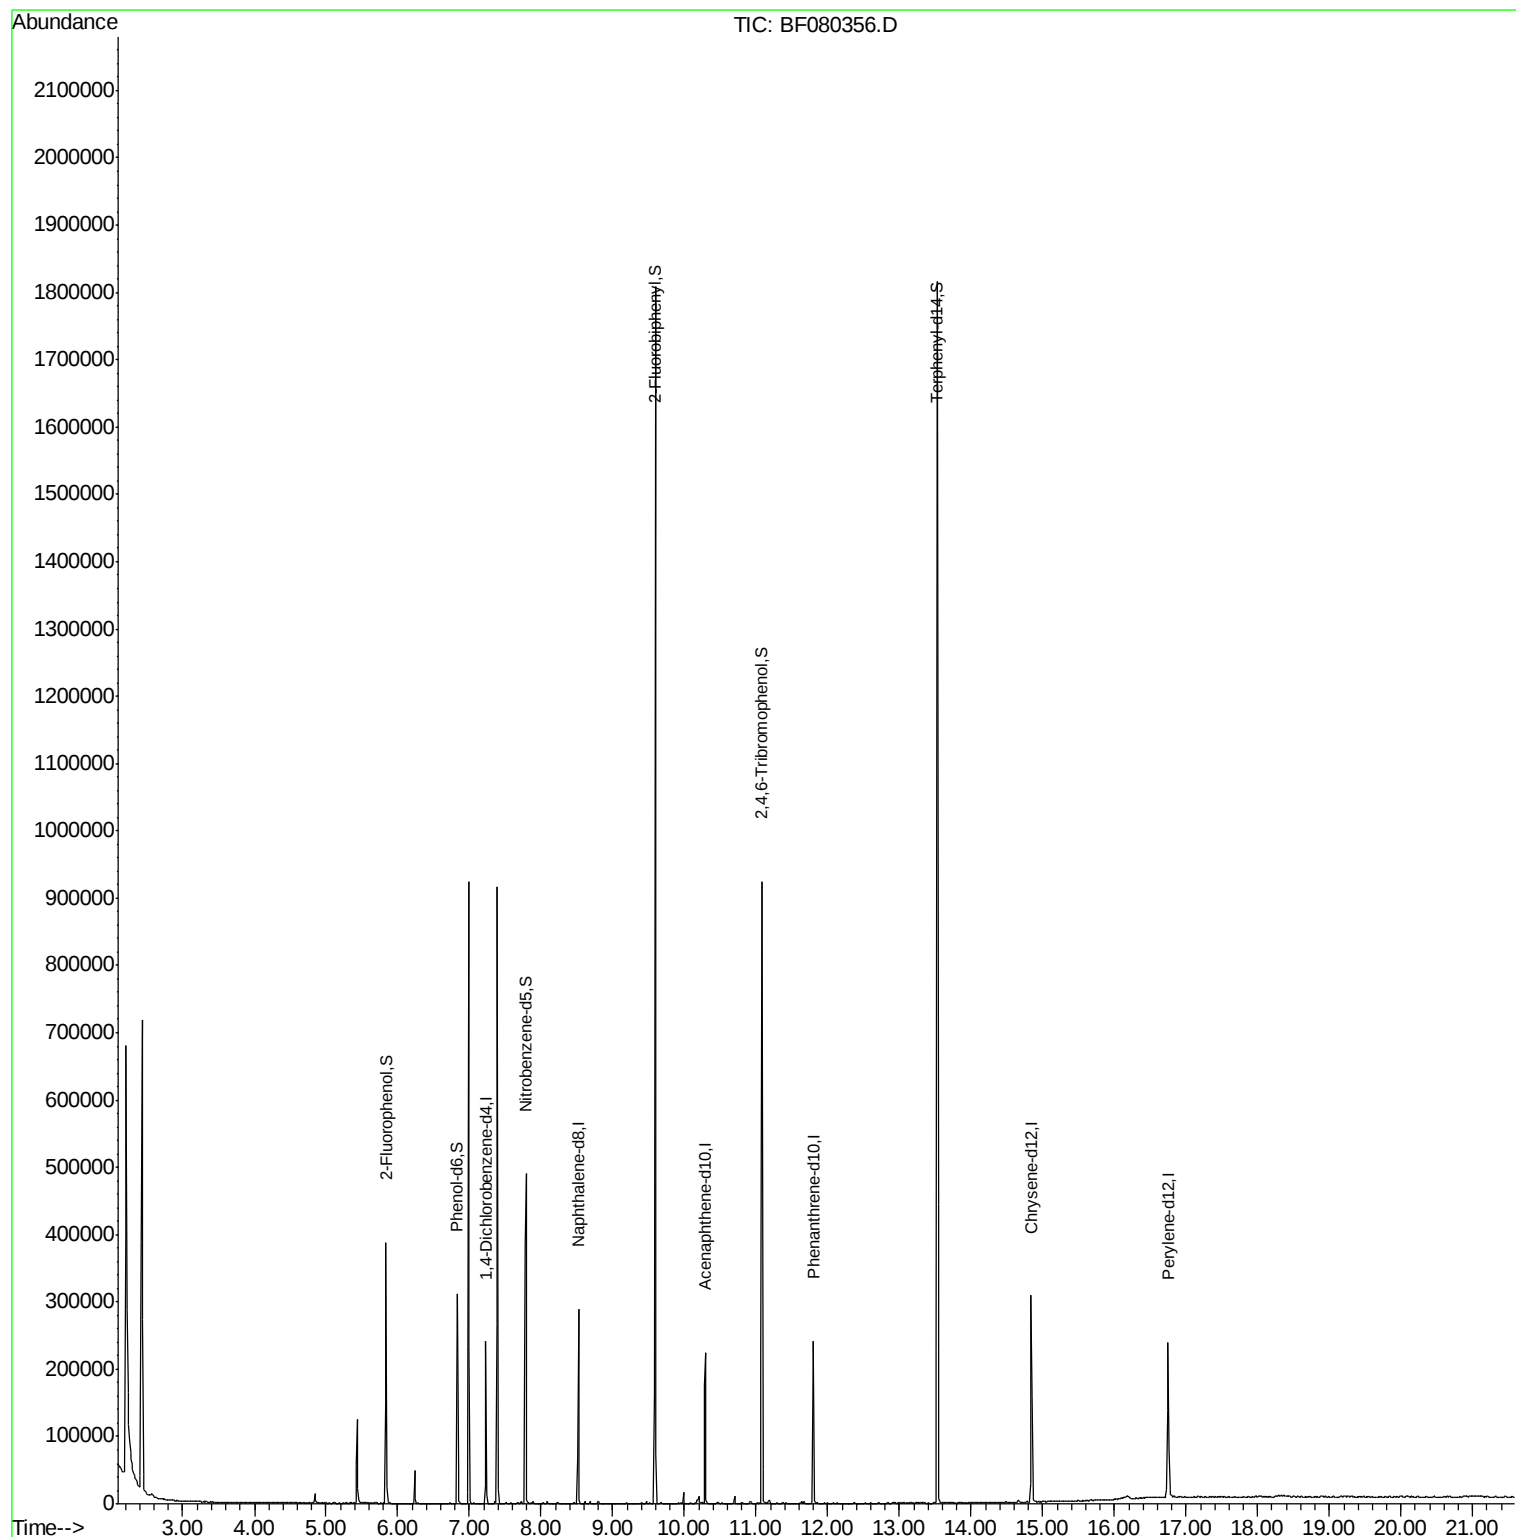


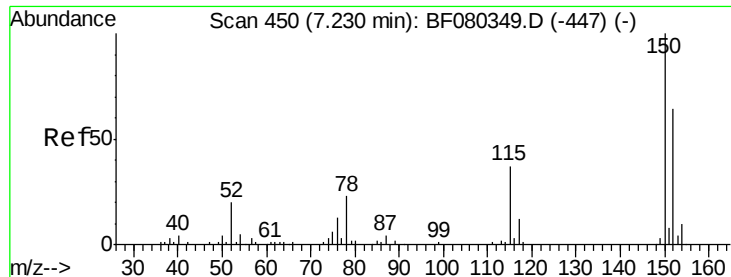

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.23 min Scan# 450
 Delta R.T. -0.00 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52




Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-152-7215


Tgt Ion:152 Resp: 34663
 Ion Ratio Lower Upper
 152 100
 150 150.5 124.7 187.1
 115 51.5 45.7 68.5

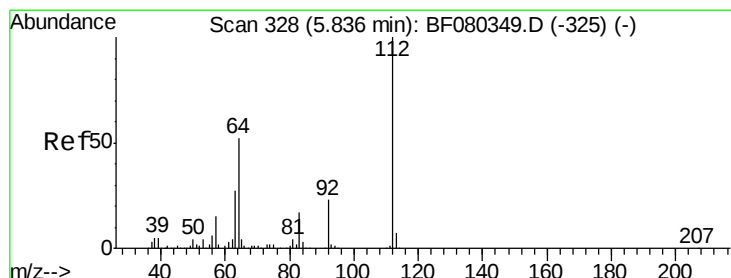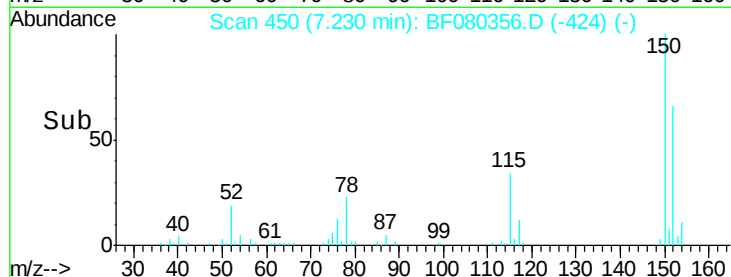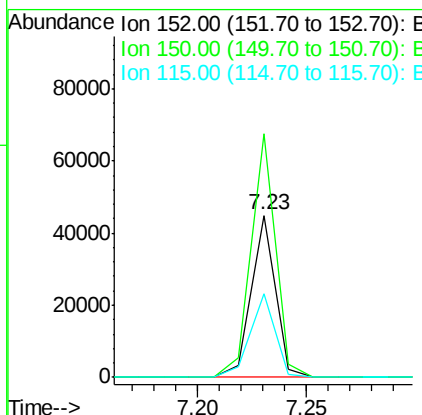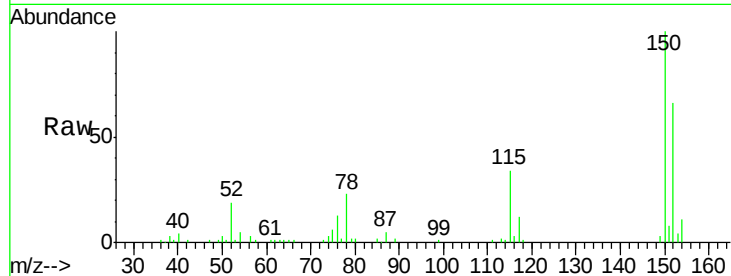

#5
 2-Fluorophenol
 Concen: 59.72 ng
 RT: 5.84 min Scan# 328
 Delta R.T. -0.00 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52

Tgt Ion:112 Resp: 113023
 Ion Ratio Lower Upper
 112 100
 64 54.2 41.8 62.6
 63 26.9 21.5 32.3

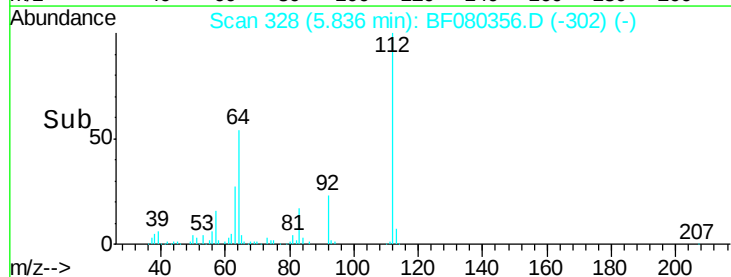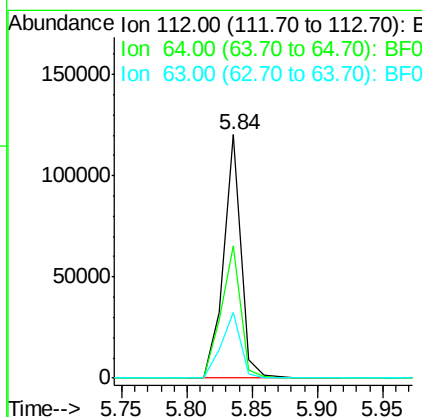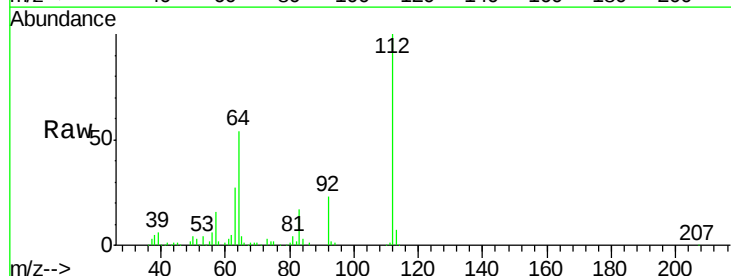

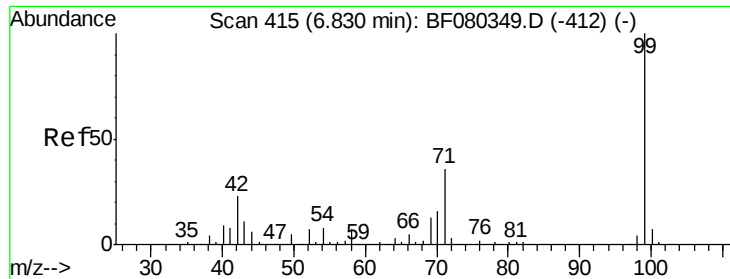

#7

Phenol-d6

Concen: 37.50 ng

RT: 6.83 min Scan# 415

Delta R.T. -0.00 min

Lab File: BF080356.D

Acq: 6 Jul 2015 20:52

Instrument :

BNA_F

ClientSampleId :

DCW-WW-152-7215


Tgt Ion: 99 Resp: 94081

Ion Ratio Lower Upper

99 100

42 19.7 18.5 27.7




71 32.7 28.5 42.7

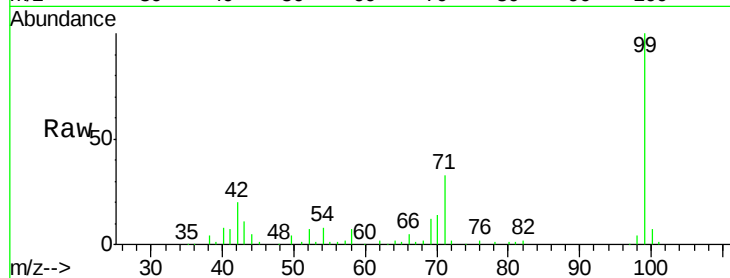

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

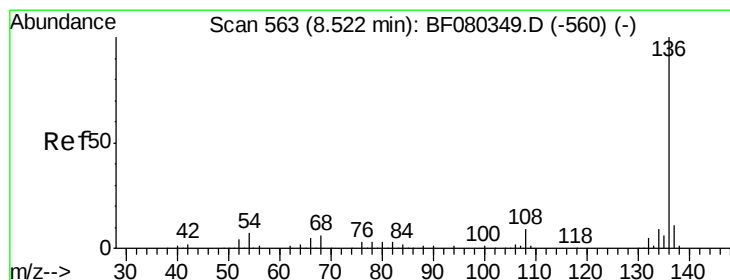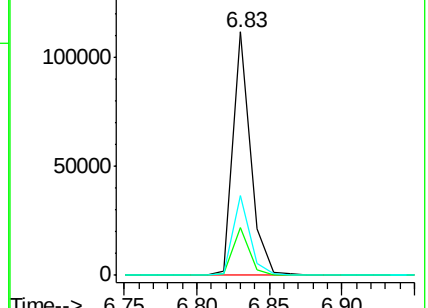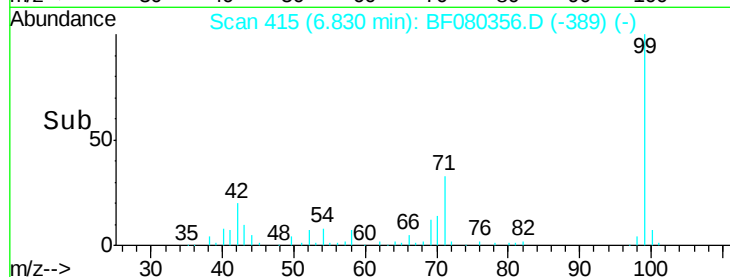

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.52 min Scan# 563

Delta R.T. -0.00 min

Lab File: BF080356.D

Acq: 6 Jul 2015 20:52

Tgt Ion: 136 Resp: 125625


Ion Ratio Lower Upper

136 100

137 10.6 8.5 12.7

54 6.5 5.8 8.8

68 5.1 4.6 6.8


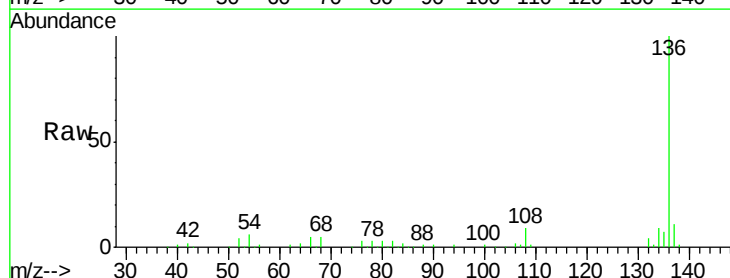



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

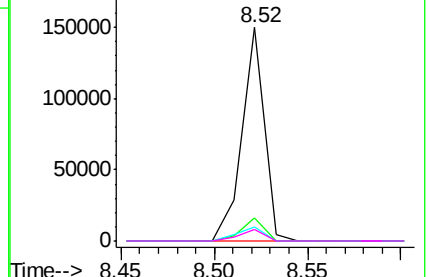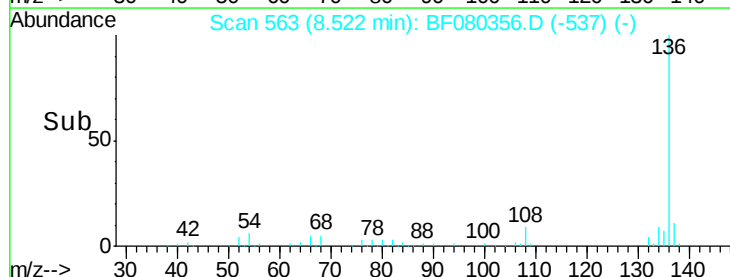


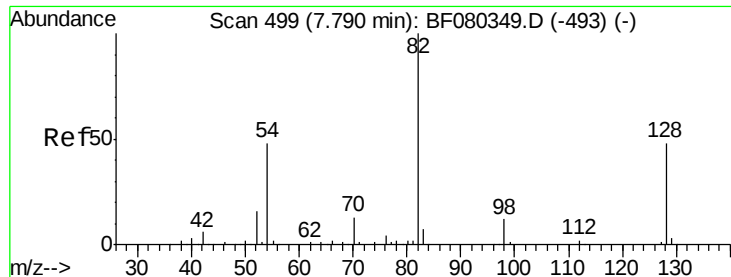




#23
 Nitrobenzene-d5
 Concen: 97.35 ng
 RT: 7.79 min Scan# 499
 Delta R.T. -0.00 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-152-7215

Tgt Ion: 82 Resp: 209670
 Ion Ratio Lower Upper
 82 100
 128 51.9 38.4 57.6
 54 44.7 38.2 57.2

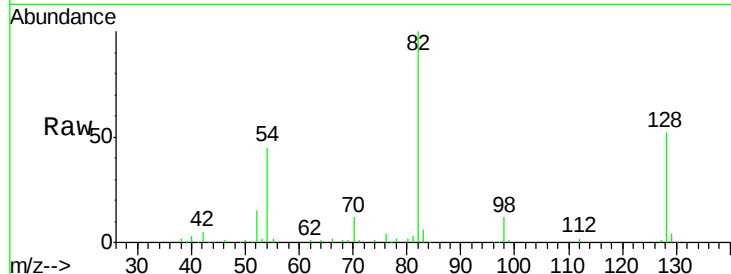


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

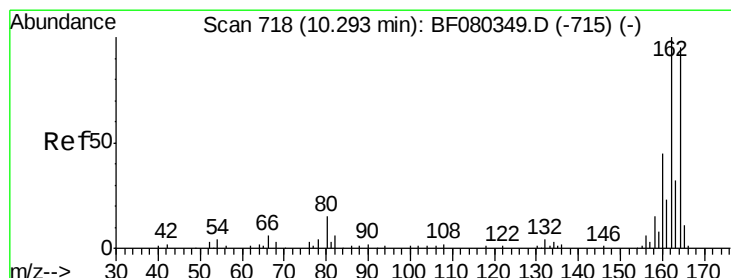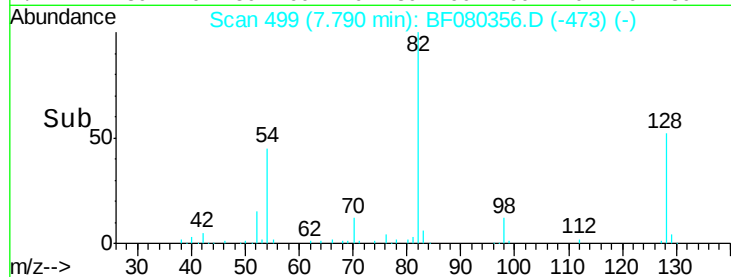
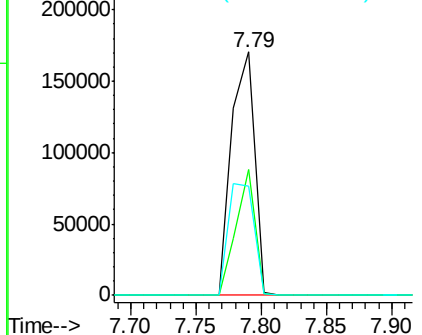



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.29 min Scan# 718
 Delta R.T. -0.00 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52

Tgt Ion: 164 Resp: 59724
 Ion Ratio Lower Upper
 164 100
 162 103.7 84.5 126.7
 160 47.6 37.7 56.5

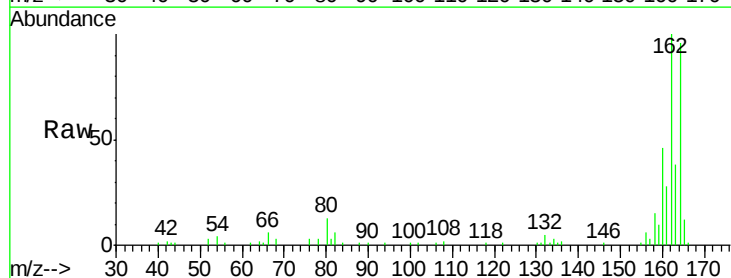

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



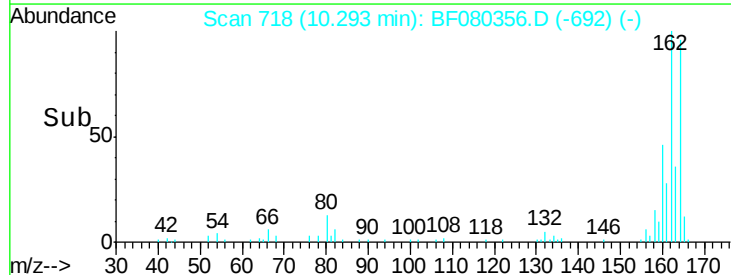
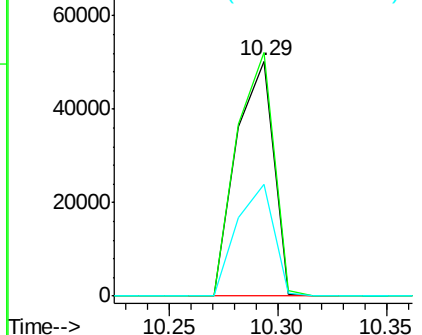


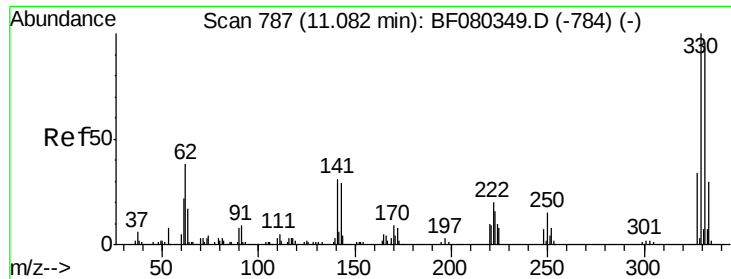

#41
 2,4,6-Tribromophenol
 Concen: 160.10 ng
 RT: 11.08 min Scan# 787
 Delta R.T. -0.00 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52




Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-152-7215


Tgt Ion:330 Resp: 100049
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.0 115.4
 141 36.1 29.6 44.4

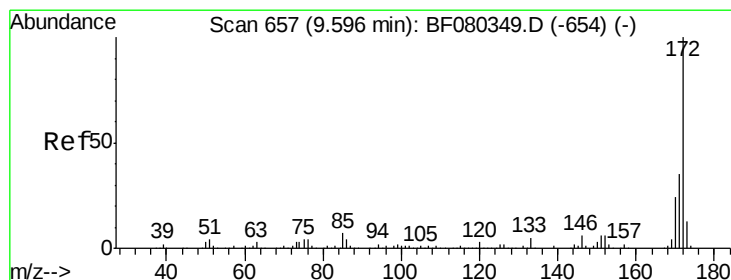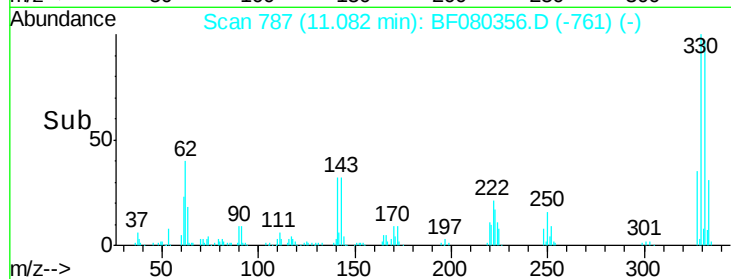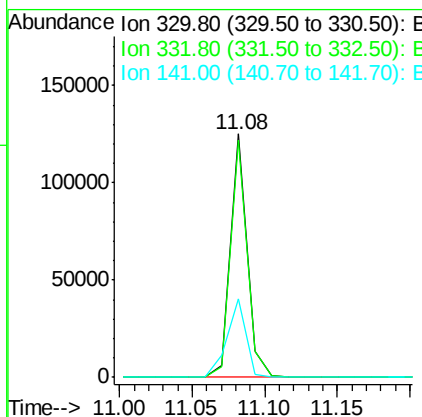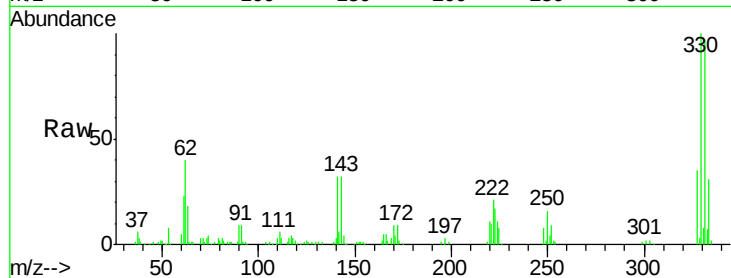

#44
 2-Fluorobiphenyl
 Concen: 109.57 ng
 RT: 9.60 min Scan# 657
 Delta R.T. -0.00 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52

Tgt Ion:172 Resp: 484917
 Ion Ratio Lower Upper
 172 100
 171 35.6 28.3 42.5
 170 24.3 19.1 28.7

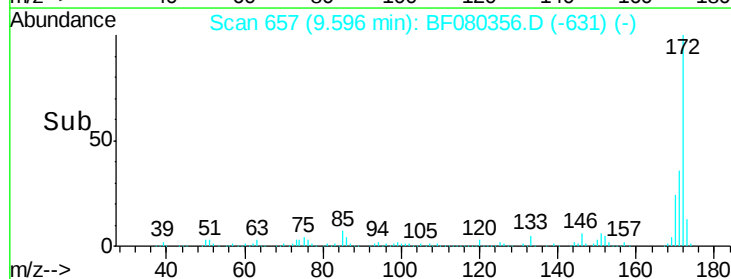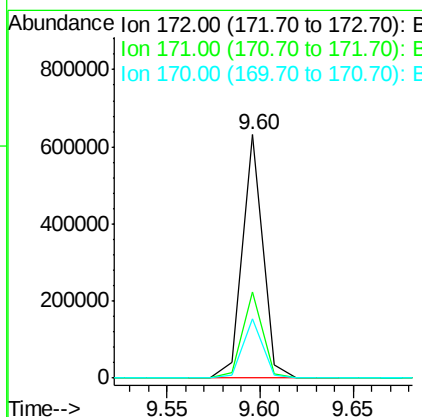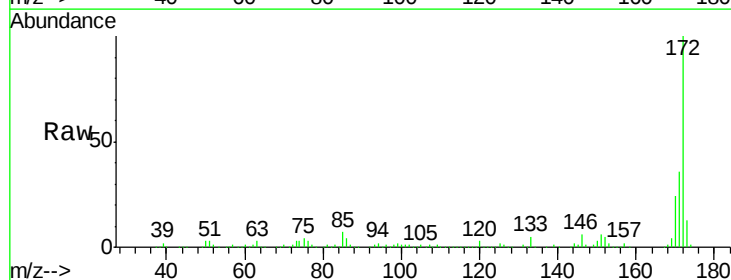


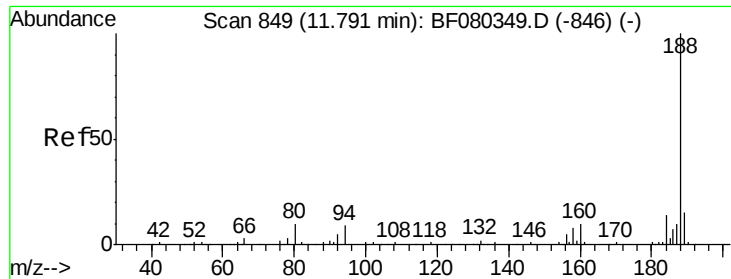




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.80 min Scan# 850
Delta R.T. 0.01 min
Lab File: BF080356.D
Acq: 6 Jul 2015 20:52

Instrument :
BNA_F
ClientSampleId :
DCW-WW-152-7215

Tgt Ion:188 Resp: 128189
Ion Ratio Lower Upper
188 100
94 6.2 7.5 11.3#
80 6.3 8.3 12.5#

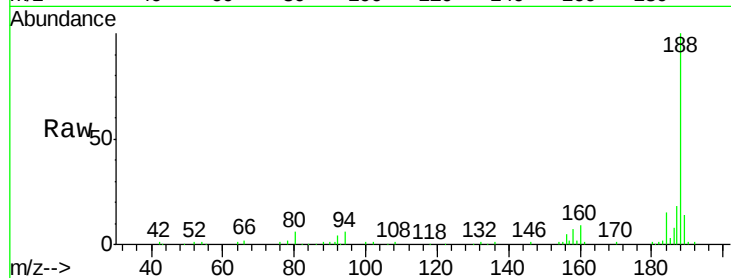


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

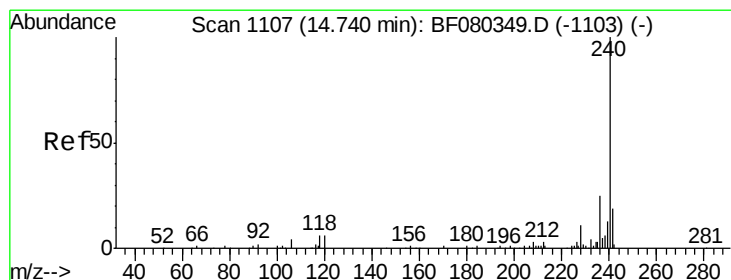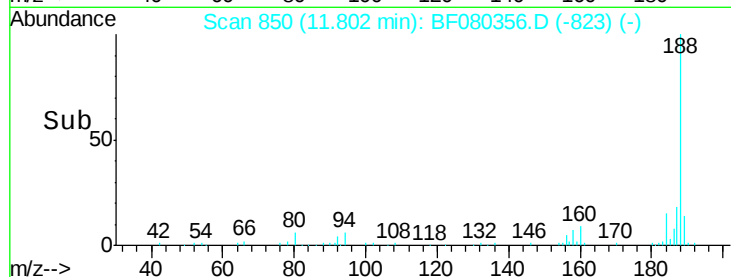
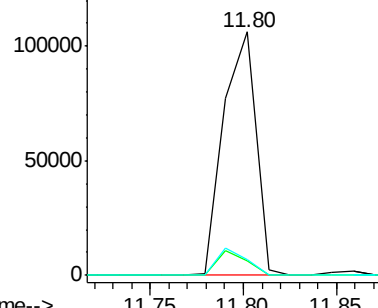



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.84 min Scan# 1116
Delta R.T. 0.10 min
Lab File: BF080356.D
Acq: 6 Jul 2015 20:52

Tgt Ion:240 Resp: 141100
Ion Ratio Lower Upper
240 100
120 11.8 5.1 7.7#
236 25.4 20.4 30.6

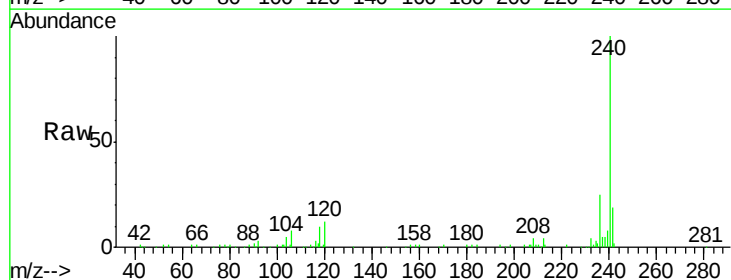

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



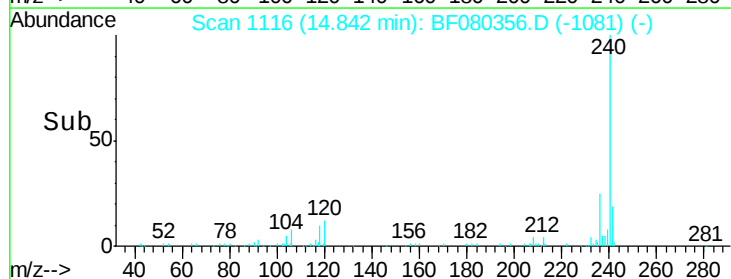
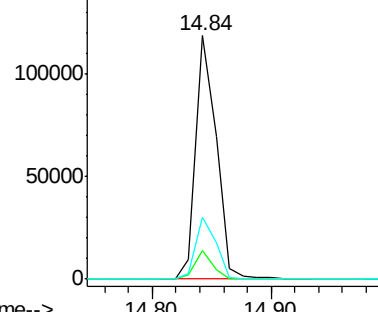


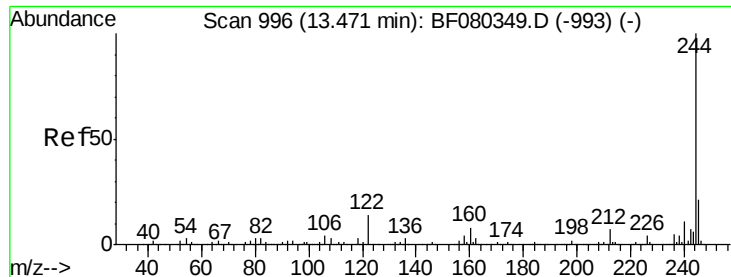

#78
 Terphenyl-d14
 Concen: 100.56 ng
 RT: 13.53 min Scan# 1001
 Delta R.T. 0.06 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-152-7215

Tgt Ion:244 Resp: 608310
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.8 8.8
 122 12.8 11.1 16.7

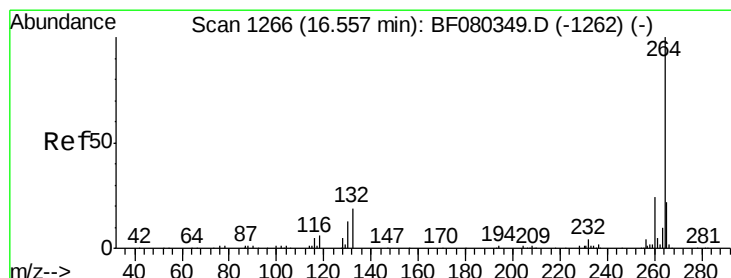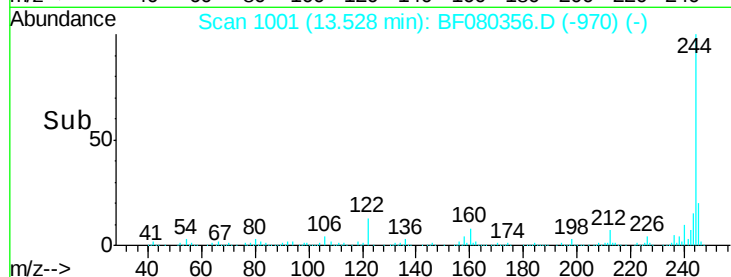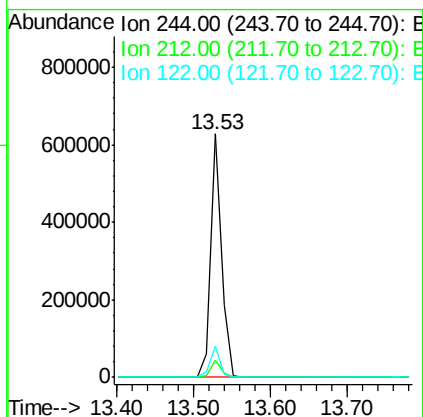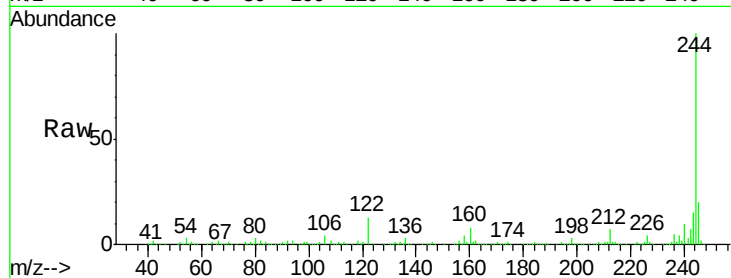

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 16.75 min Scan# 1283
 Delta R.T. 0.19 min
 Lab File: BF080356.D
 Acq: 6 Jul 2015 20:52

Tgt Ion:264 Resp: 129558
 Ion Ratio Lower Upper
 264 100
 260 22.8 19.2 28.8
 265 21.1 17.6 26.4

