

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070615\
 Data File : BF080357.D
 Acq On : 6 Jul 2015 21:21
 Operator : TP/IZ
 Sample : G2877-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-153-7215

Quant Time: Jul 07 05:17:32 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 03:05:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.23	152	36029	20.00	ng	0.00
21) Naphthalene-d8	8.52	136	132789	20.00	ng	0.00
38) Acenaphthene-d10	10.29	164	63758	20.00	ng	0.00
63) Phenanthrene-d10	11.79	188	148144	20.00	ng	0.00
75) Chrysene-d12	14.74	240	149196	20.00	ng	0.00
86) Perylene-d12	16.59	264	134372	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.84	112	109602	55.71	ng	0.00
7) Phenol-d6	6.83	99	90505	34.71	ng	0.00
23) Nitrobenzene-d5	7.79	82	195013	85.66	ng	0.00
41) 2,4,6-Tribromophenol	11.08	330	94755	142.03	ng	0.00
44) 2-Fluorobiphenyl	9.60	172	475104	100.56	ng	0.00
78) Terphenyl-d14	13.48	244	611448	95.59	ng	0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070615\
Data File : BF080357.D
Acq On : 6 Jul 2015 21:21
Operator : TP/IZ
Sample : G2877-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-153-7215

Quant Time: Jul 07 05:17:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 03:05:40 2015
Response via : Initial Calibration

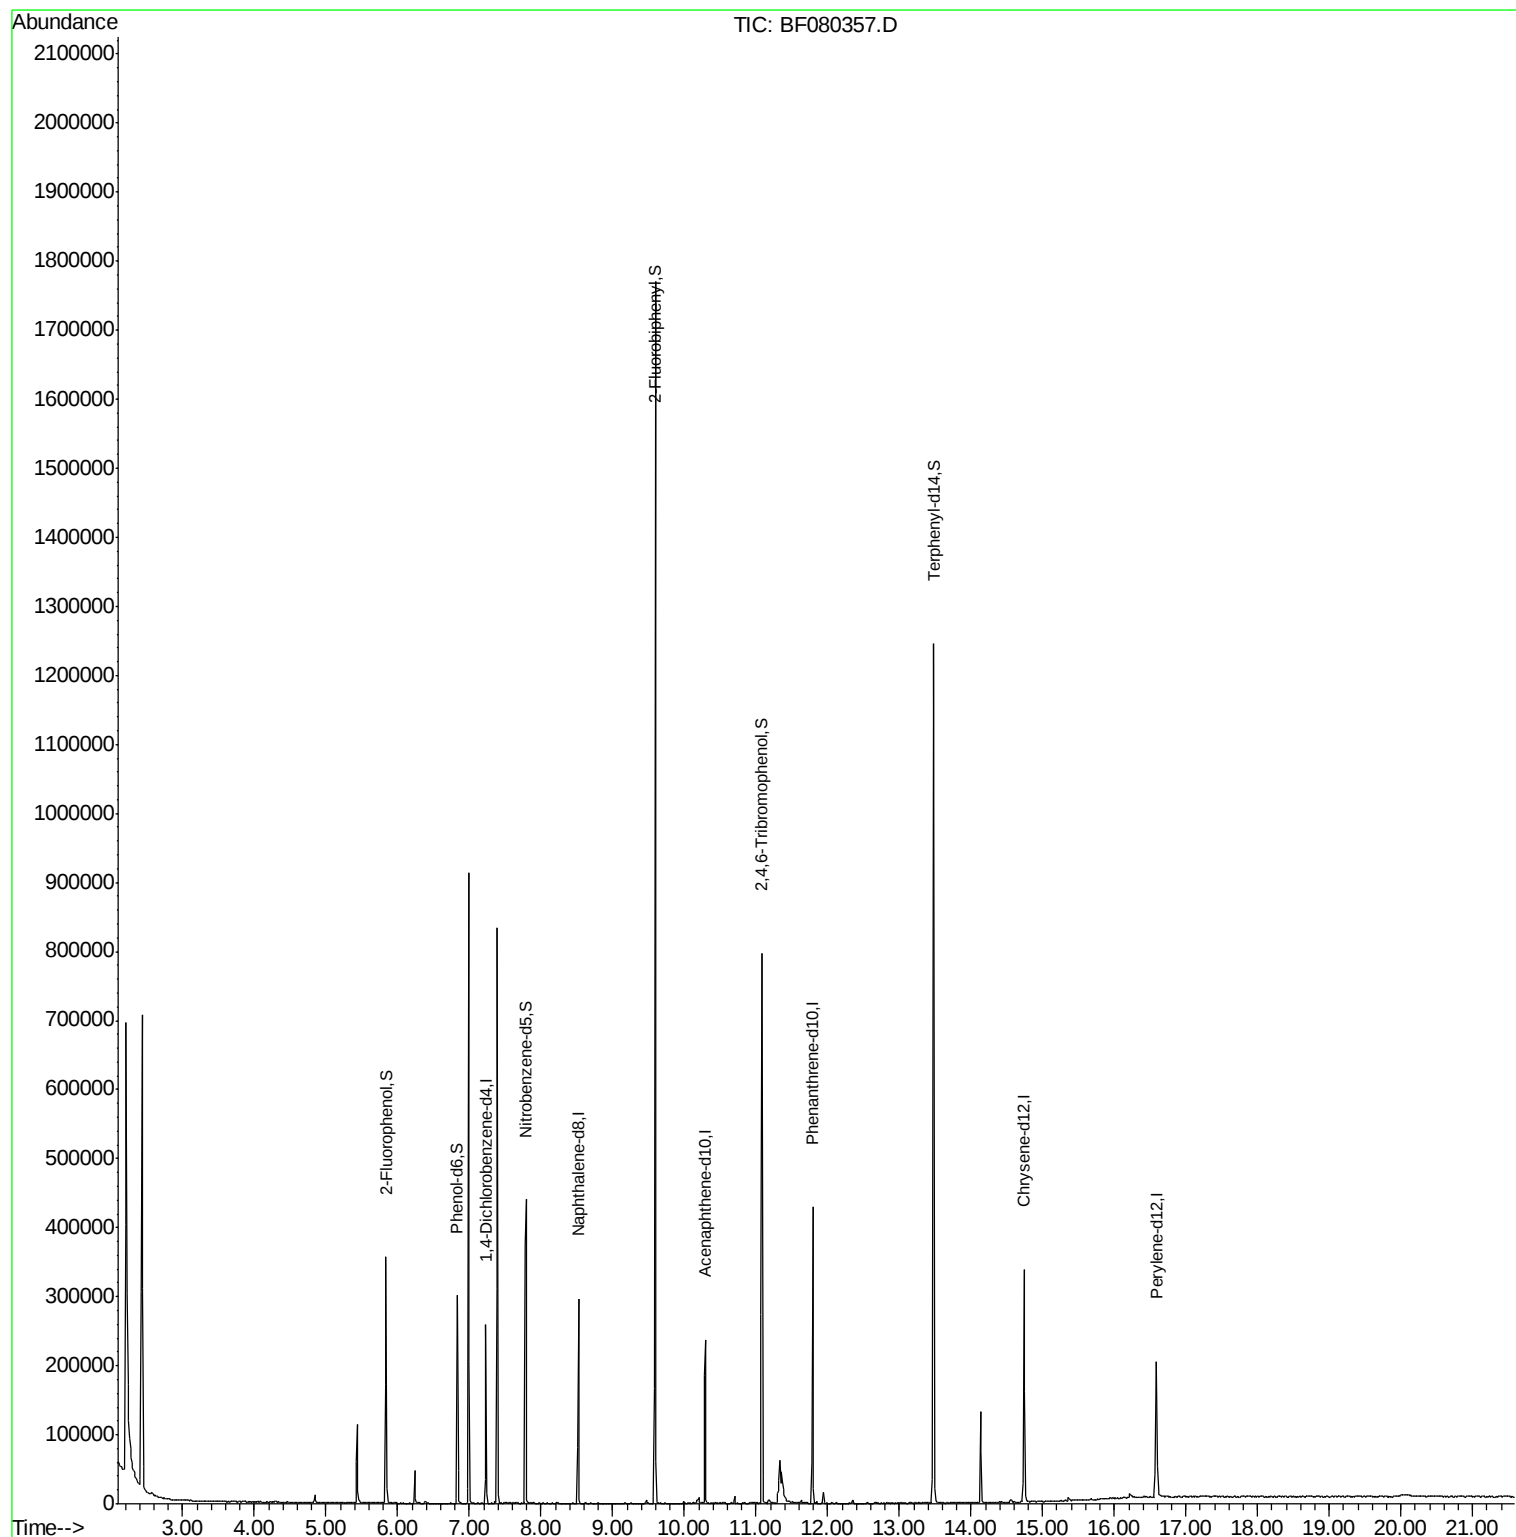




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.23 min Scan# 450
 Delta R.T. 0.00 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-153-7215

Tgt Ion:152 Resp: 36029
 Ion Ratio Lower Upper
 152 100
 150 158.8 124.7 187.1
 115 55.0 45.7 68.5

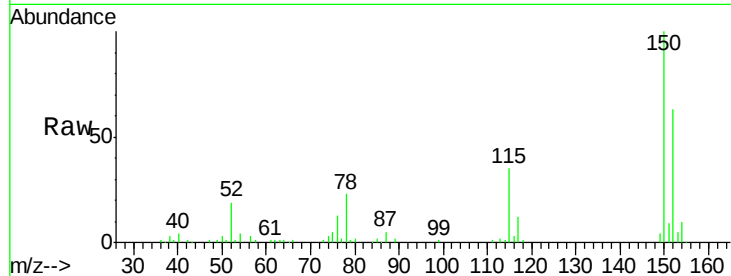


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

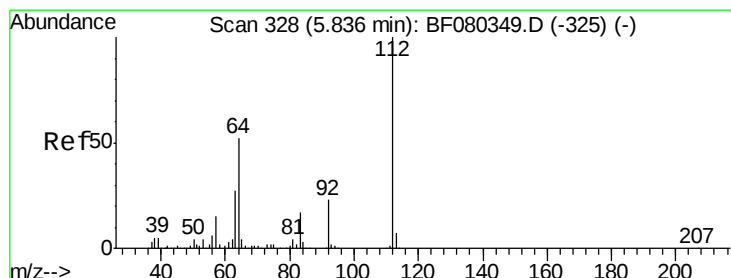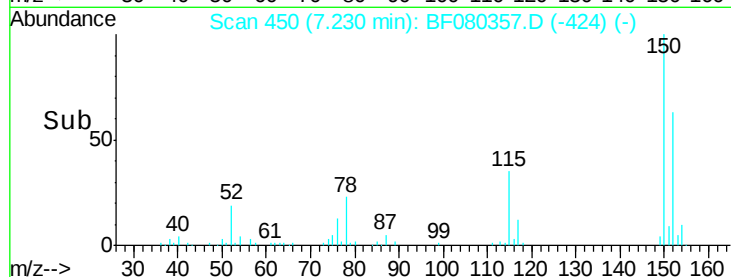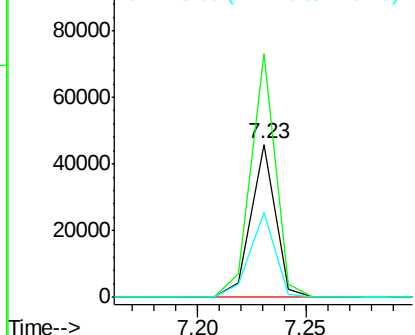



#5


2-Fluorophenol
 Concen: 55.71 ng
 RT: 5.84 min Scan# 328
 Delta R.T. 0.00 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Tgt Ion:112 Resp: 109602
 Ion Ratio Lower Upper
 112 100
 64 53.8 41.8 62.6
 63 26.6 21.5 32.3

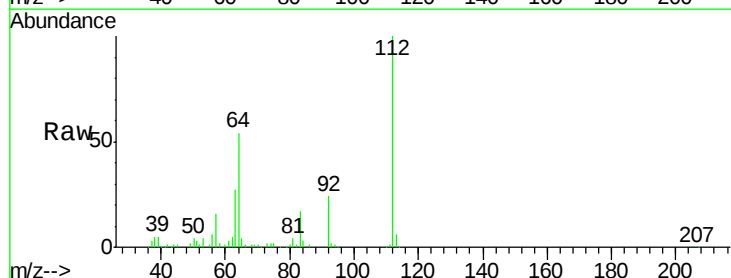

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

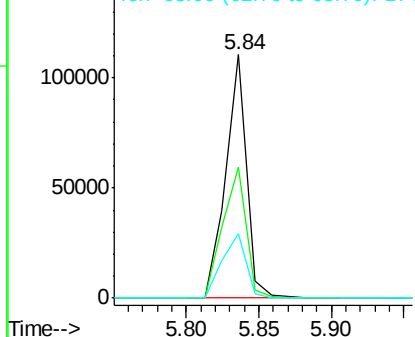



#7

Phenol-d6

Concen: 34.71 ng

RT: 6.83 min Scan# 415

Delta R.T. 0.00 min

Lab File: BF080357.D

Acq: 6 Jul 2015 21:21

Instrument :

BNA_F

ClientSampleId :

DCW-WW-153-7215


Tgt Ion: 99 Resp: 90505

Ion Ratio Lower Upper

99 100

42 19.2 18.5 27.7




71 32.3 28.5 42.7

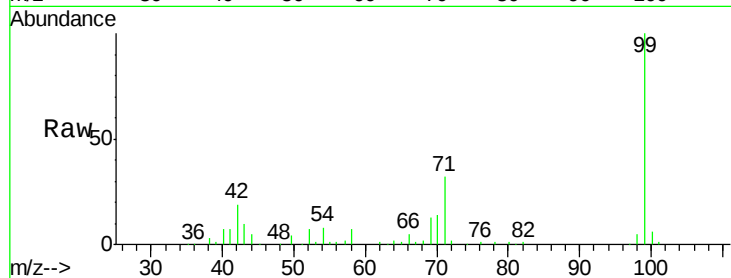

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

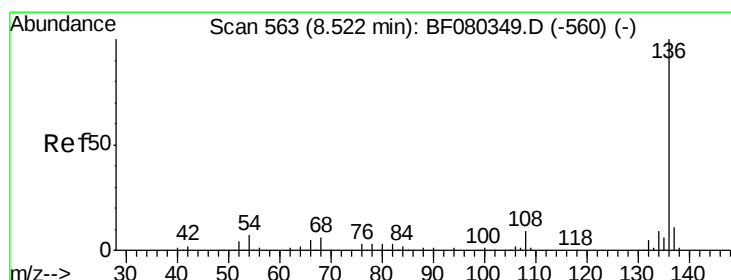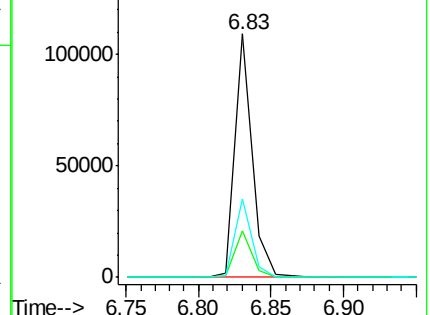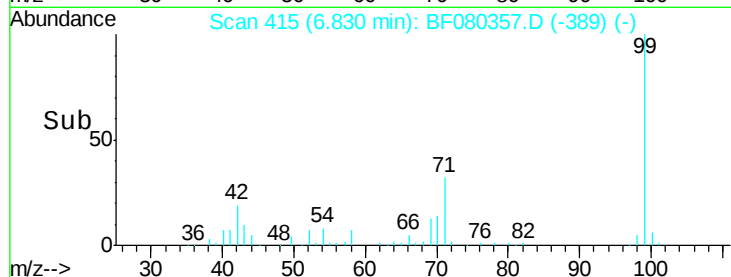

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.52 min Scan# 563

Delta R.T. 0.00 min

Lab File: BF080357.D

Acq: 6 Jul 2015 21:21

Tgt Ion: 136 Resp: 132789


Ion Ratio Lower Upper

136 100

137 10.4 8.5 12.7

54 6.5 5.8 8.8

68 4.8 4.6 6.8


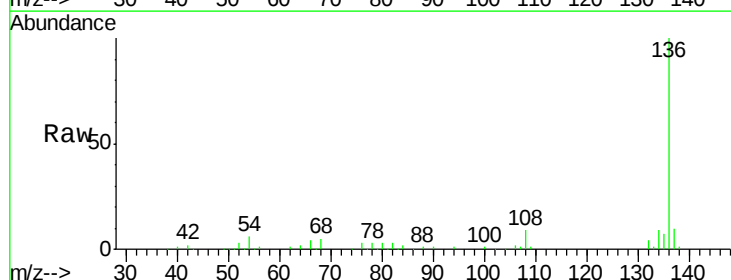



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

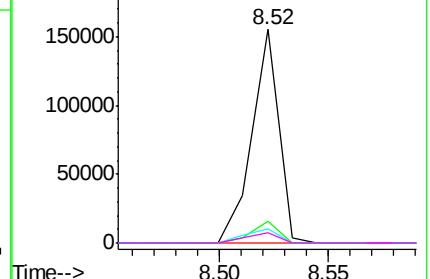


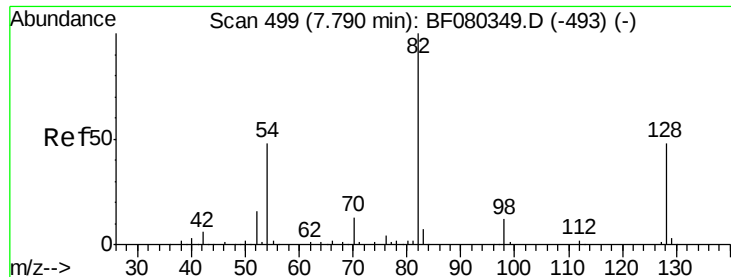




#23
 Nitrobenzene-d5
 Concen: 85.66 ng
 RT: 7.79 min Scan# 499
 Delta R.T. 0.00 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-153-7215

Tgt Ion: 82 Resp: 195013
 Ion Ratio Lower Upper
 82 100
 128 53.3 38.4 57.6
 54 44.2 38.2 57.2

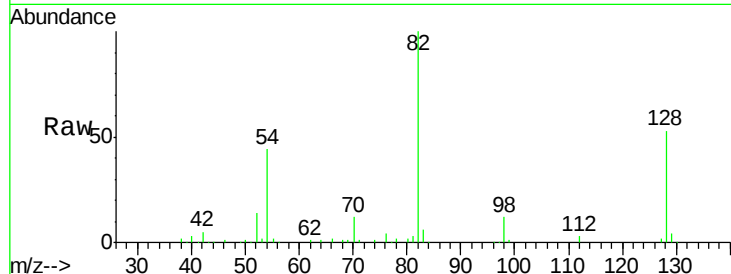


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

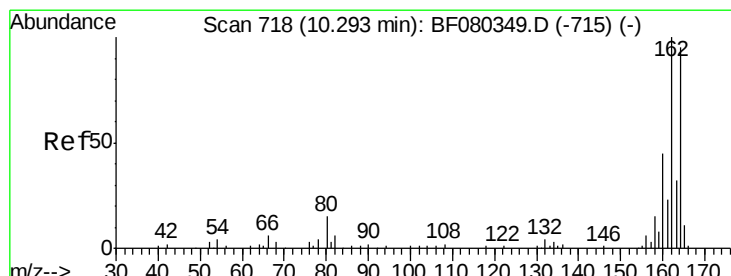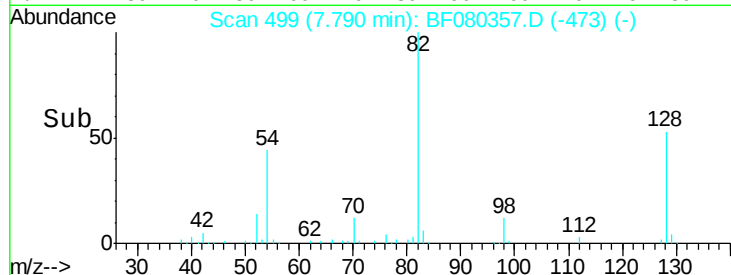
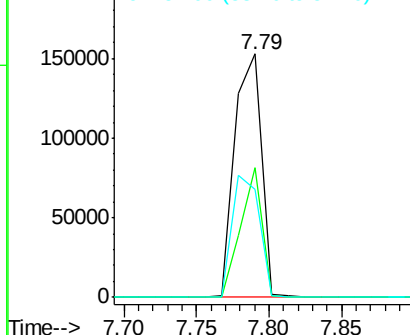



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.29 min Scan# 718
 Delta R.T. 0.00 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Tgt Ion: 164 Resp: 63758
 Ion Ratio Lower Upper
 164 100
 162 104.4 84.5 126.7
 160 46.8 37.7 56.5

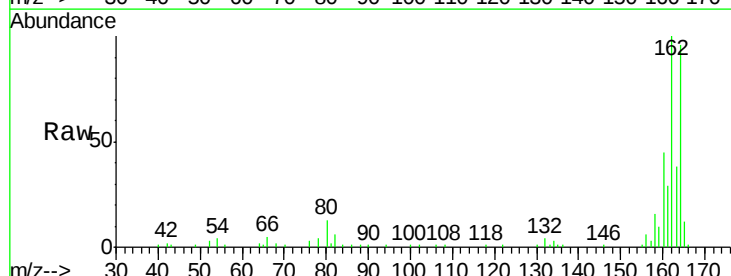

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E




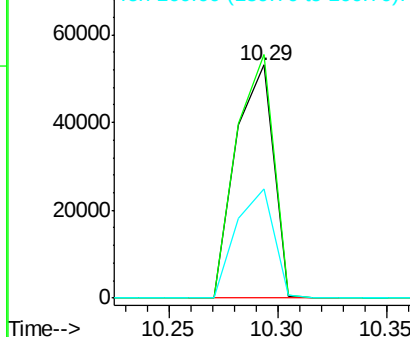




#41
 2,4,6-Tribromophenol
 Concen: 142.03 ng
 RT: 11.08 min Scan# 787
 Delta R.T. 0.00 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21




Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-153-7215


Tgt Ion:330 Resp: 94755
 Ion Ratio Lower Upper
 330 100
 332 95.6 77.0 115.4
 141 34.5 29.6 44.4

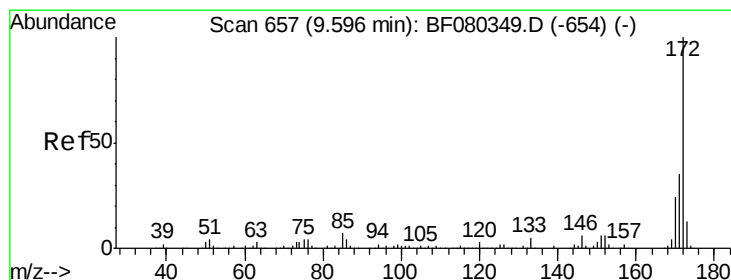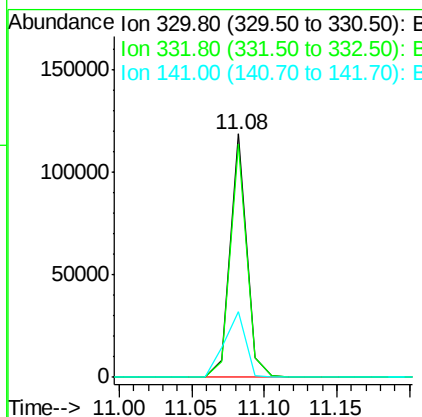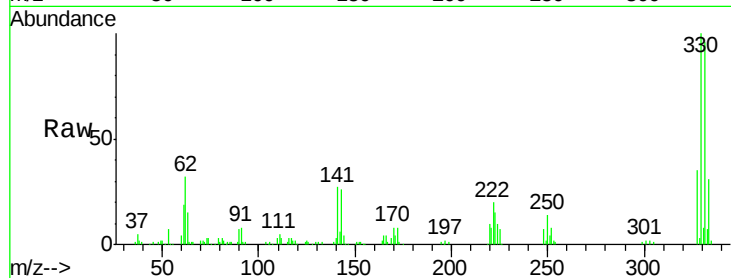

#44
 2-Fluorobiphenyl
 Concen: 100.56 ng
 RT: 9.60 min Scan# 657
 Delta R.T. 0.00 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Tgt Ion:172 Resp: 475104
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.3 42.5
 170 24.3 19.1 28.7

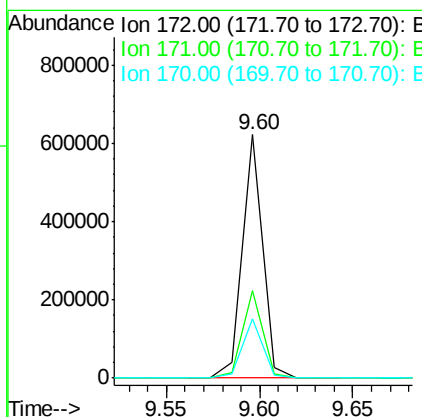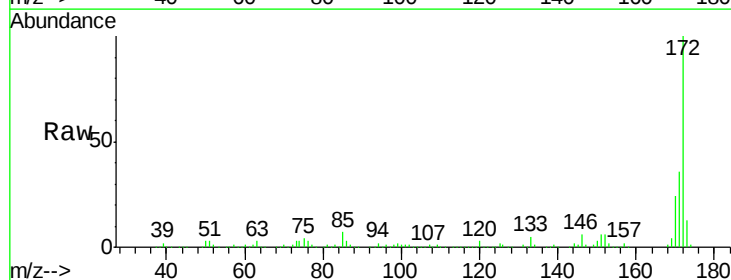







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.79 min Scan# 849
Delta R.T. 0.00 min
Lab File: BF080357.D
Acq: 6 Jul 2015 21:21

Instrument :
BNA_F
ClientSampleId :
DCW-WW-153-7215

Tgt Ion:188 Resp: 148144
Ion Ratio Lower Upper
188 100
94 8.0 7.5 11.3
80 8.5 8.3 12.5

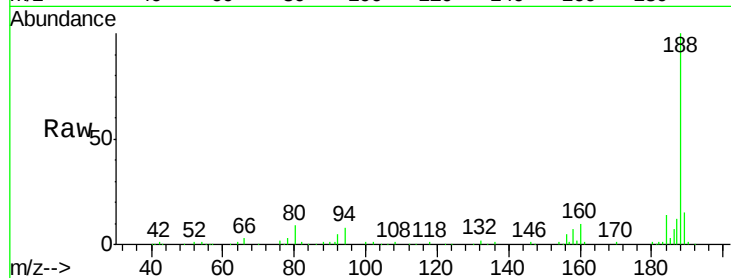


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

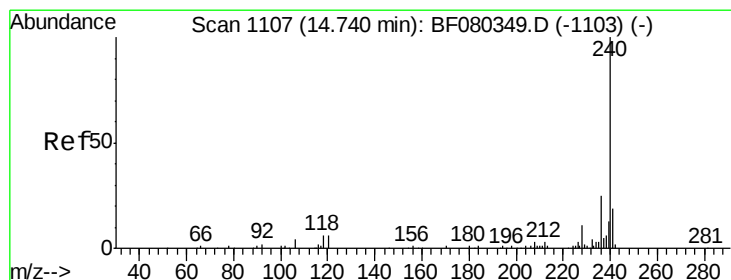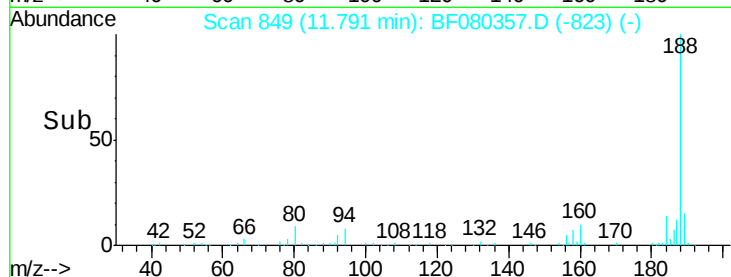
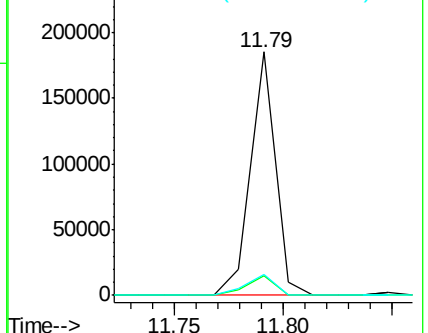



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.74 min Scan# 1107
Delta R.T. 0.00 min
Lab File: BF080357.D
Acq: 6 Jul 2015 21:21

Tgt Ion:240 Resp: 149196
Ion Ratio Lower Upper
240 100
120 12.1 5.1 7.7#
236 25.9 20.4 30.6

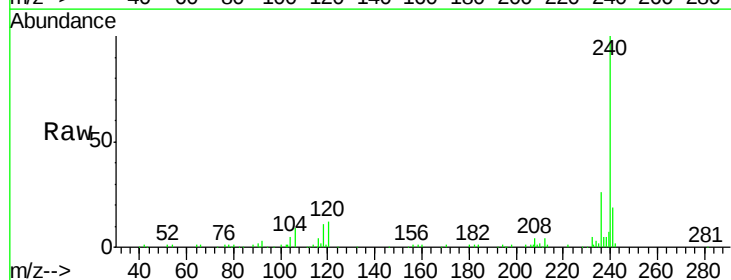

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




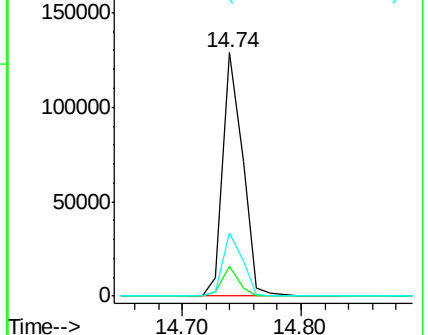




#78
 Terphenyl-d14
 Concen: 95.59 ng
 RT: 13.48 min Scan# 997
 Delta R.T. 0.01 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-153-7215

Tgt Ion:244 Resp: 611448
 Ion Ratio Lower Upper
 244 100
 212 6.2 5.8 8.8
 122 6.3 11.1 16.7#

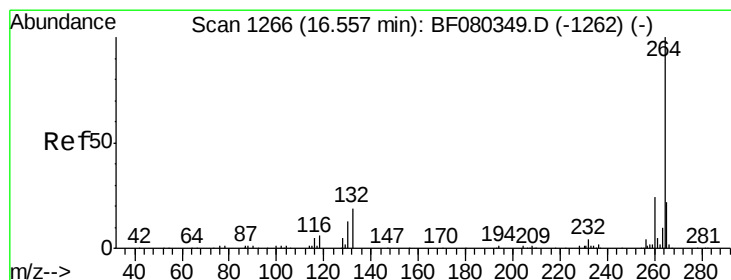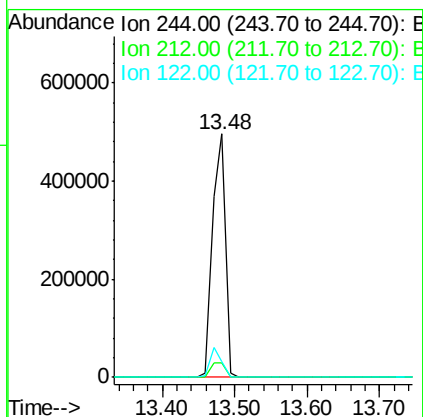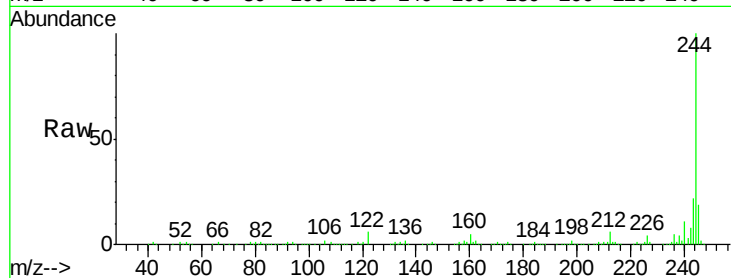

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 16.59 min Scan# 1269
 Delta R.T. 0.03 min
 Lab File: BF080357.D
 Acq: 6 Jul 2015 21:21

Tgt Ion:264 Resp: 134372
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.2 28.8
 265 21.2 17.6 26.4

