


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070615\
 Data File : BF080361.D
 Acq On : 7 Jul 2015 00:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 03:05:40 2015

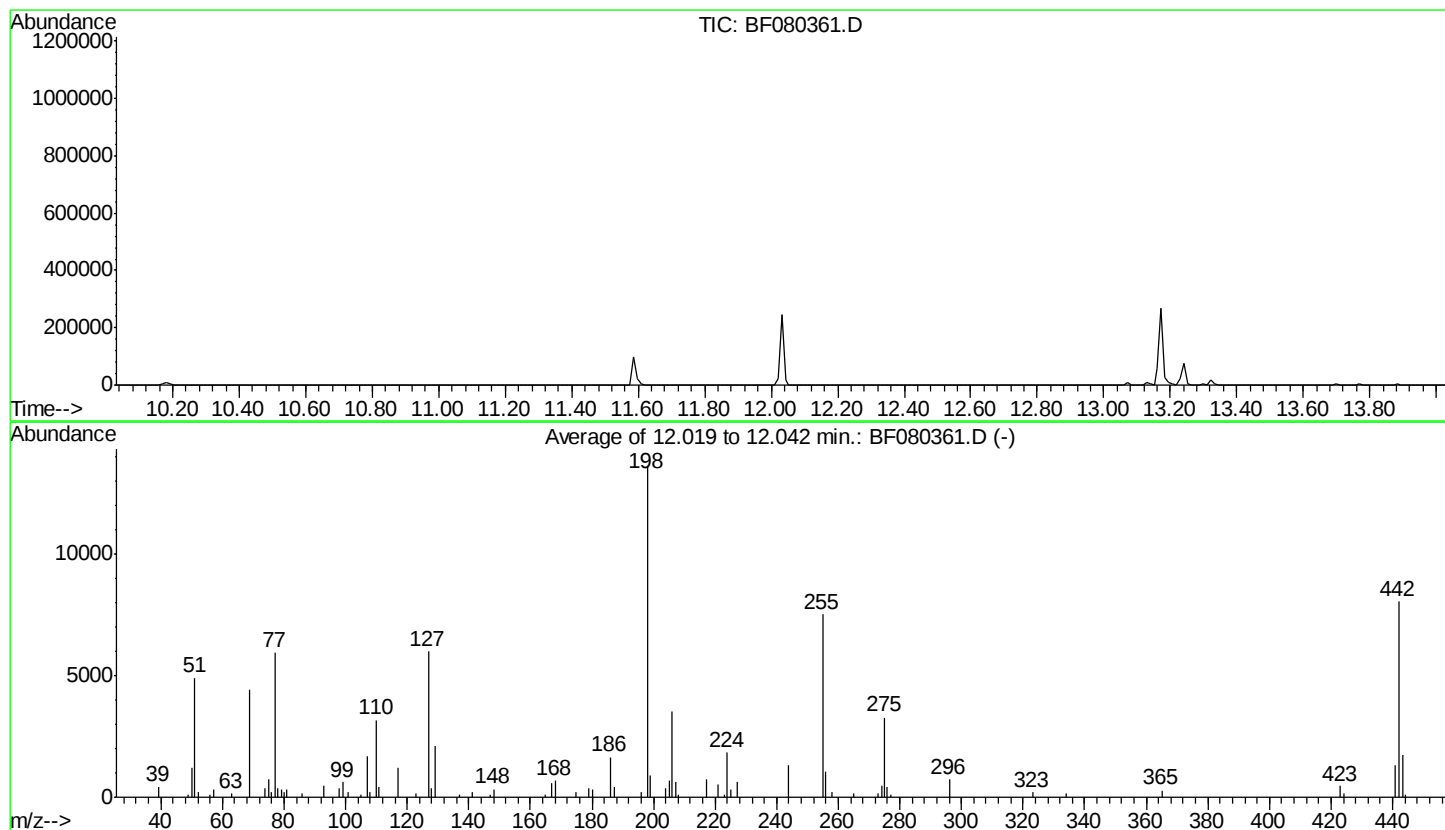

AutoFind: Scans 869, 870, 871; Background Corrected with Scan 866

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	4900	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	4418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	5990	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13641	PASS
199	198	5	9	6.5	887	PASS
275	198	10	60	24.1	3284	PASS
365	198	1	100	2.1	281	PASS
441	442	0.01	24	16.1	1292	PASS
442	198	50	100	59.0	8045	PASS
443	442	15	24	21.3	1717	PASS