

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070616\
 Data File : BF088747.D
 Acq On : 6 Jul 2016 21:29
 Operator : UM/SJ
 Sample : H3880-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 C2.2-06

Quant Time: Jul 07 01:06:39 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 05 17:15:08 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	86078	20.00	ng	-0.03
21) Naphthalene-d8	8.03	136	390039	20.00	ng	-0.03
38) Acenaphthene-d10	9.78	164	183839	20.00	ng	-0.03
63) Phenanthrene-d10	11.26	188	378146	20.00	ng	-0.03
75) Chrysene-d12	13.87	240	293335	20.00	ng	-0.05
86) Perylene-d12	15.26	264	236383	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	505258	87.97	ng	-0.03
7) Phenol-d6	6.39	99	760955	102.54	ng	-0.02
23) Nitrobenzene-d5	7.31	82	473925	63.68	ng	-0.03
41) 2,4,6-Tribromophenol	10.56	330	135140	79.16	ng	-0.05
44) 2-Fluorobiphenyl	9.11	172	656991	56.45	ng	-0.03
78) Terphenyl-d14	12.83	244	728172	55.29	ng	-0.03
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.31	70	63560	12.75	ng	# 70
49) Dimethylphthalate	9.51	163	115040	8.78	ng	98
56) 2,4-Dinitrotoluene	9.78	165	23373	6.16	ng	# 38
66) 4-Bromophenyl-phenylether	10.56	248	8677	2.28	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070616\
Data File : BF088747.D
Acq On : 6 Jul 2016 21:29
Operator : UM/SJ
Sample : H3880-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C2.2-06

Quant Time: Jul 07 01:06:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

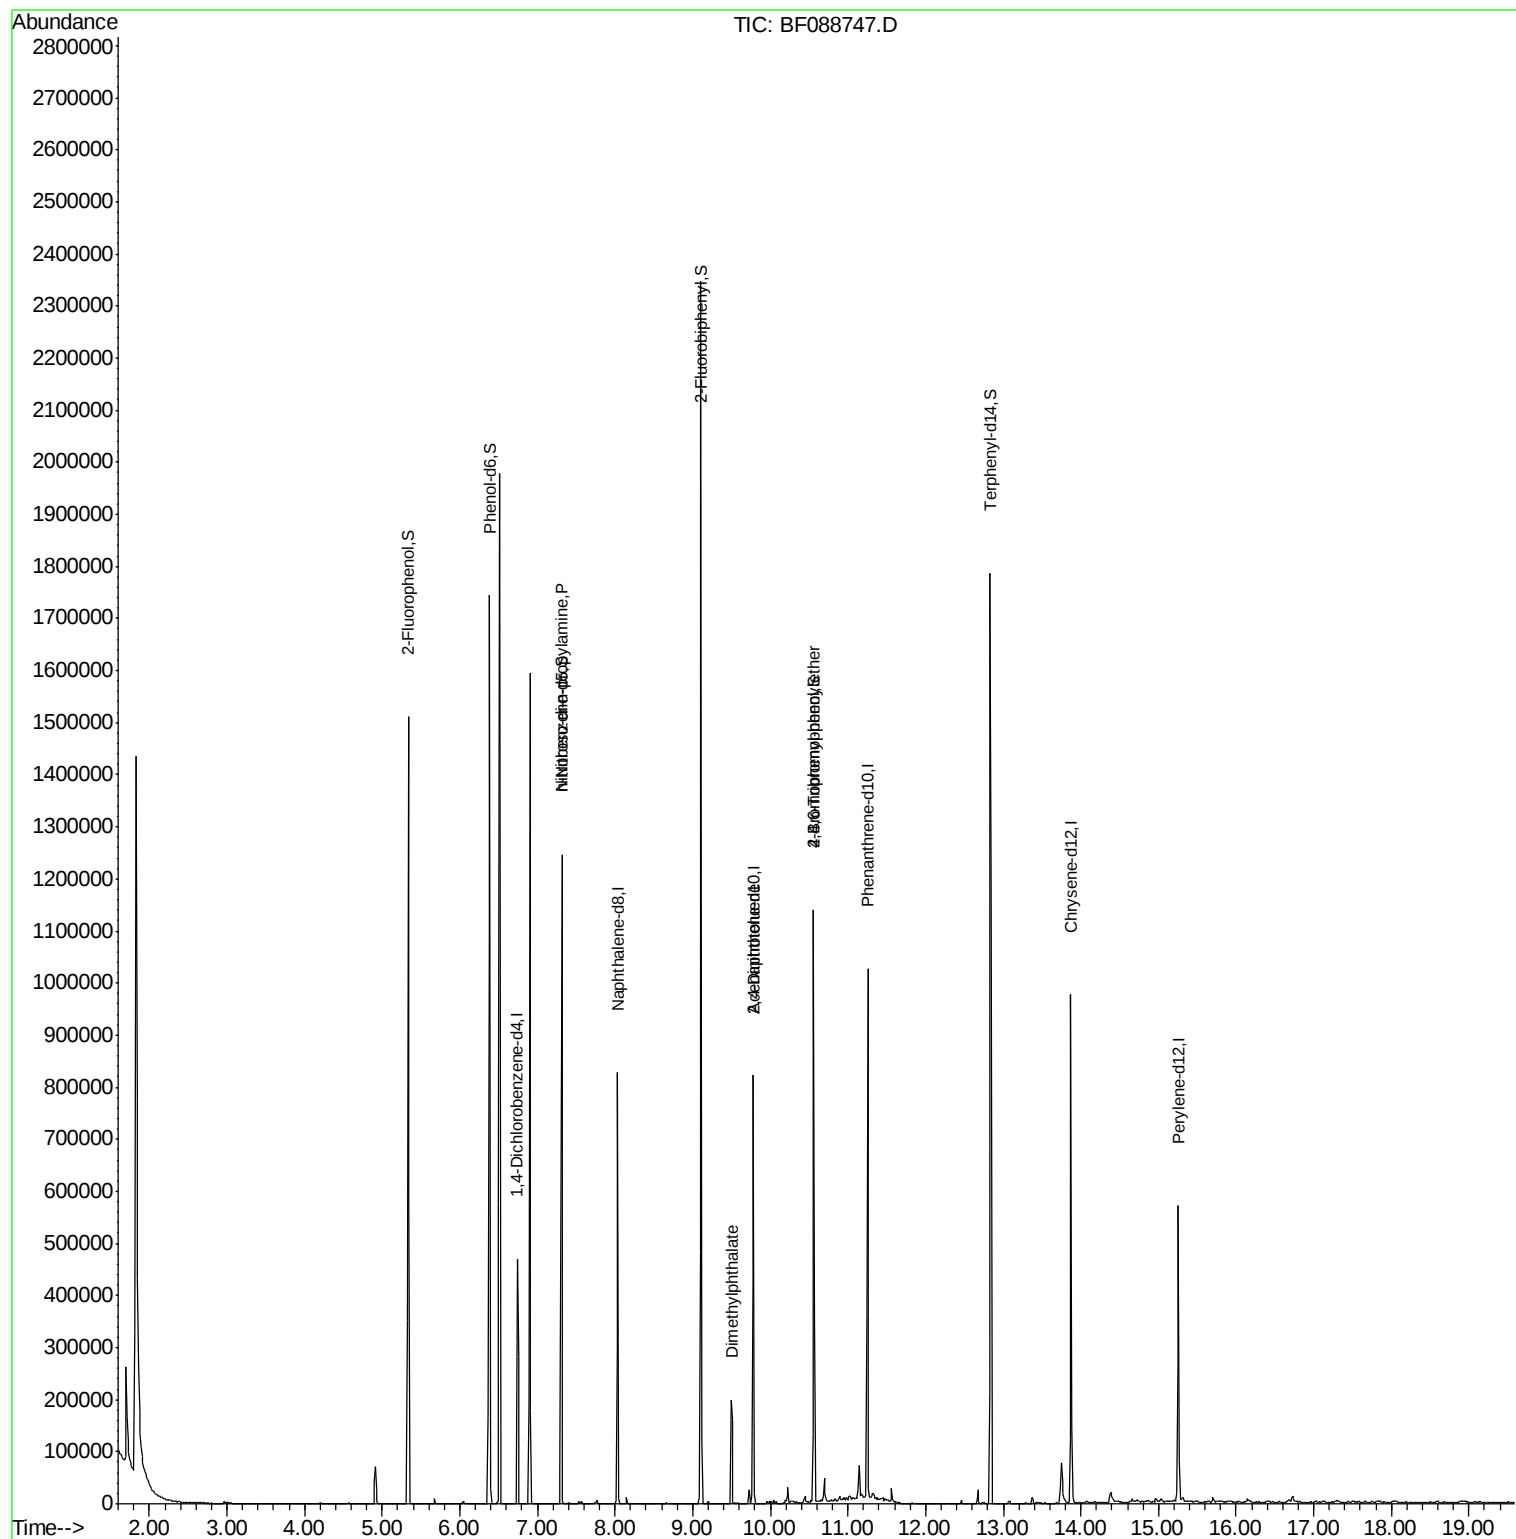



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 451

Delta R.T. -0.03 min

Lab File: BF088747.D

Acq: 6 Jul 2016 21:29

Instrument :

BNA_F

ClientSampleId :

C2.2-06


Tgt Ion:152 Resp: 86078

Ion Ratio Lower Upper

152 100

150 160.5 123.8 185.6




115 76.8 39.6 59.4#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

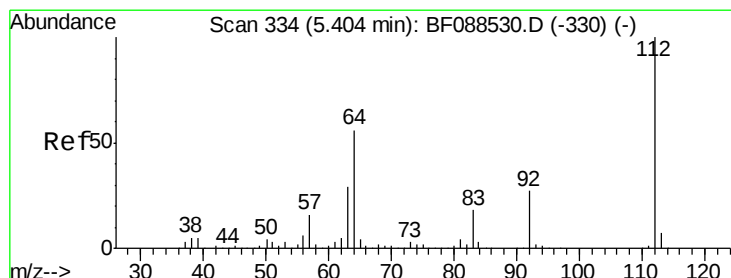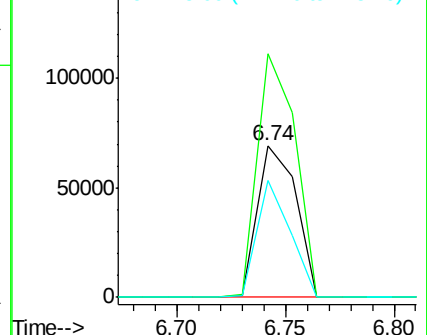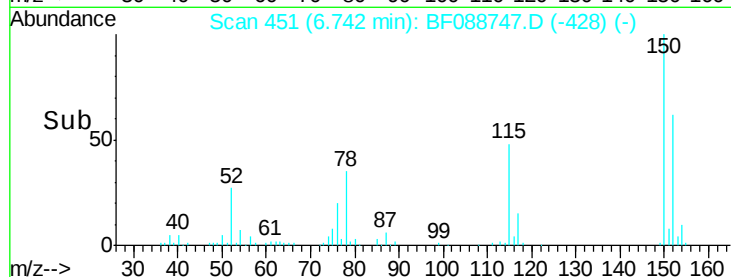

#5

2-Fluorophenol

Concen: 87.97 ng

RT: 5.34 min Scan# 328

Delta R.T. -0.03 min

Lab File: BF088747.D

Acq: 6 Jul 2016 21:29


Tgt Ion:112 Resp: 505258

Ion Ratio Lower Upper

112 100

64 61.4 42.2 63.2



63 32.2 21.8 32.8



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

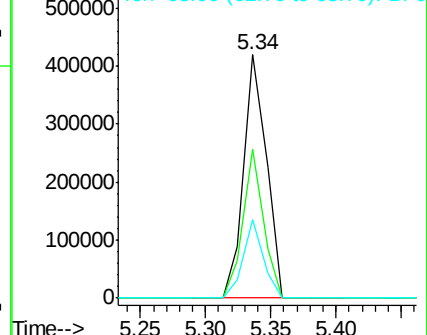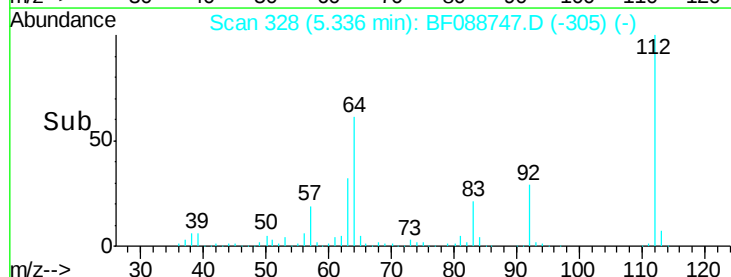



#7

Phenol-d6

Concen: 102.54 ng

RT: 6.39 min Scan# 420

Delta R.T. -0.02 min

Lab File: BF088747.D

Acq: 6 Jul 2016 21:29

Instrument :

BNA_F

ClientSampleId :

C2.2-06


Tgt Ion: 99 Resp: 760955

Ion Ratio Lower Upper

99 100

42 15.2 12.2 18.2



71 35.5 23.4 35.0#

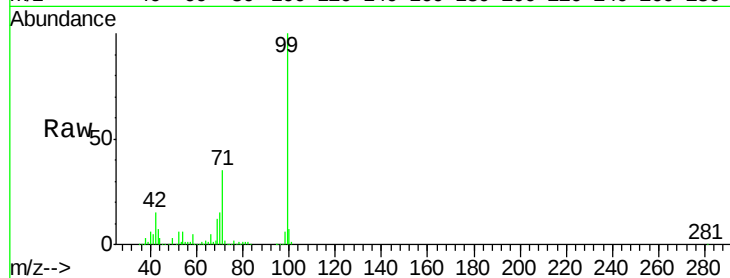

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

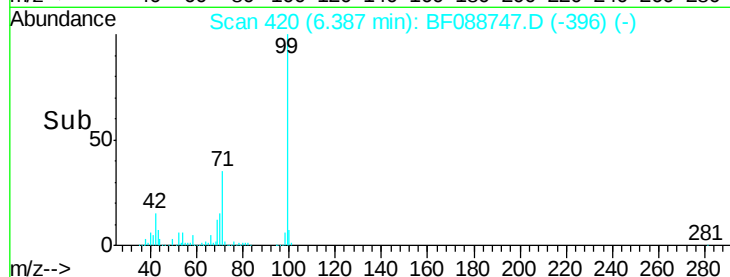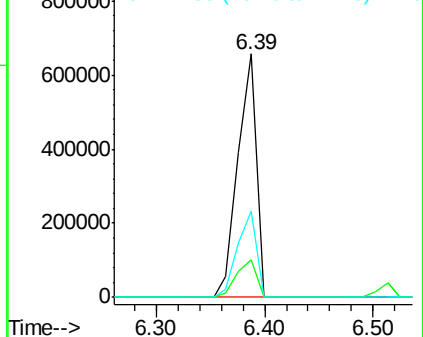

#19

n-Nitroso-di-n-propylamine

Concen: 12.75 ng

RT: 7.31 min Scan# 501

Delta R.T. 0.11 min

Lab File: BF088747.D

Acq: 6 Jul 2016 21:29

Tgt Ion: 70 Resp: 63560


Ion Ratio Lower Upper

70 100

42 40.4 49.6 74.4#

101 0.0 7.1 10.7#

130 2.1 15.4 23.2#


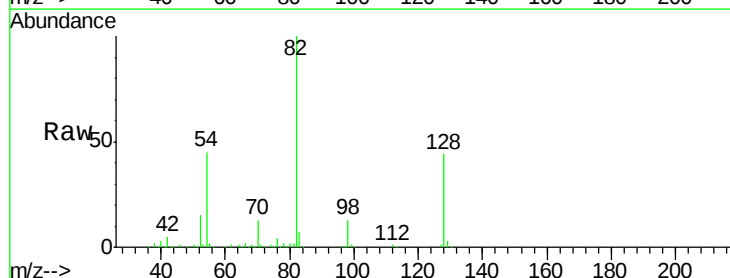


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

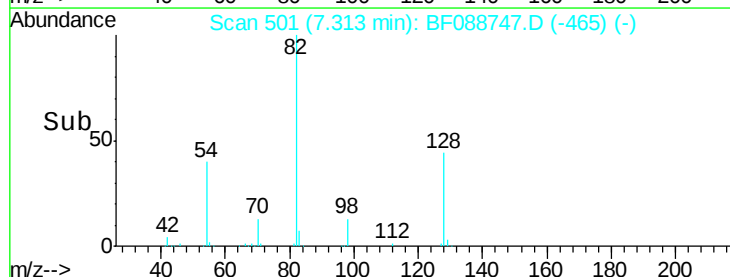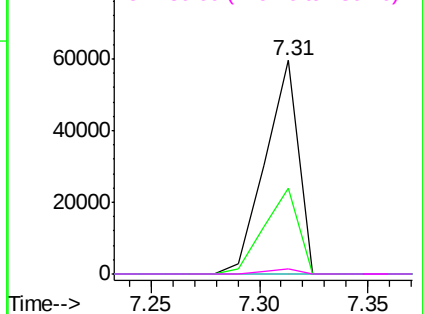



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.03 min Scan# 564

Delta R.T. -0.03 min

Lab File: BF088747.D

Acq: 6 Jul 2016 21:29

Instrument :

BNA_F

ClientSampleId :

C2.2-06

Tgt Ion: 136 Resp: 390039


Ion Ratio Lower Upper

136 100

137 10.8 9.1 13.7

54 6.1 6.6 10.0#

68 5.2 5.1 7.7




Abundance Ion 136.00 (135.70 to 136.70): E



Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

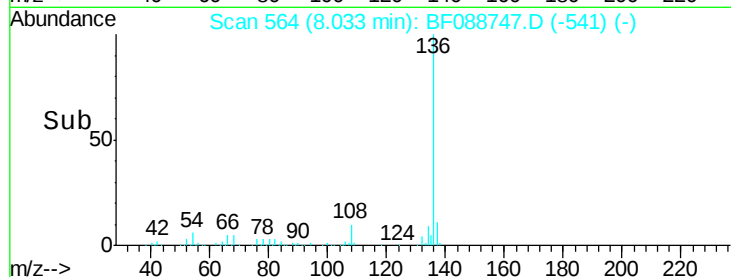

Time-->

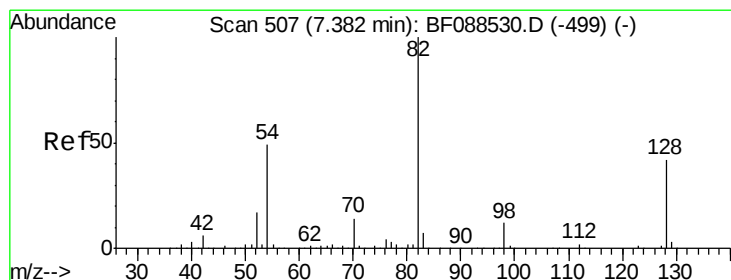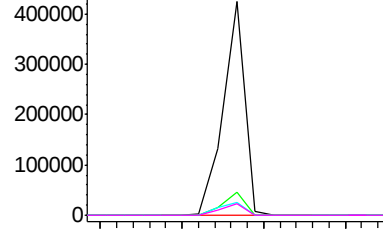

#23

Nitrobenzene-d5

Concen: 63.68 ng

RT: 7.31 min Scan# 501

Delta R.T. -0.03 min

Lab File: BF088747.D

Acq: 6 Jul 2016 21:29


Tgt Ion: 82 Resp: 473925

Ion Ratio Lower Upper

82 100

128 44.5 35.9 53.9


54 44.6 40.9 61.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

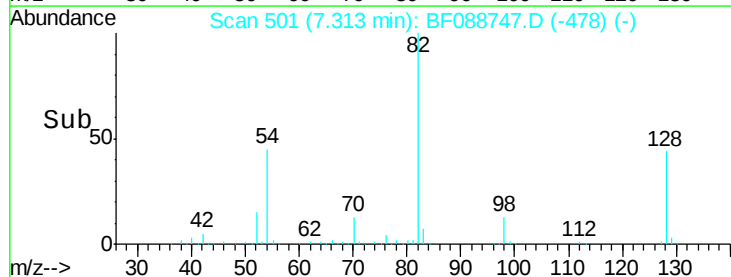





Time-->

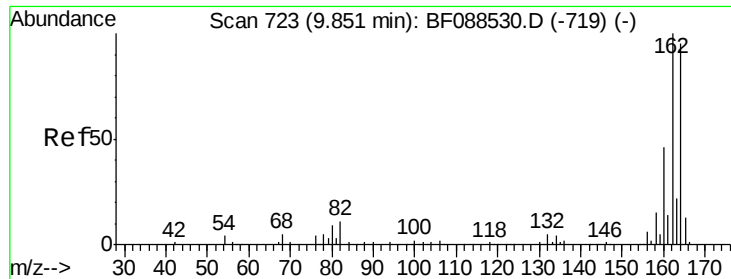

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.78 min Scan# 717
 Delta R.T. -0.03 min
 Lab File: BF088747.D
 Acq: 6 Jul 2016 21:29




Instrument :
 BNA_F
 ClientSampleId :
 C2.2-06

Tgt Ion:164 Resp: 183839
 Ion Ratio Lower Upper
 164 100
 162 106.9 85.4 128.2
 160 48.7 39.5 59.3

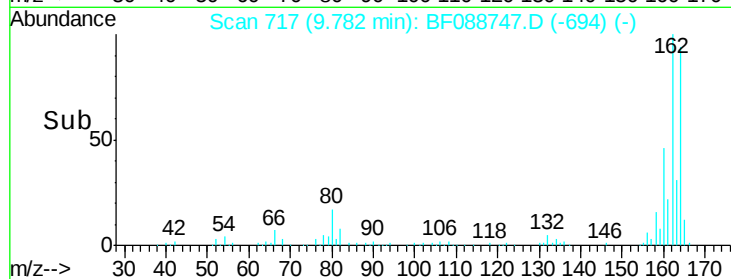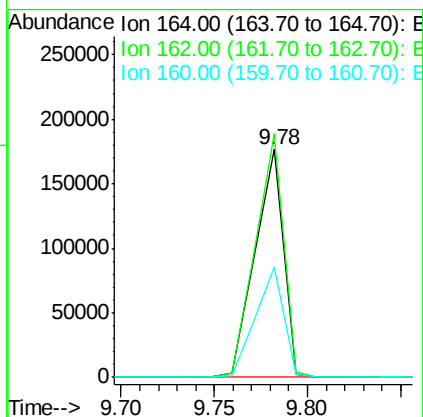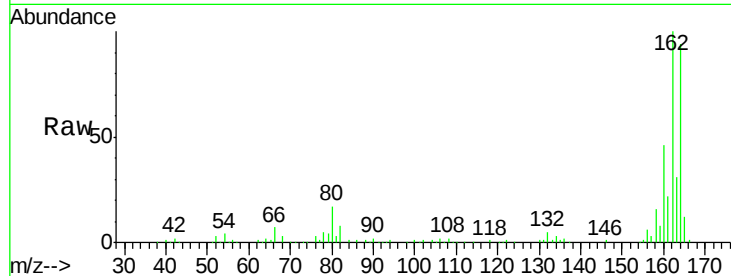

#41
 2,4,6-Tribromophenol
 Concen: 79.16 ng
 RT: 10.56 min Scan# 785
 Delta R.T. -0.05 min
 Lab File: BF088747.D
 Acq: 6 Jul 2016 21:29

Tgt Ion:330 Resp: 135140
 Ion Ratio Lower Upper
 330 100
 332 97.1 0.0 0.0#
 141 38.4 0.0 0.0#


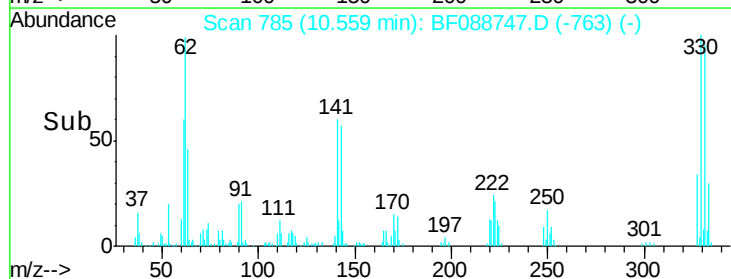
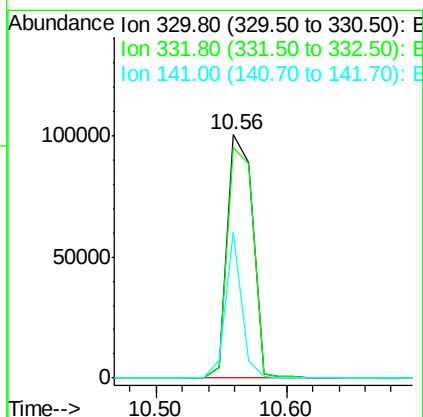





#44
2-Fluorobiphenyl
Concen: 56.45 ng
RT: 9.11 min Scan# 658
Delta R.T. -0.03 min
Lab File: BF088747.D
Acq: 6 Jul 2016 21:29




Instrument :
BNA_F
ClientSampleId :
C2.2-06

Tgt Ion:172 Resp: 656991
Ion Ratio Lower Upper
172 100
171 36.3 28.6 43.0
170 24.4 19.2 28.8

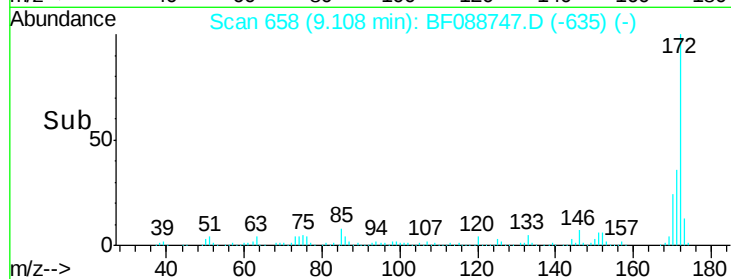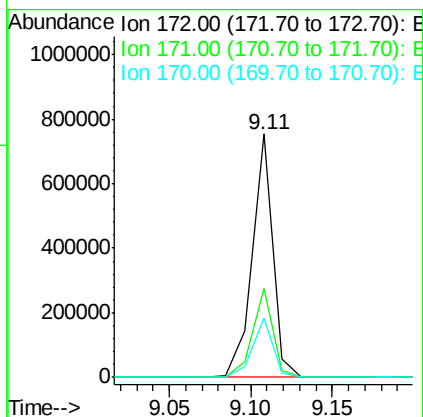

#49
Dimethylphthalate
Concen: 8.78 ng
RT: 9.51 min Scan# 693
Delta R.T. -0.03 min
Lab File: BF088747.D
Acq: 6 Jul 2016 21:29

Tgt Ion:163 Resp: 115040
Ion Ratio Lower Upper
163 100
194 3.9 2.8 4.2
164 9.4 8.3 12.5

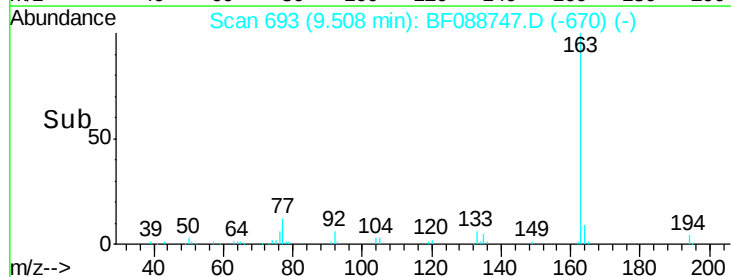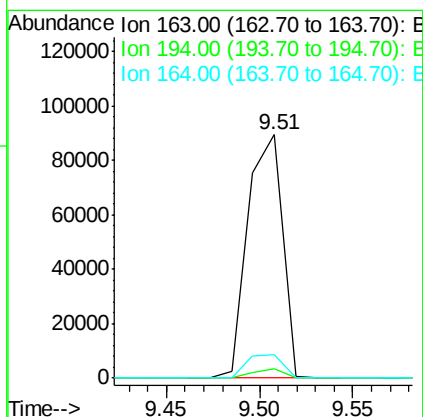




#56
 2,4-Dinitrotoluene
 Concen: 6.16 ng
 RT: 9.78 min Scan# 717
 Delta R.T. -0.22 min
 Lab File: BF088747.D
 Acq: 6 Jul 2016 21:29

Instrument :
 BNA_F
 ClientSampleId :
 C2.2-06

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.7	22.0	33.0#
89	1.6	41.1	61.7#
182	0.0	2.0	3.0#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

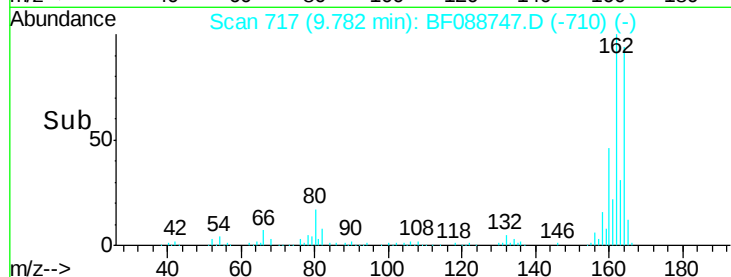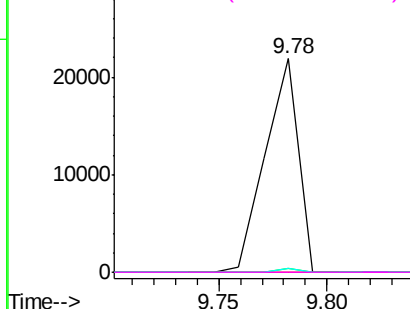




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.26 min Scan# 846
 Delta R.T. -0.03 min
 Lab File: BF088747.D
 Acq: 6 Jul 2016 21:29


Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.4	9.0	13.6#
80	9.3	10.0	15.0#

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

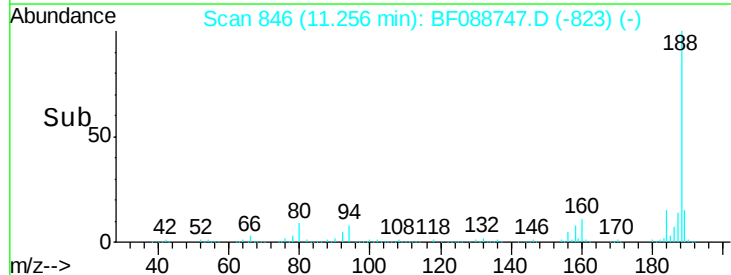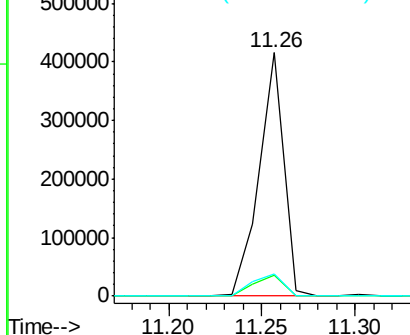


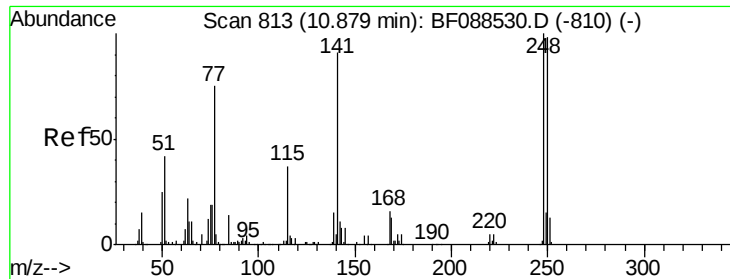




#66
4-Bromophenyl-phenylether
Concen: 2.28 ng
RT: 10.56 min Scan# 785
Delta R.T. -0.29 min
Lab File: BF088747.D
Acq: 6 Jul 2016 21:29

Instrument :
BNA_F
ClientSampleId :
C2.2-06

Tgt Ion:248 Resp: 8677
Ion Ratio Lower Upper
248 100
250 198.7 77.1 115.7#
141 693.1 50.6 76.0#

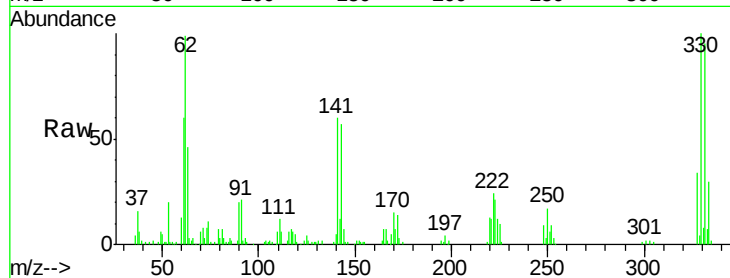


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

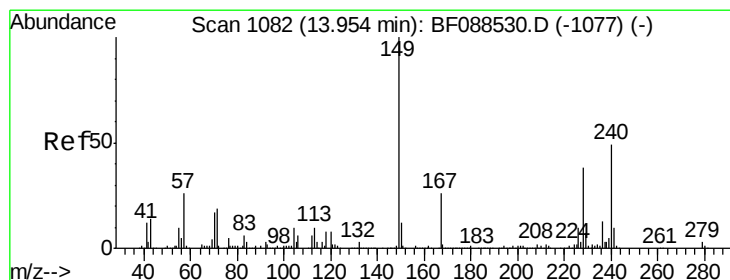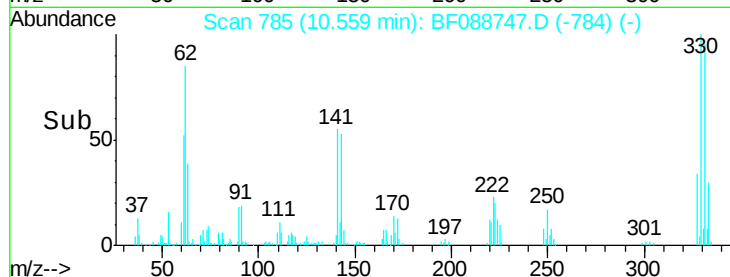
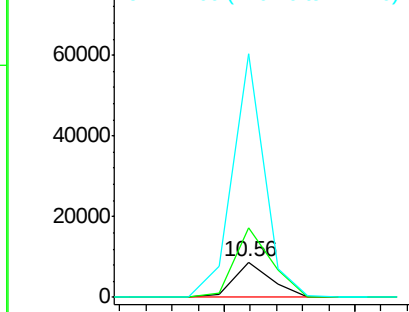


#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.87 min Scan# 1075
Delta R.T. -0.05 min
Lab File: BF088747.D
Acq: 6 Jul 2016 21:29

Tgt Ion:240 Resp: 293335
Ion Ratio Lower Upper
240 100
120 14.4 6.8 10.2#
236 26.1 20.2 30.2

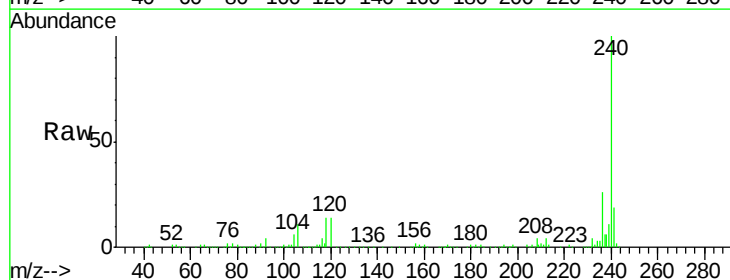

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



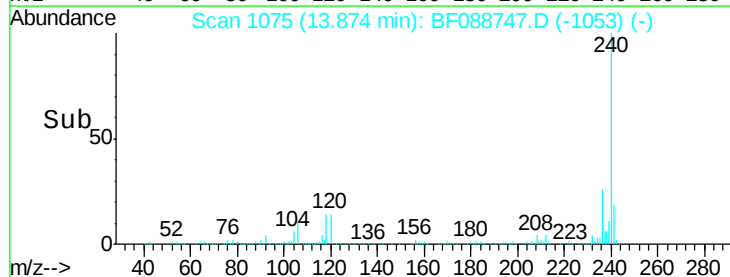
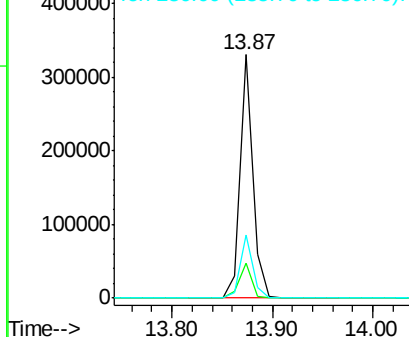




#78
 Terphenyl-d14
 Concen: 55.29 ng
 RT: 12.83 min Scan# 984
 Delta R.T. -0.03 min
 Lab File: BF088747.D
 Acq: 6 Jul 2016 21:29

Instrument :
 BNA_F
 ClientSampleId :
 C2.2-06

Tgt Ion:244 Resp: 728172
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.0 9.0
 122 16.0 11.2 16.8

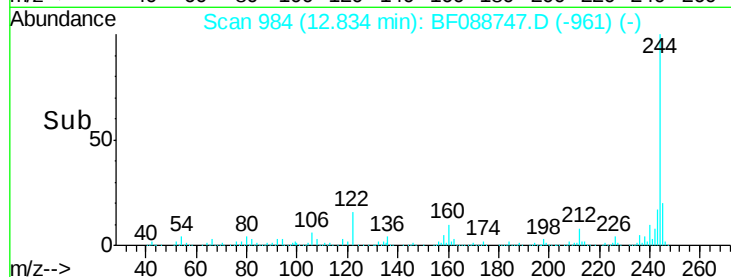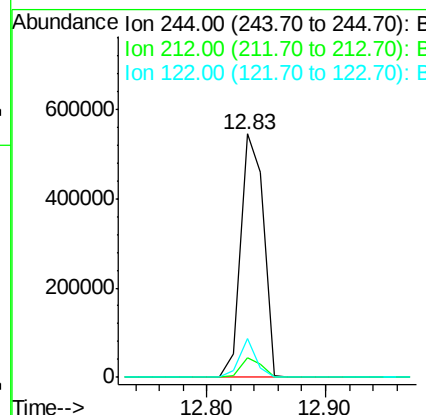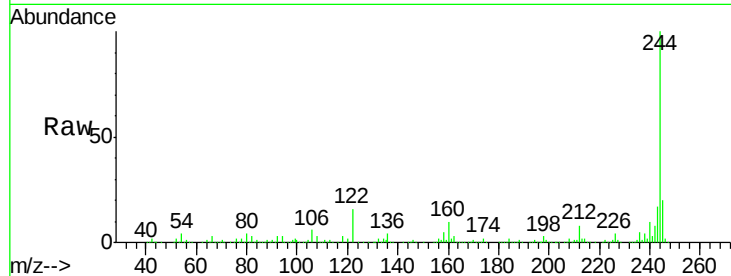

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.26 min Scan# 1196
 Delta R.T. -0.05 min
 Lab File: BF088747.D
 Acq: 6 Jul 2016 21:29

Tgt Ion:264 Resp: 236383
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.2 28.8
 265 22.1 16.9 25.3

