


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070616\
 Data File : BF088730.D
 Acq On : 6 Jul 2016 10:30
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 17:15:08 2016

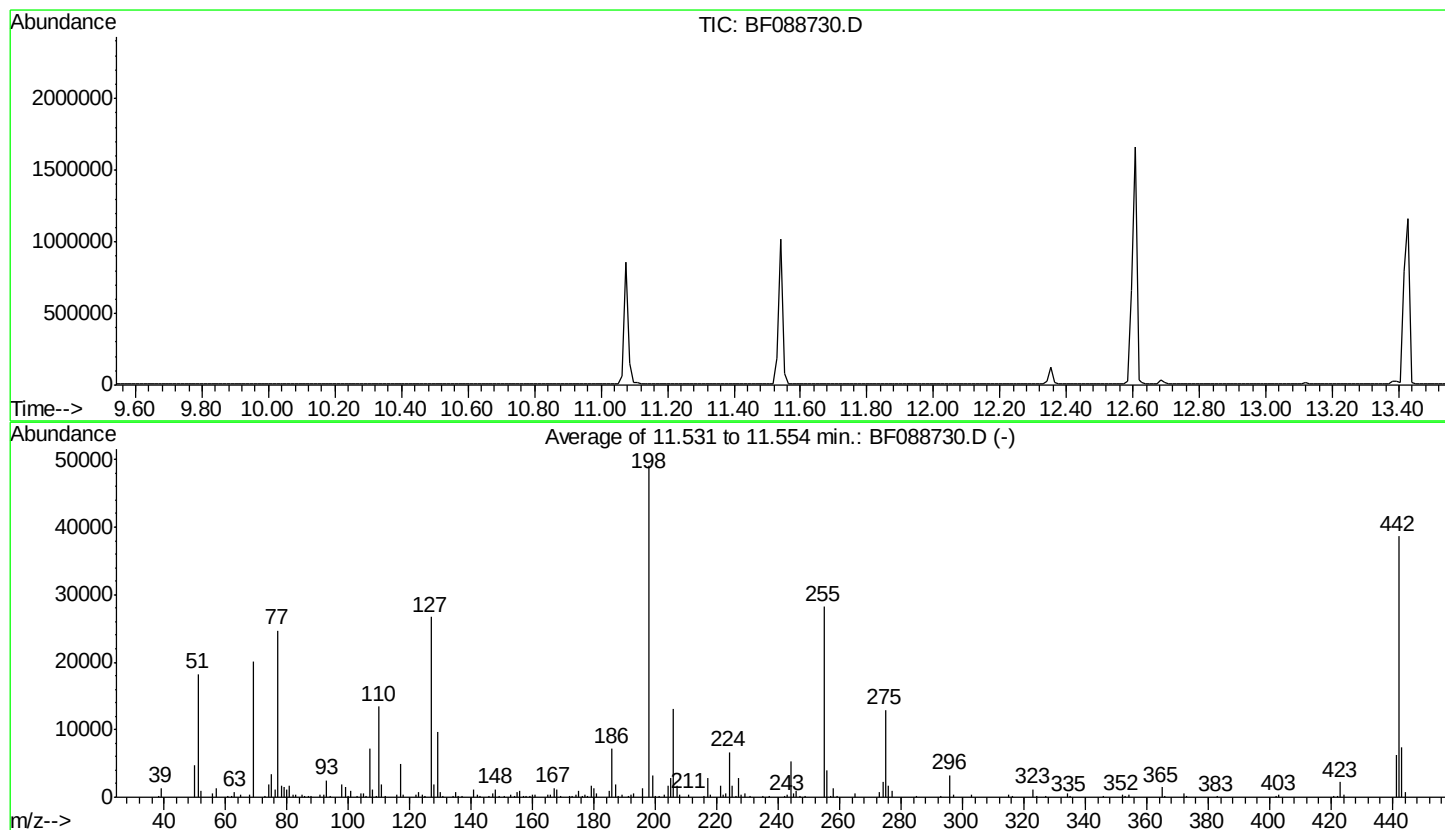

AutoFind: Scans 870, 871, 872; Background Corrected with Scan 867

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	18217	PASS
68	69	0.00	2	1.9	387	PASS
69	198	0.00	100	40.9	20074	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	26682	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49099	PASS
199	198	5	9	6.5	3171	PASS
275	198	10	60	26.3	12902	PASS
365	198	1	100	2.9	1428	PASS
441	442	0.01	24	16.1	6224	PASS
442	198	50	100	78.7	38643	PASS
443	442	15	24	19.2	7421	PASS