


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070616\
 Data File : BF088739.D
 Acq On : 6 Jul 2016 17:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 17:15:08 2016

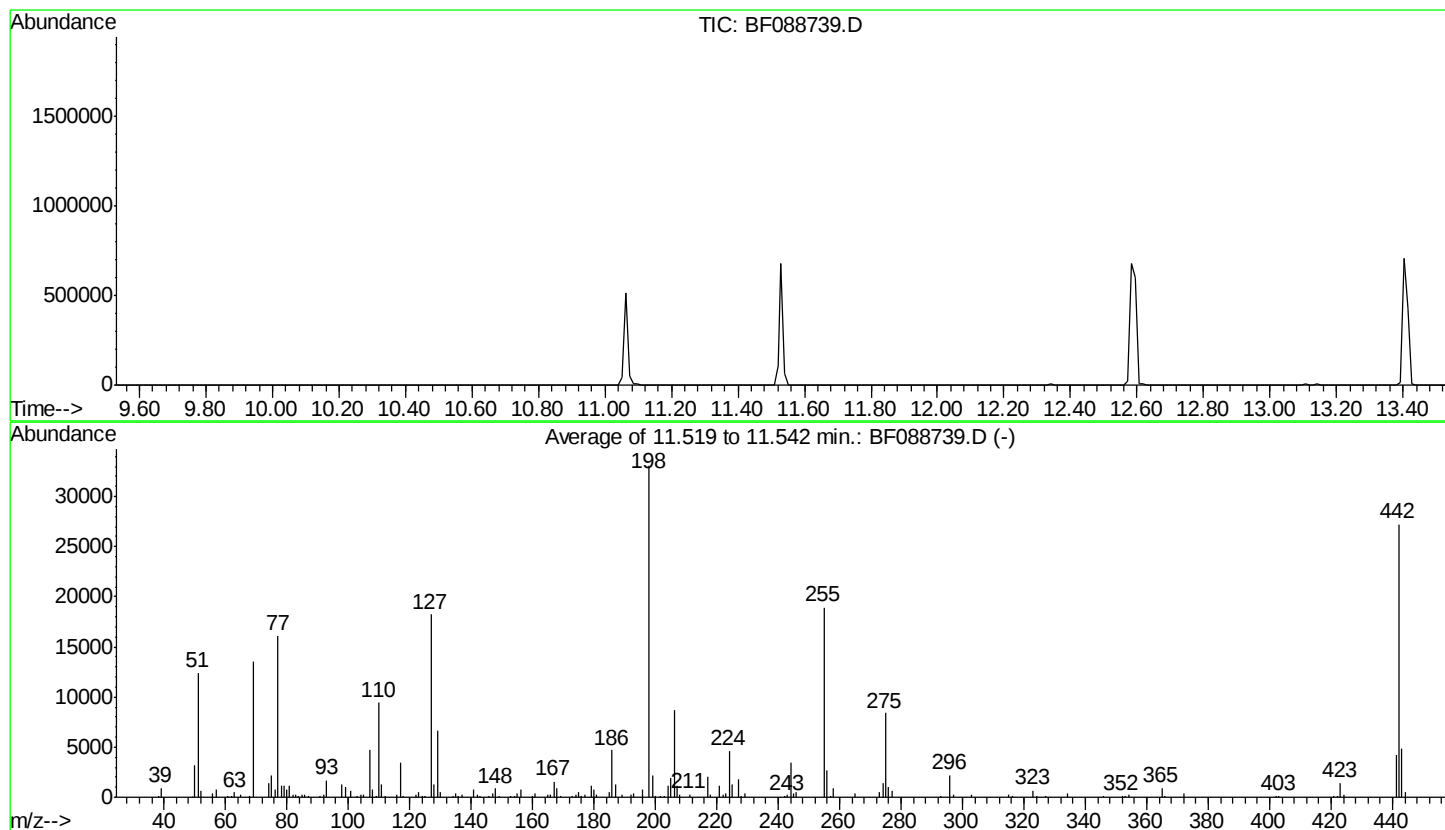

AutoFind: Scans 869, 870, 871; Background Corrected with Scan 866

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	12403	PASS
68	69	0.00	2	1.1	154	PASS
69	198	0.00	100	40.9	13520	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.1	18221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33071	PASS
199	198	5	9	6.5	2141	PASS
275	198	10	60	25.5	8425	PASS
365	198	1	100	2.8	940	PASS
441	442	0.01	24	15.4	4182	PASS
442	198	50	100	82.3	27215	PASS
443	442	15	24	18.0	4908	PASS