
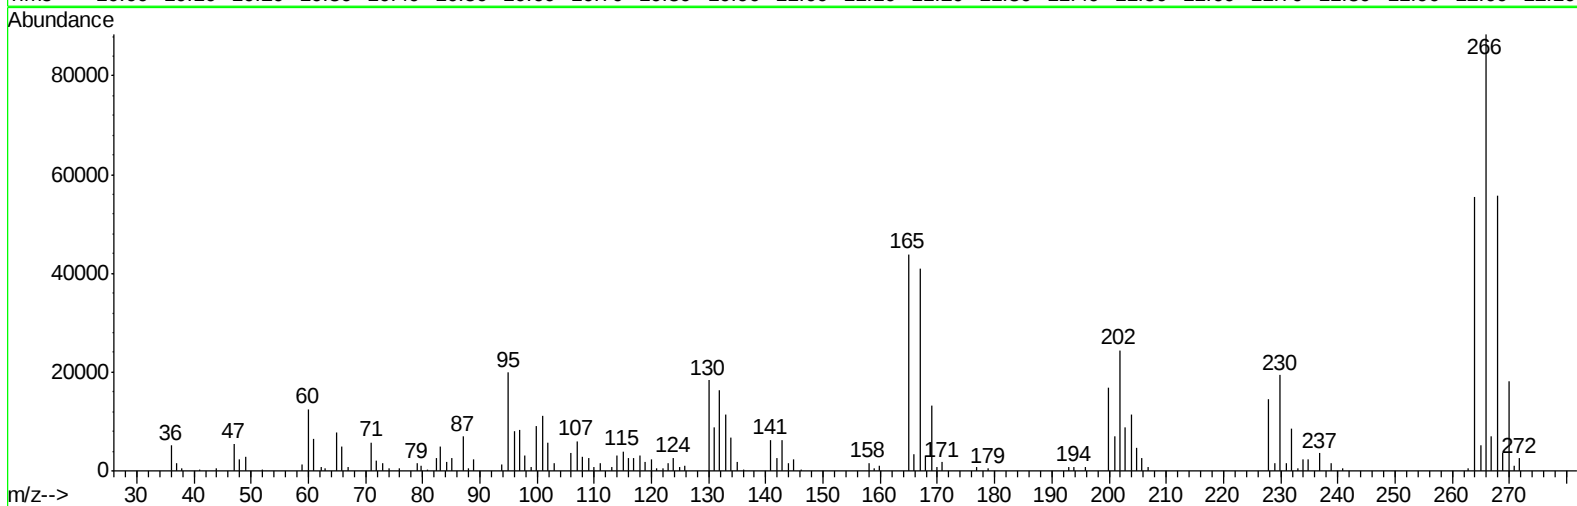


Data Path : Z:\HPCHEM1\BNA F\DATA\BF070617\
Data File : BF096522.D
Acq On : 6 Jul 2017 10:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 05:24:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 13:27:10 2017
Response via : Initial Calibration

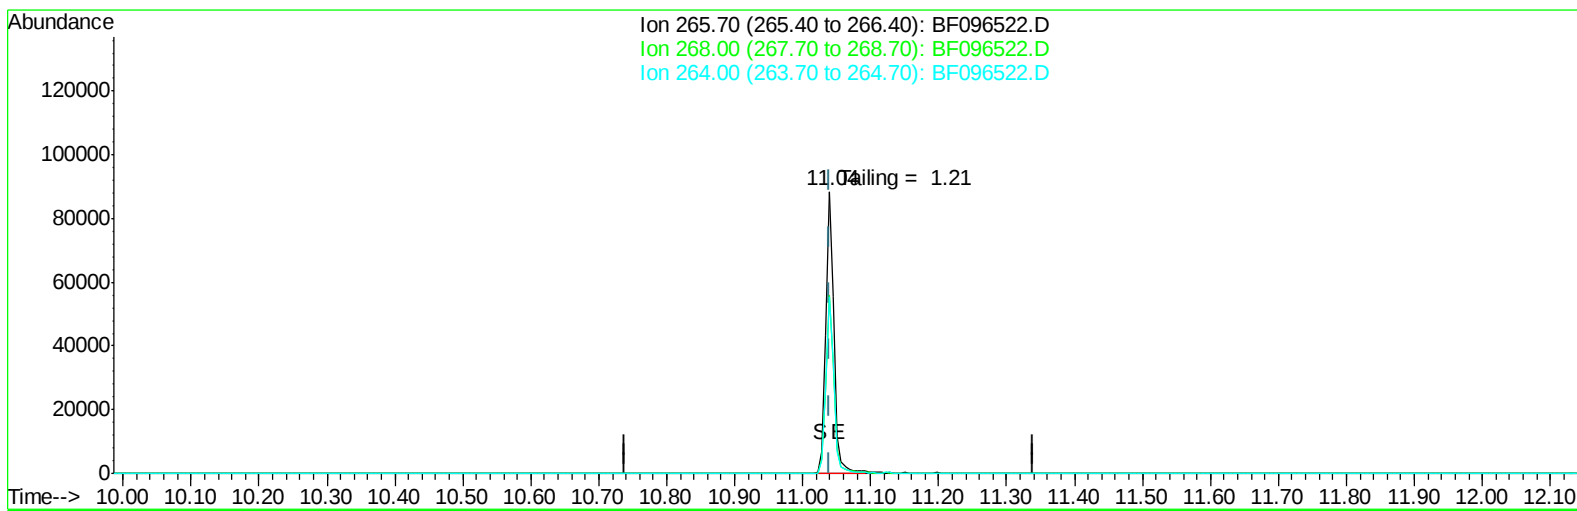

TIC: BF096522.D

(69) Pentachlorophenol (C)

11.039min (-0.000) 66211.08ng

response 76943

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.11
264.00	64.60	62.79
0.00	0.00	0.00