
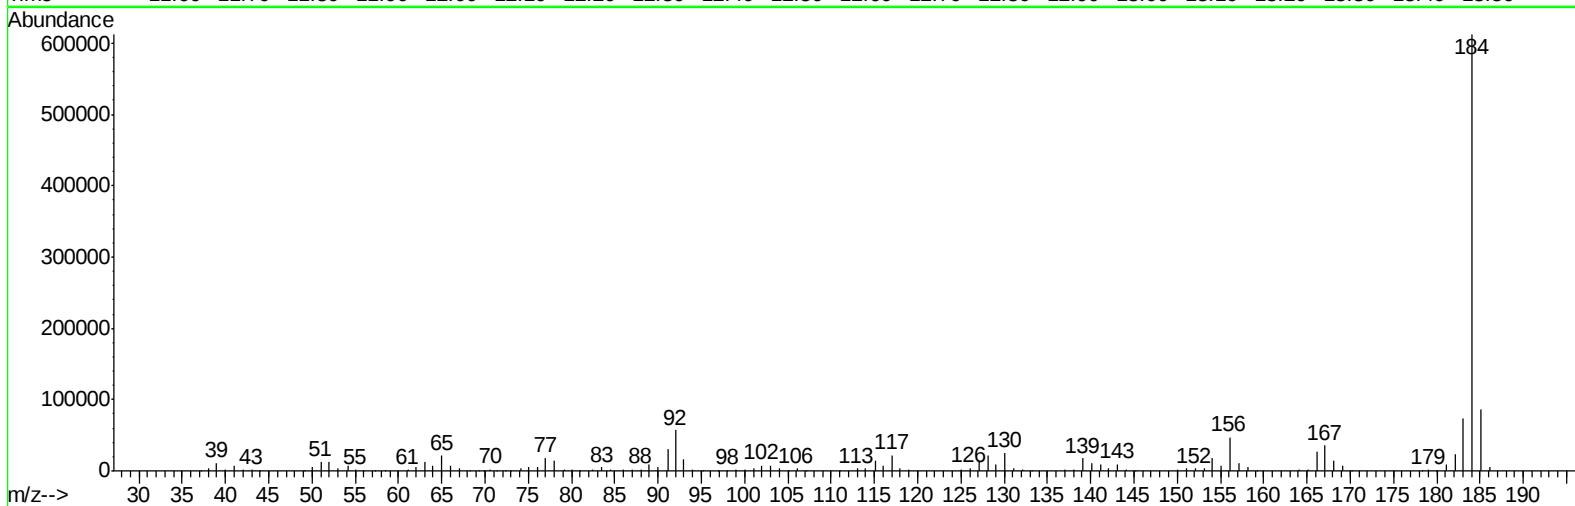


Data Path : Z:\HPCHEM1\BNA F\DATA\BF070617\
 Data File : BF096522.D
 Acq On : 6 Jul 2017 10:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 05:24:04 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 13:27:10 2017
 Response via : Initial Calibration

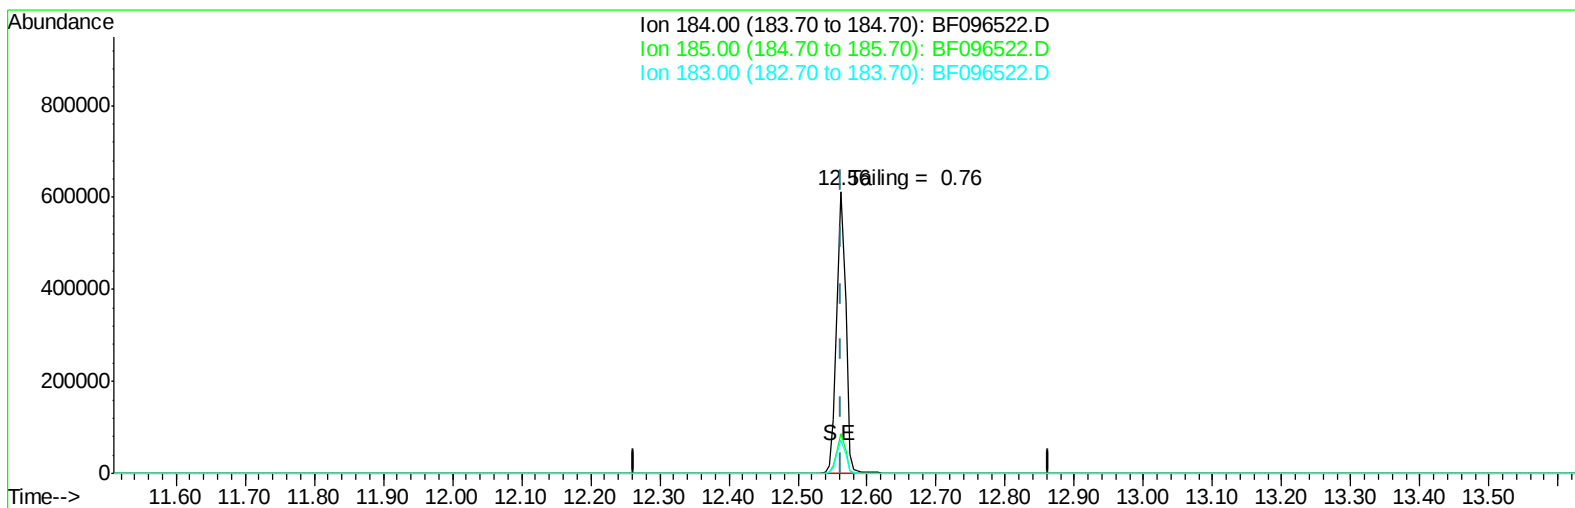

TIC: BF096522.D

(76) Benzidine



12.563min (-0.000) 0.00ng

response 549762

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.05#
183.00	12.20	11.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070617\
Data File : BF096522.D
Acq On : 6 Jul 2017 10:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 05:24:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 13:27:10 2017
Response via : Initial Calibration

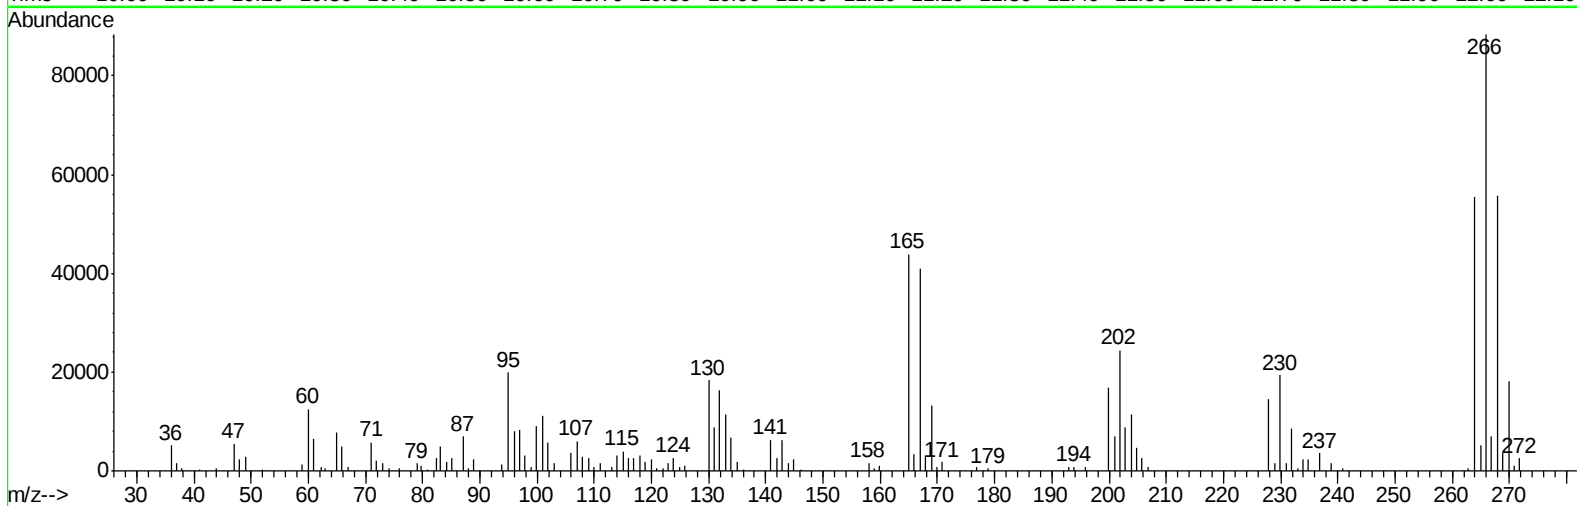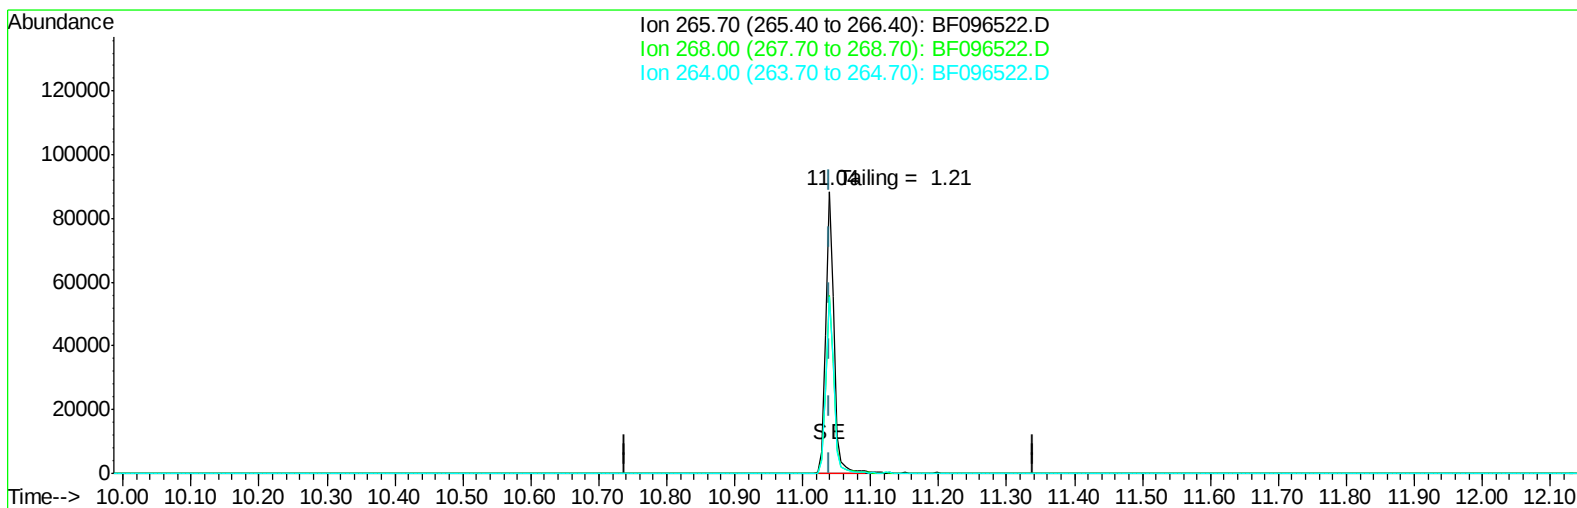

TIC: BF096522.D

(69) Pentachlorophenol (C)

11.039min (-0.000) 66211.08ng

response 76943

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.11
264.00	64.60	62.79
0.00	0.00	0.00