


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070617\
 Data File : BF096522.D
 Acq On : 6 Jul 2017 10:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 13:02:33 2017

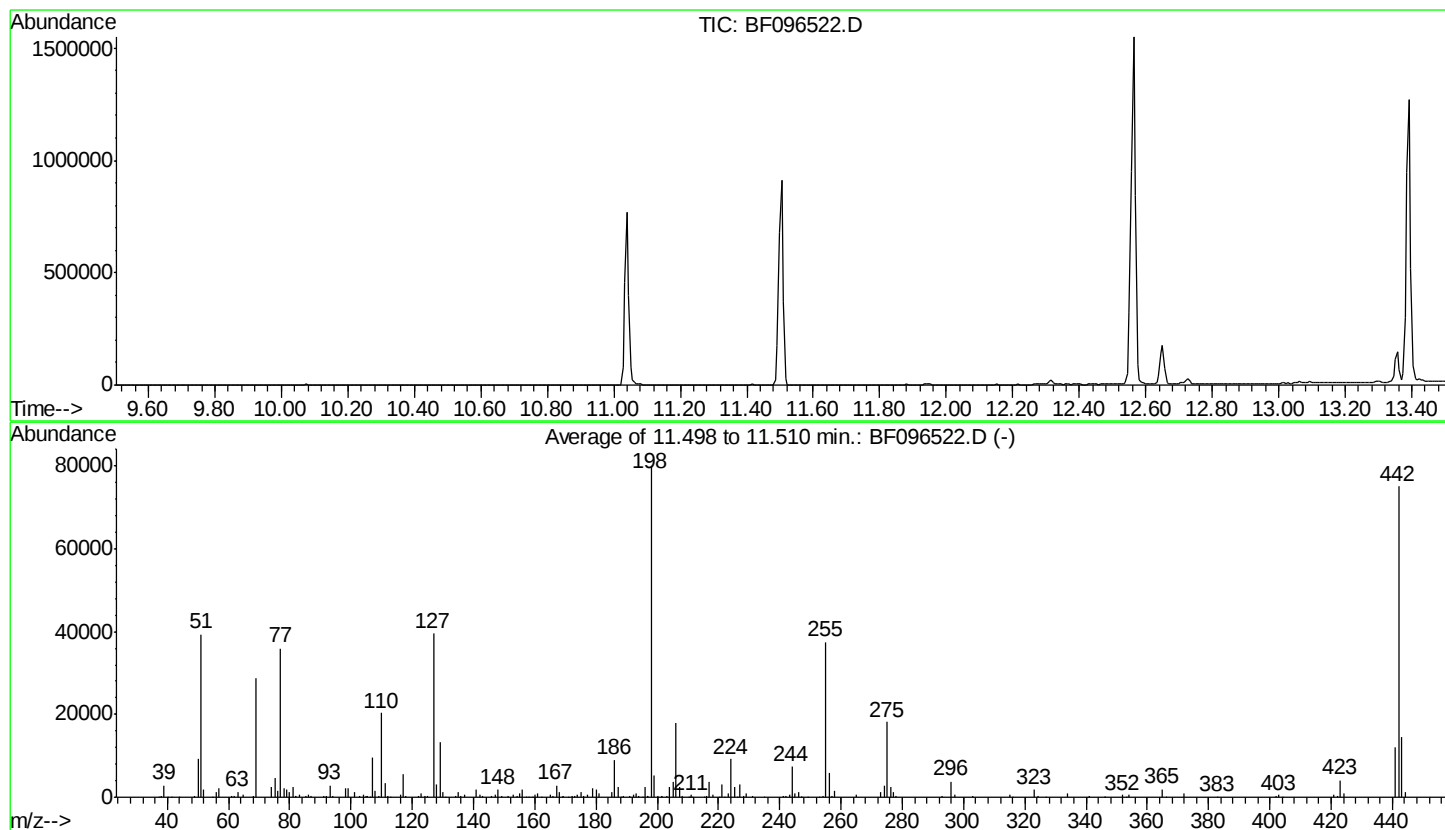

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	39303	PASS
68	69	0.00	2	1.6	451	PASS
69	198	0.00	100	35.9	28747	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	39509	PASS
197	198	0.00	2	0.5	367	PASS
198	198	100	100	100.0	80106	PASS
199	198	5	9	6.5	5186	PASS
275	198	10	60	22.7	18224	PASS
365	198	1	100	2.4	1932	PASS
441	442	0.01	24	16.2	12139	PASS
442	198	50	100	93.7	75034	PASS
443	442	15	24	19.4	14525	PASS