


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070620\
 Data File : BF120766.D
 Acq On : 6 Jul 2020 9:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 18:51:52 2020

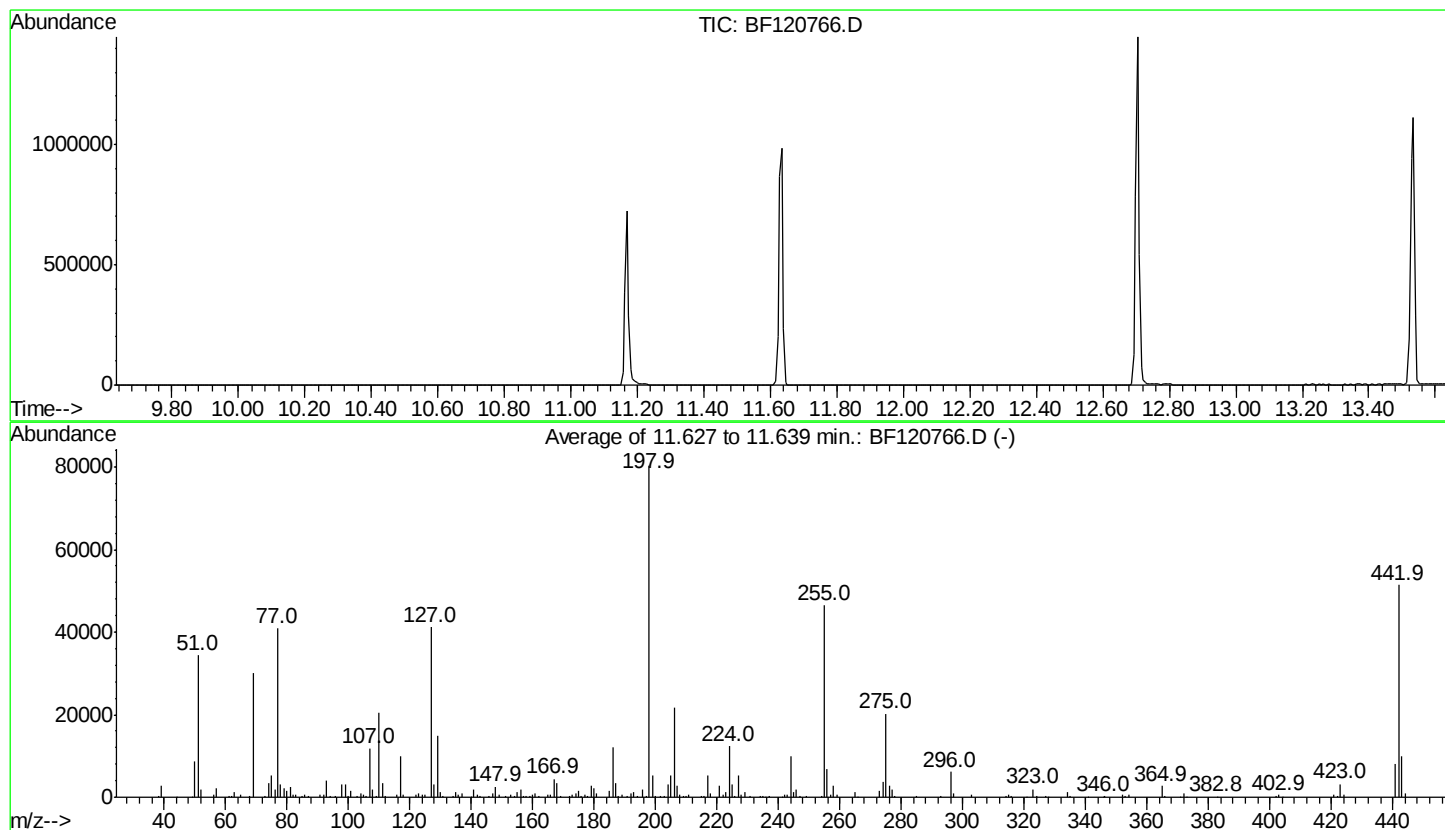

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	34365	PASS
68	69	0.00	2	1.4	414	PASS
69	198	0.00	100	37.4	30015	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	41210	PASS
197	198	0.00	2	0.3	201	PASS
198	198	100	100	100.0	80338	PASS
199	198	5	9	6.5	5222	PASS
275	198	10	60	25.2	20256	PASS
365	198	1	100	3.4	2743	PASS
441	198	0.01	100	9.9	7938	PASS
442	198	50	100	64.0	51413	PASS
443	442	15	24	19.2	9883	PASS