

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
 Data File : BF129141.D
 Acq On : 06 Jul 2022 14:09
 Operator : CG\JU
 Sample : PB146035BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146035BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.351	3	11	17	rVB	138315	194947	1.81%	0.299%
2	4.122	307	312	318	rVB	137685	167063	1.55%	0.257%
3	5.587	556	561	564	rBV	6699611	7293937	67.78%	11.199%
4	6.581	724	730	733	rBV	6654627	7427662	69.02%	11.404%
5	6.957	790	794	797	rBV	2627361	2116940	19.67%	3.250%
6	7.522	884	890	893	rBV	4977264	5146335	47.82%	7.902%
7	8.239	1007	1012	1015	rBV	3367021	2905809	27.00%	4.462%
8	9.316	1189	1195	1198	rBV	10234848	10282828	95.55%	15.788%
9	9.998	1306	1311	1315	rBV	3793578	3337368	31.01%	5.124%
10	10.792	1440	1446	1449	rBV	7323128	6722363	62.47%	10.321%
11	11.492	1561	1565	1569	rBV	3983060	3326902	30.91%	5.108%
12	13.086	1831	1836	1839	rBV	10961679	10761489	100.00%	16.523%
13	14.145	2011	2016	2023	rBV	2656154	2524273	23.46%	3.876%
14	14.233	2025	2031	2037	rBV	438798	516232	4.80%	0.793%
15	14.374	2048	2055	2065	rVB3	69648	222385	2.07%	0.341%
16	15.668	2269	2275	2282	rBV	1590569	2183595	20.29%	3.353%




Sum of corrected areas: 65130128

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
Data File : BF129141.D
Acq On : 06 Jul 2022 14:09
Operator : CG\JU
Sample : PB146035BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146035BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

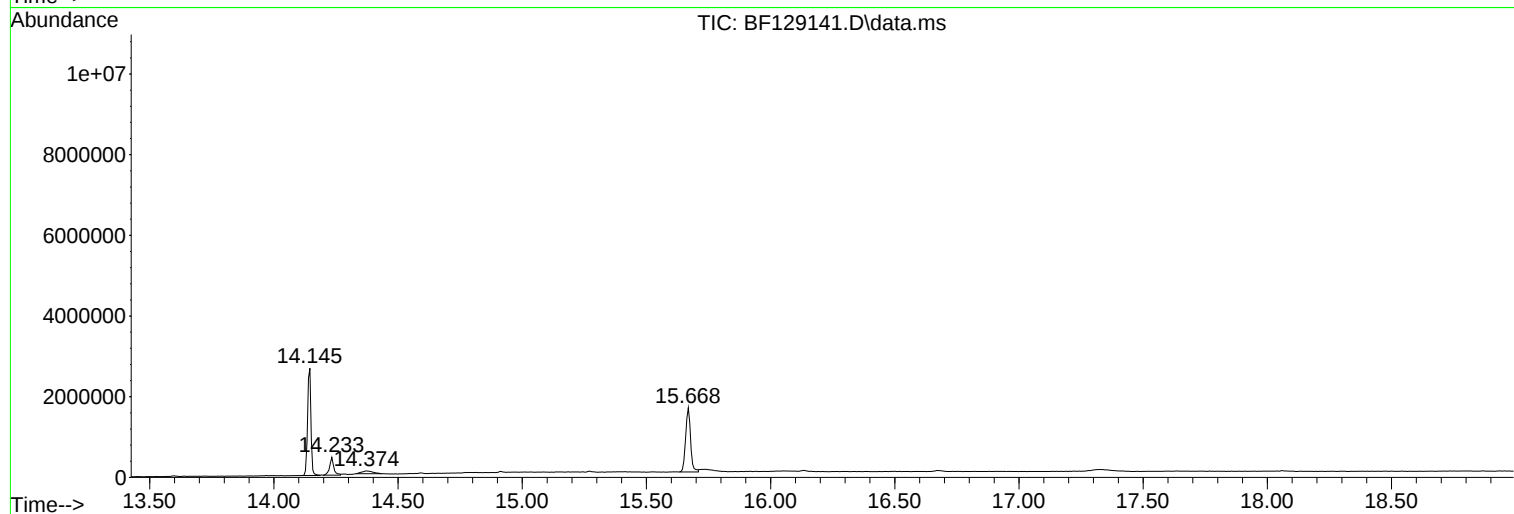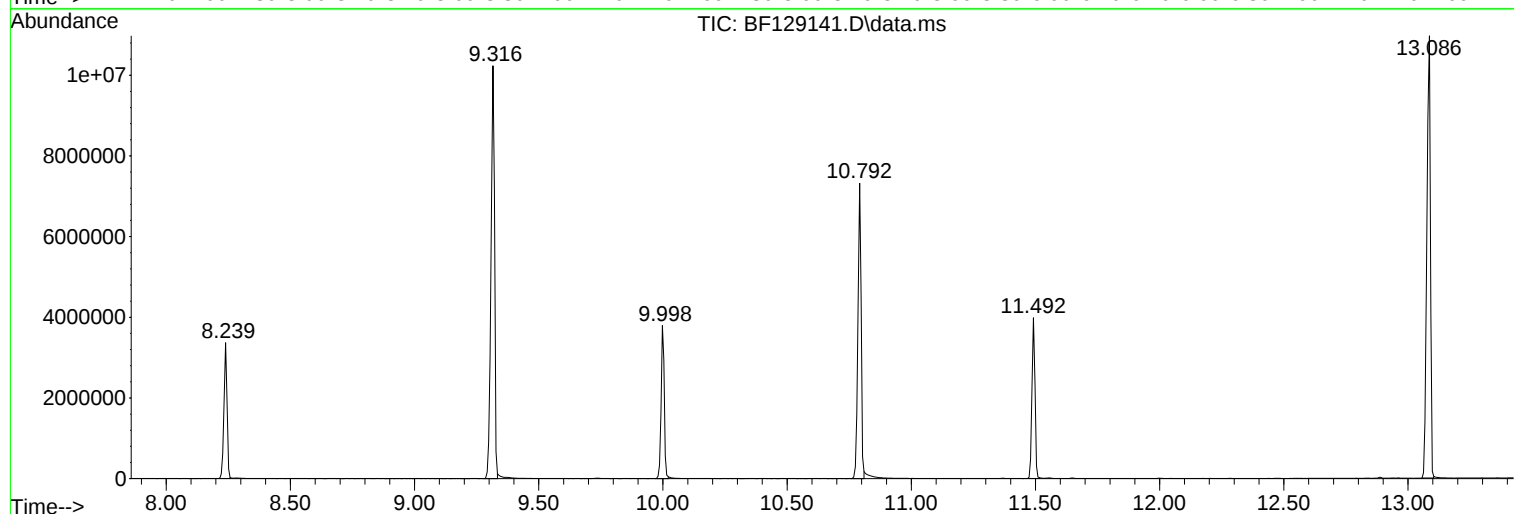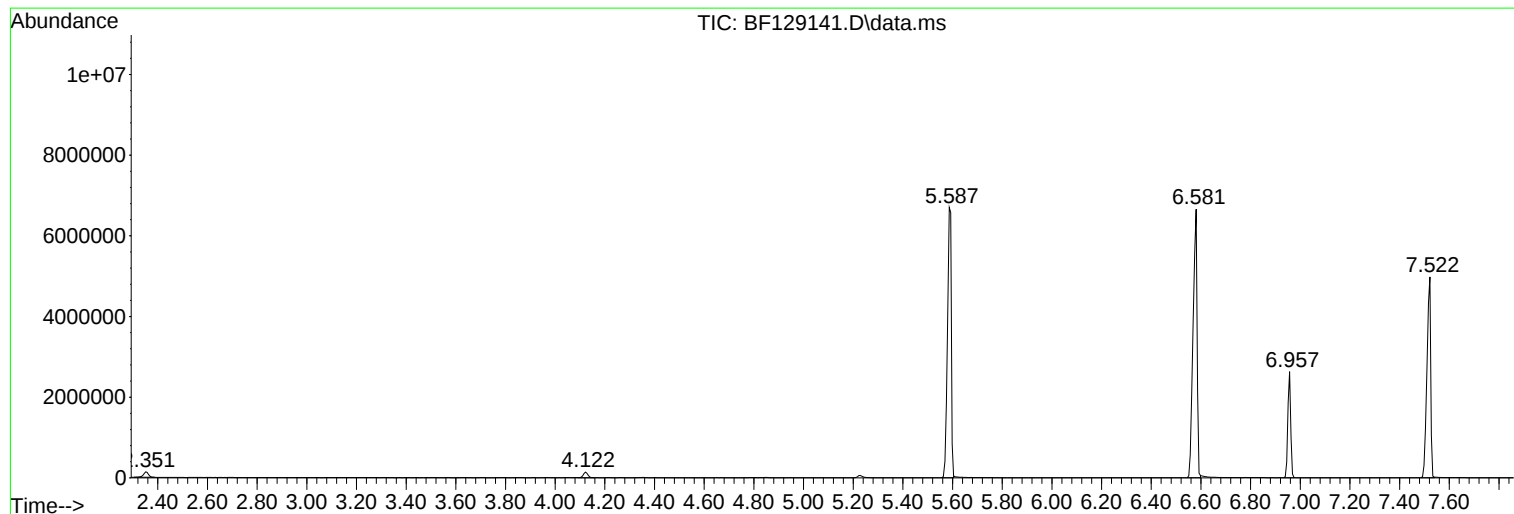

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
Data File : BF129141.D
Acq On : 06 Jul 2022 14:09
Operator : CG\JU
Sample : PB146035BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146035BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.233	4.09 ng	516232	Chrysene-d12	14.145

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	36
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28

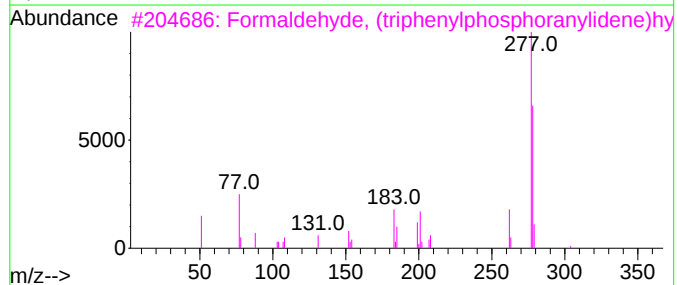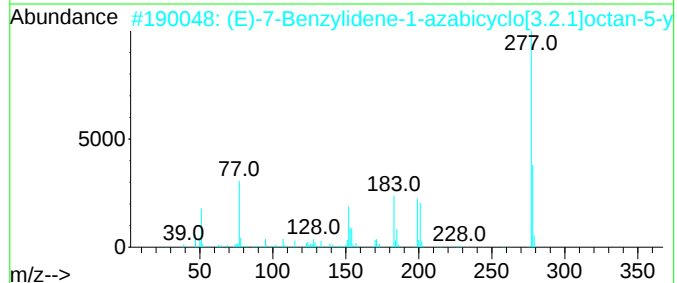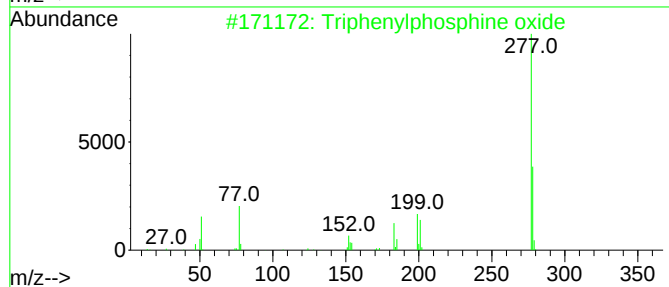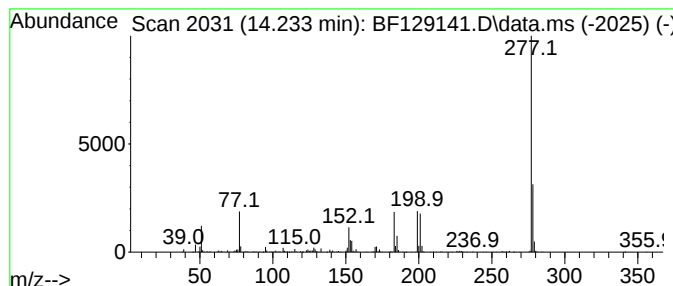

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
Data File : BF129141.D
Acq On : 06 Jul 2022 14:09
Operator : CG\JU
Sample : PB146035BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146035BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.233	4.1	ng	516232	5	14.145	2524270	20.0