


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
 Data File : BF129136.D
 Acq On : 06 Jul 2022 11:32
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

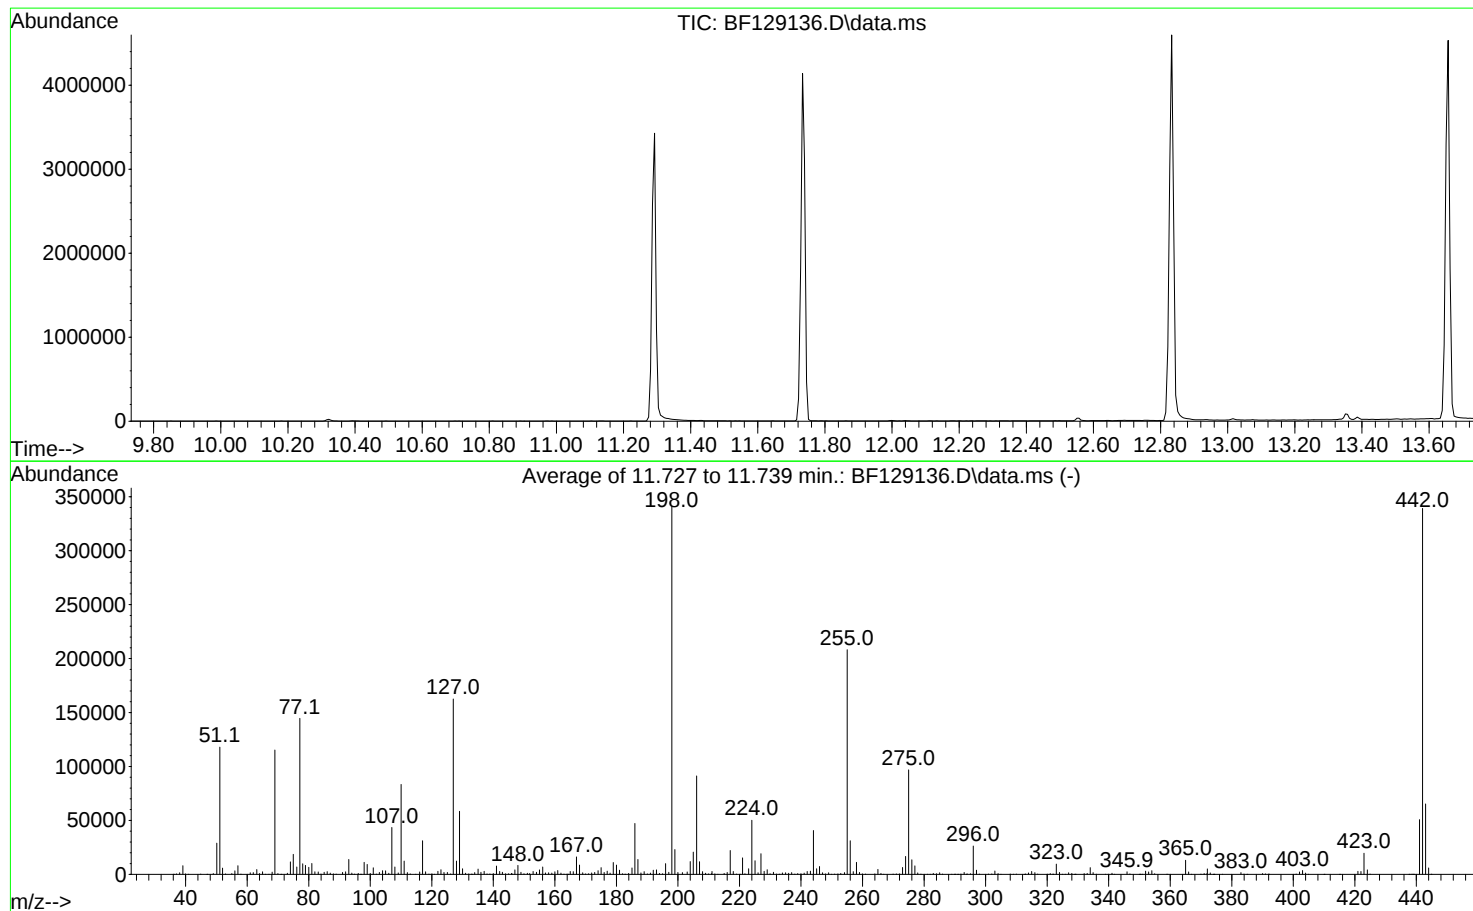




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	117853	PASS
68	69	0.00	2	1.8	2027	PASS
69	198	0.00	100	33.8	115173	PASS
70	69	0.00	2	0.6	712	PASS
127	198	10	80	47.7	162536	PASS
197	198	0.00	2	0.6	1938	PASS
198	198	100	100	100.0	340949	PASS
199	198	5	9	6.8	23048	PASS
275	198	10	60	28.4	96819	PASS
365	198	1	100	3.8	13079	PASS
441	198	0.01	100	14.9	50771	PASS
442	442	50	100	100.0	339099	PASS
443	442	15	24	19.2	65197	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
Data File : BF129136.D
Acq On : 06 Jul 2022 11:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 06 13:55:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

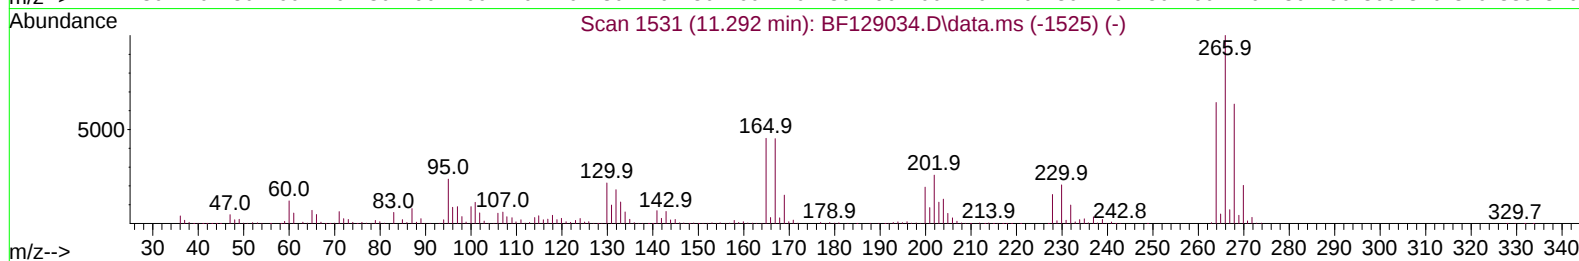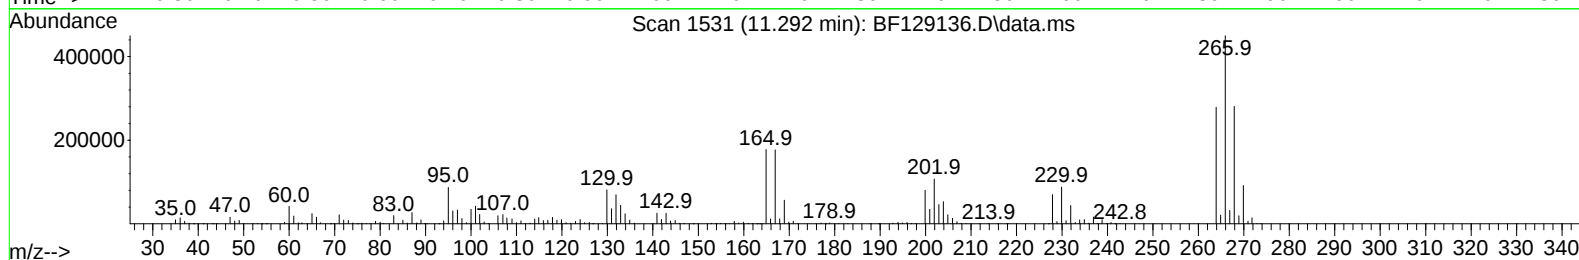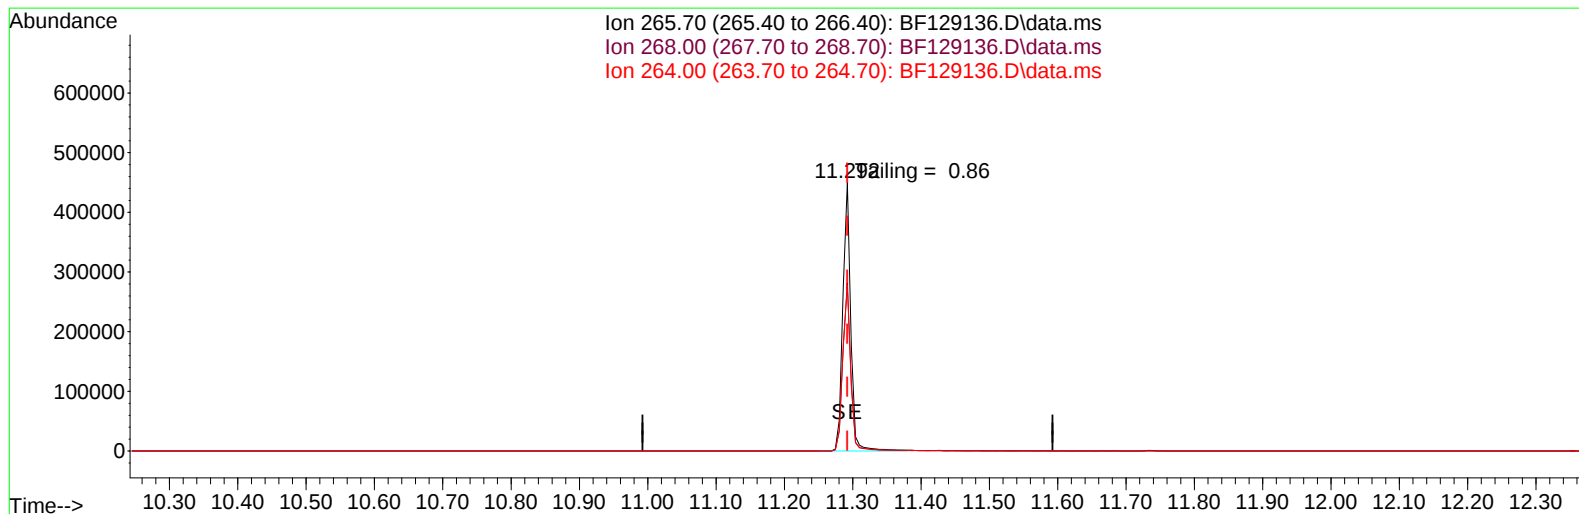

TIC: BF129136.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 730814.76 ng




response 360915

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.49
264.00	61.80	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070622\
Data File : BF129136.D
Acq On : 06 Jul 2022 11:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 06 13:55:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

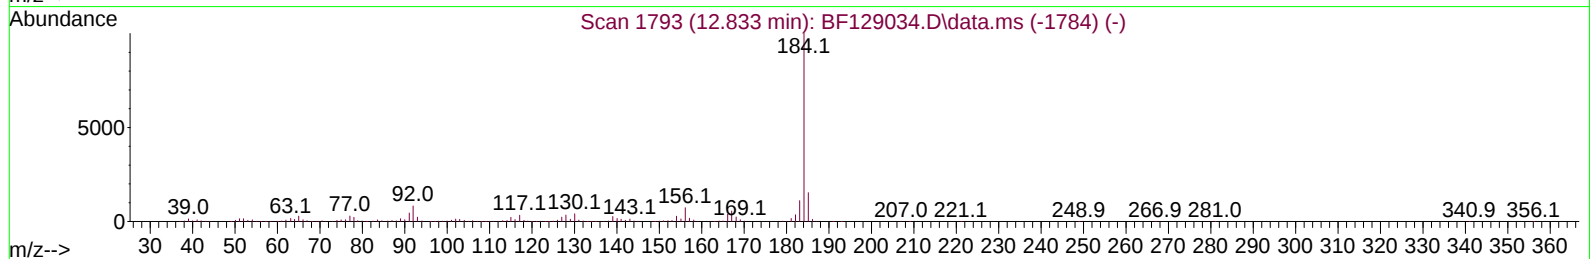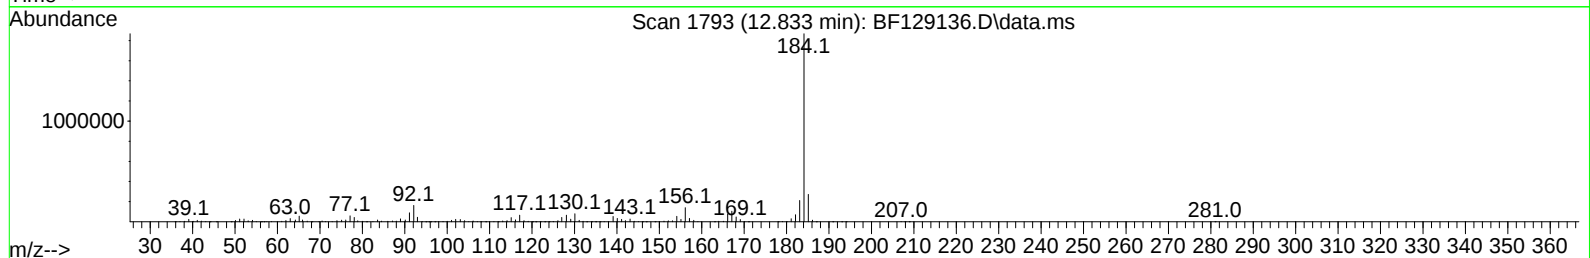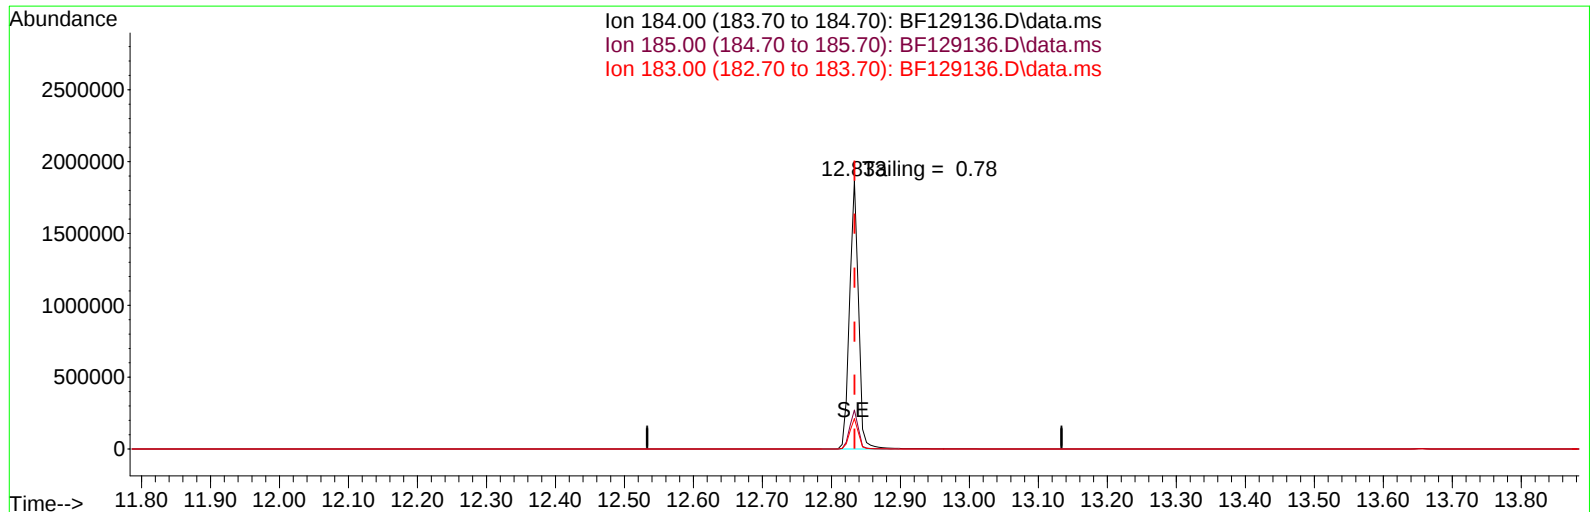

TIC: BF129136.D\data.ms

(77) Benzidine

12.833min (-0.000) 8579.40 ng m

response 1671889

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.58
183.00	11.60	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2022	BNA_F	<u>BF129136.D</u>
Compound Name	Response	Retention Time
DDT	758415	13.65
DDD	12360	13.35
DDE	2889	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15249	773664	1.97

Instrument :
BNA_F
ClientSampleId :
DFTPP