
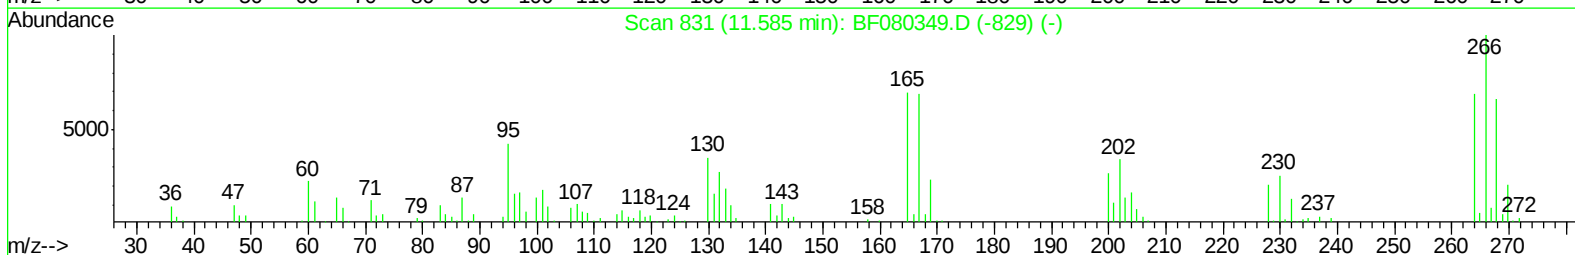
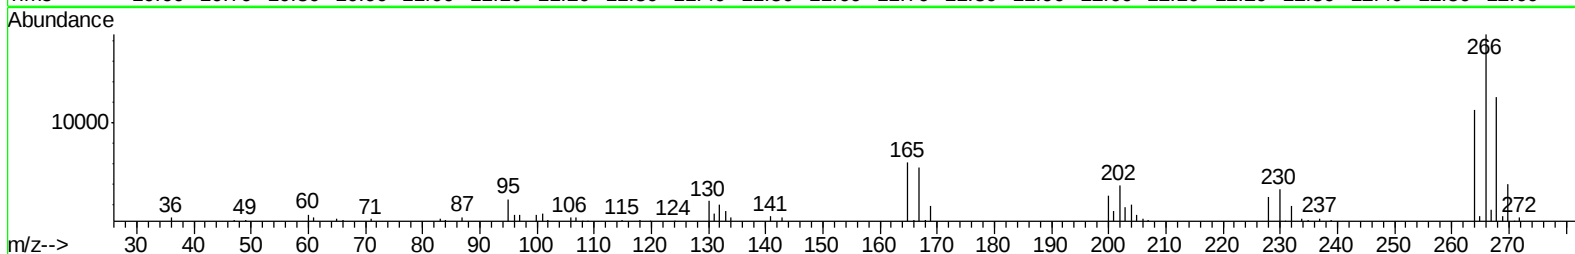


Data Path : Z:\HPCHEM1\BNA F\Data\BF070715\
Data File : BF080370.D
Acq On : 7 Jul 2015 11:15
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 04:42:41 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 03:05:40 2015
Response via : Initial Calibration

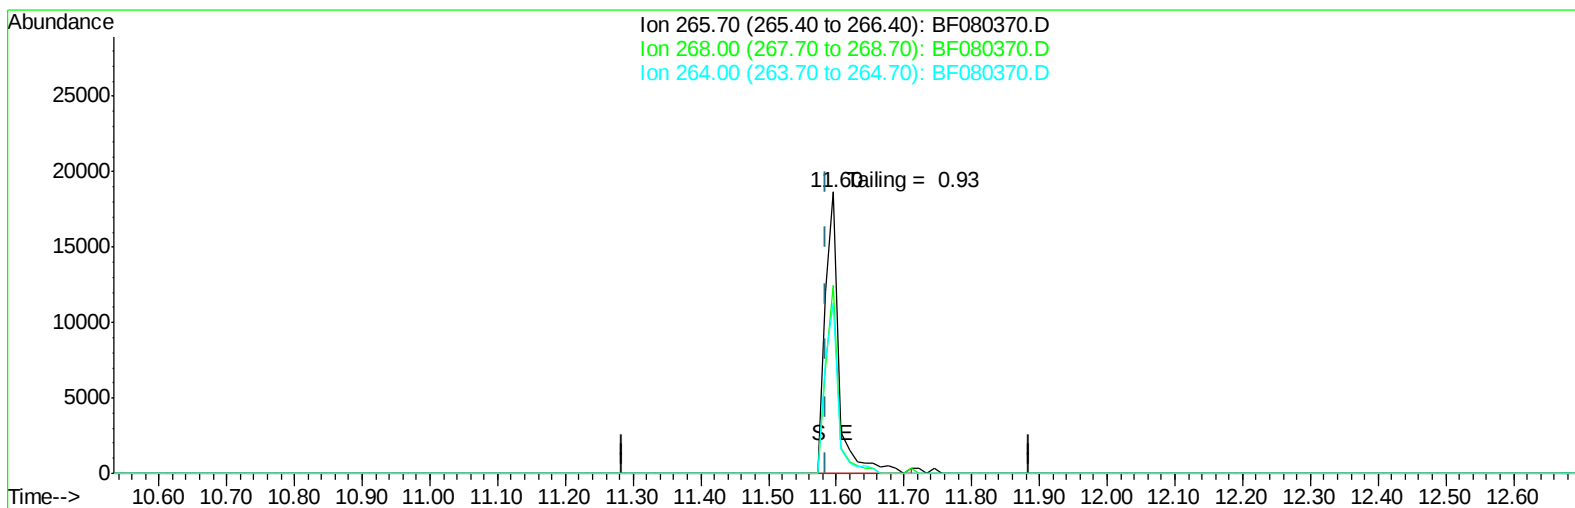

TIC: BF080370.D

(69) Pentachlorophenol (C)




11.596min (+0.011) 0.00ng

response 26367

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	66.88
264.00	68.80	60.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF070715\
Data File : BF080370.D
Acq On : 7 Jul 2015 11:15
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 04:42:41 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 03:05:40 2015
Response via : Initial Calibration

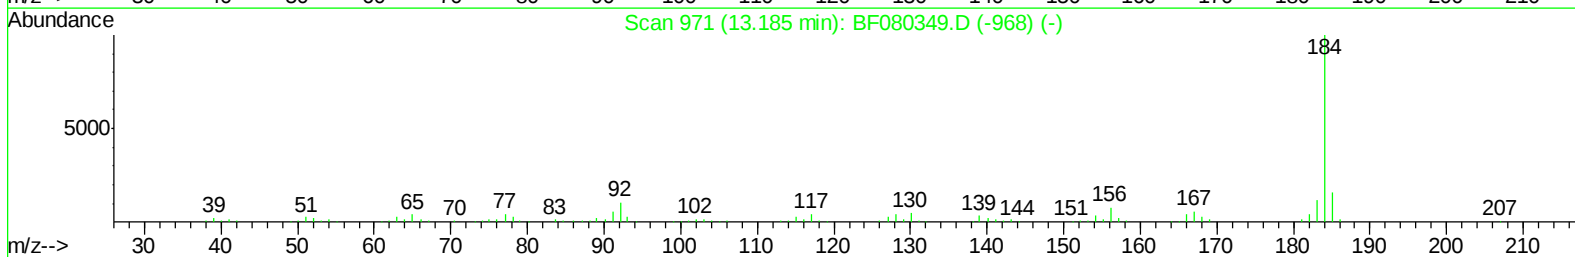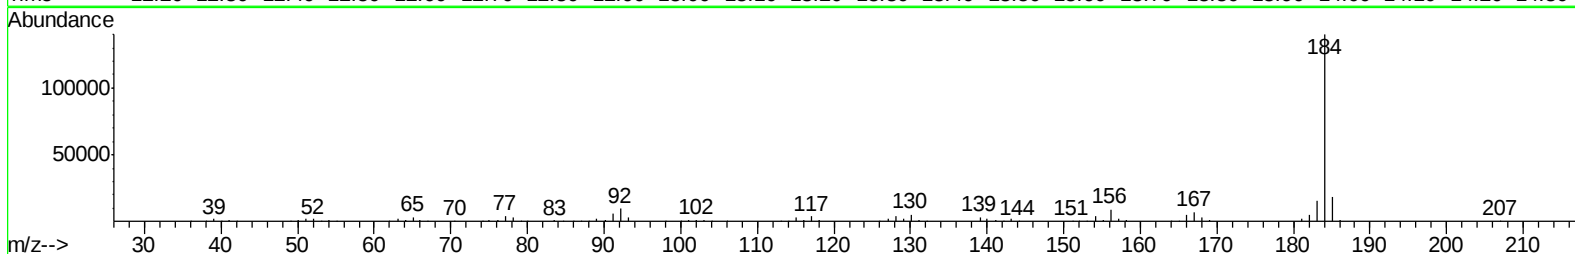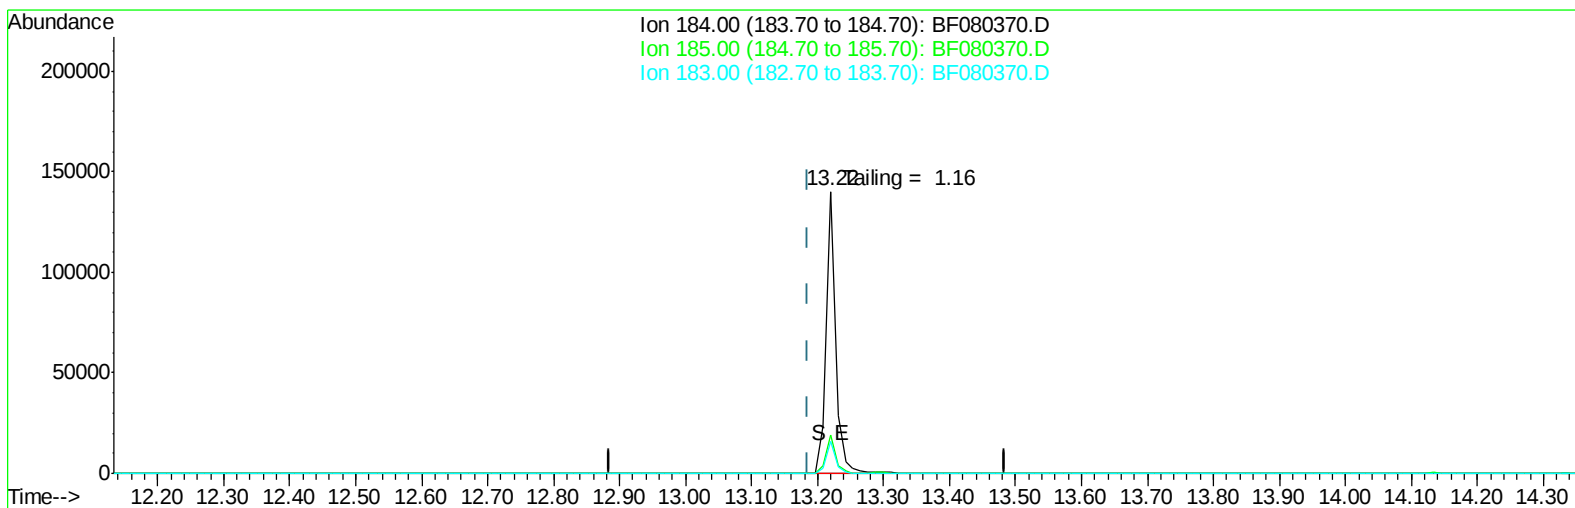

TIC: BF080370.D

(76) Benzidine

13.219min (+0.034) 0.00ng

response 141218

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.47
183.00	11.50	11.42
0.00	0.00	0.00