


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070715\
 Data File : BF080370.D
 Acq On : 7 Jul 2015 11:15
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 03:05:40 2015

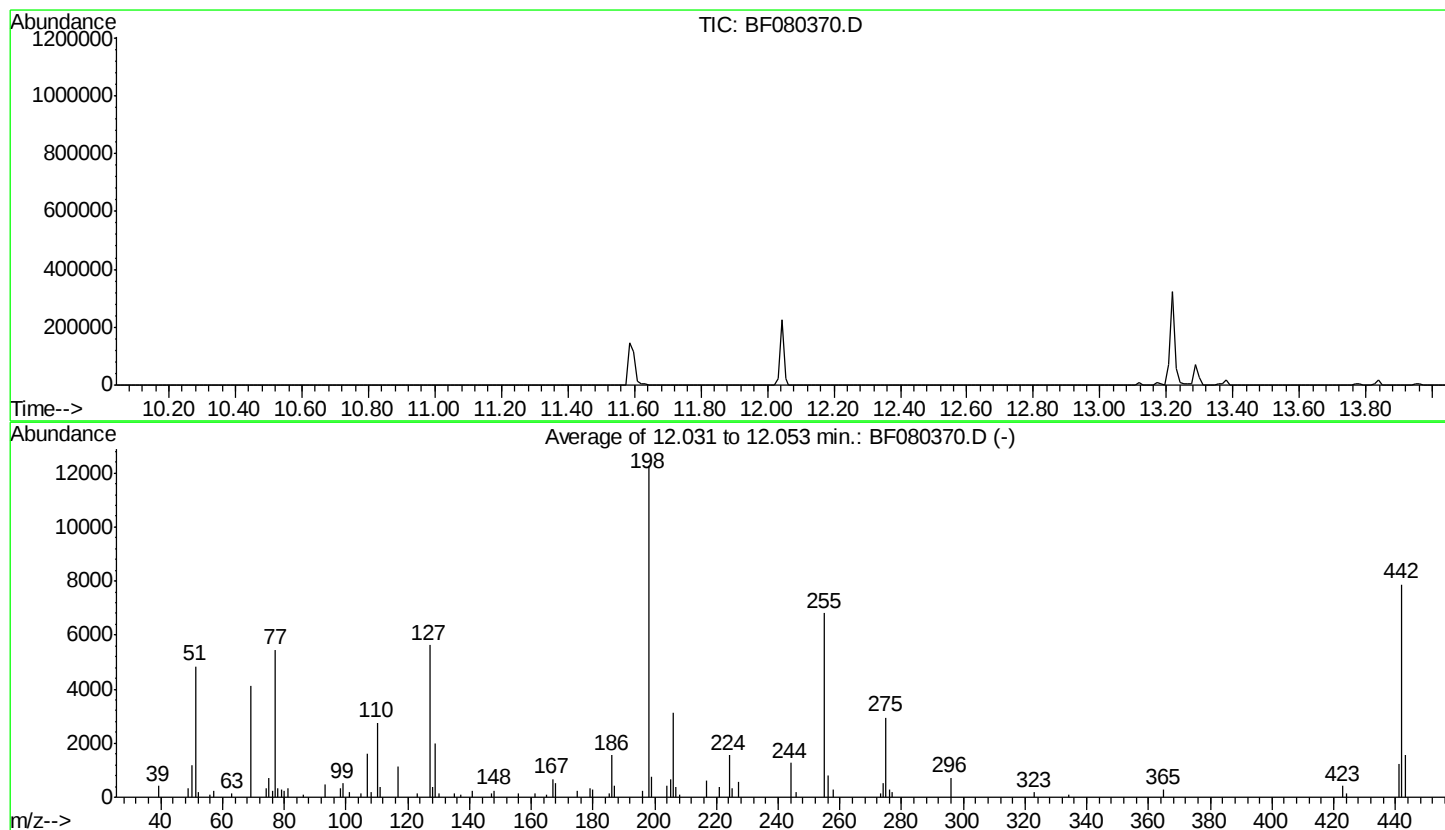

AutoFind: Scans 870, 871, 872; Background Corrected with Scan 867

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	4856	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.6	4126	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	5627	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12271	PASS
199	198	5	9	6.1	751	PASS
275	198	10	60	24.0	2944	PASS
365	198	1	100	2.1	263	PASS
441	442	0.01	24	15.7	1234	PASS
442	198	50	100	64.2	7877	PASS
443	442	15	24	19.7	1551	PASS