

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
 Data File : BF088809.D
 Acq On : 8 Jul 2016 6:25
 Operator : UM/SJ
 Sample : H3897-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-04-COMP

Quant Time: Jul 08 06:56:12 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:56:42 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	88953	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	302777	20.00	ng	-0.01
38) Acenaphthene-d10	9.78	164	124001	20.00	ng	0.00
63) Phenanthrene-d10	11.26	188	200676	20.00	ng	0.00
75) Chrysene-d12	13.89	240	186488	20.00	ng	0.00
86) Perylene-d12	15.27	264	136469	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	435698	73.41	ng	0.01
7) Phenol-d6	6.39	99	634477	82.73	ng	0.00
23) Nitrobenzene-d5	7.30	82	322159	55.76	ng	-0.01
41) 2,4,6-Tribromophenol	10.56	330	87758	76.21	ng	-0.01
44) 2-Fluorobiphenyl	9.11	172	584163	74.41	ng	0.00
78) Terphenyl-d14	12.85	244	407824	48.71	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.30	70	42050	8.16	ng	# 73
25) Isophorone	7.30	82	290225	27.12	ng	# 65
49) Dimethylphthalate	9.50	163	59326	6.72	ng	99
56) 2,4-Dinitrotoluene	9.78	165	15351	6.00	ng	# 36
66) 4-Bromophenyl-phenylether	10.56	248	5723	2.83	ng	# 1
83) Bis(2-ethylhexyl)phthalate	13.89	149	24652	3.06	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
Data File : BF088809.D
Acq On : 8 Jul 2016 6:25
Operator : UM/SJ
Sample : H3897-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-04-COMP

Quant Time: Jul 08 06:56:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:56:42 2016
Response via : Initial Calibration

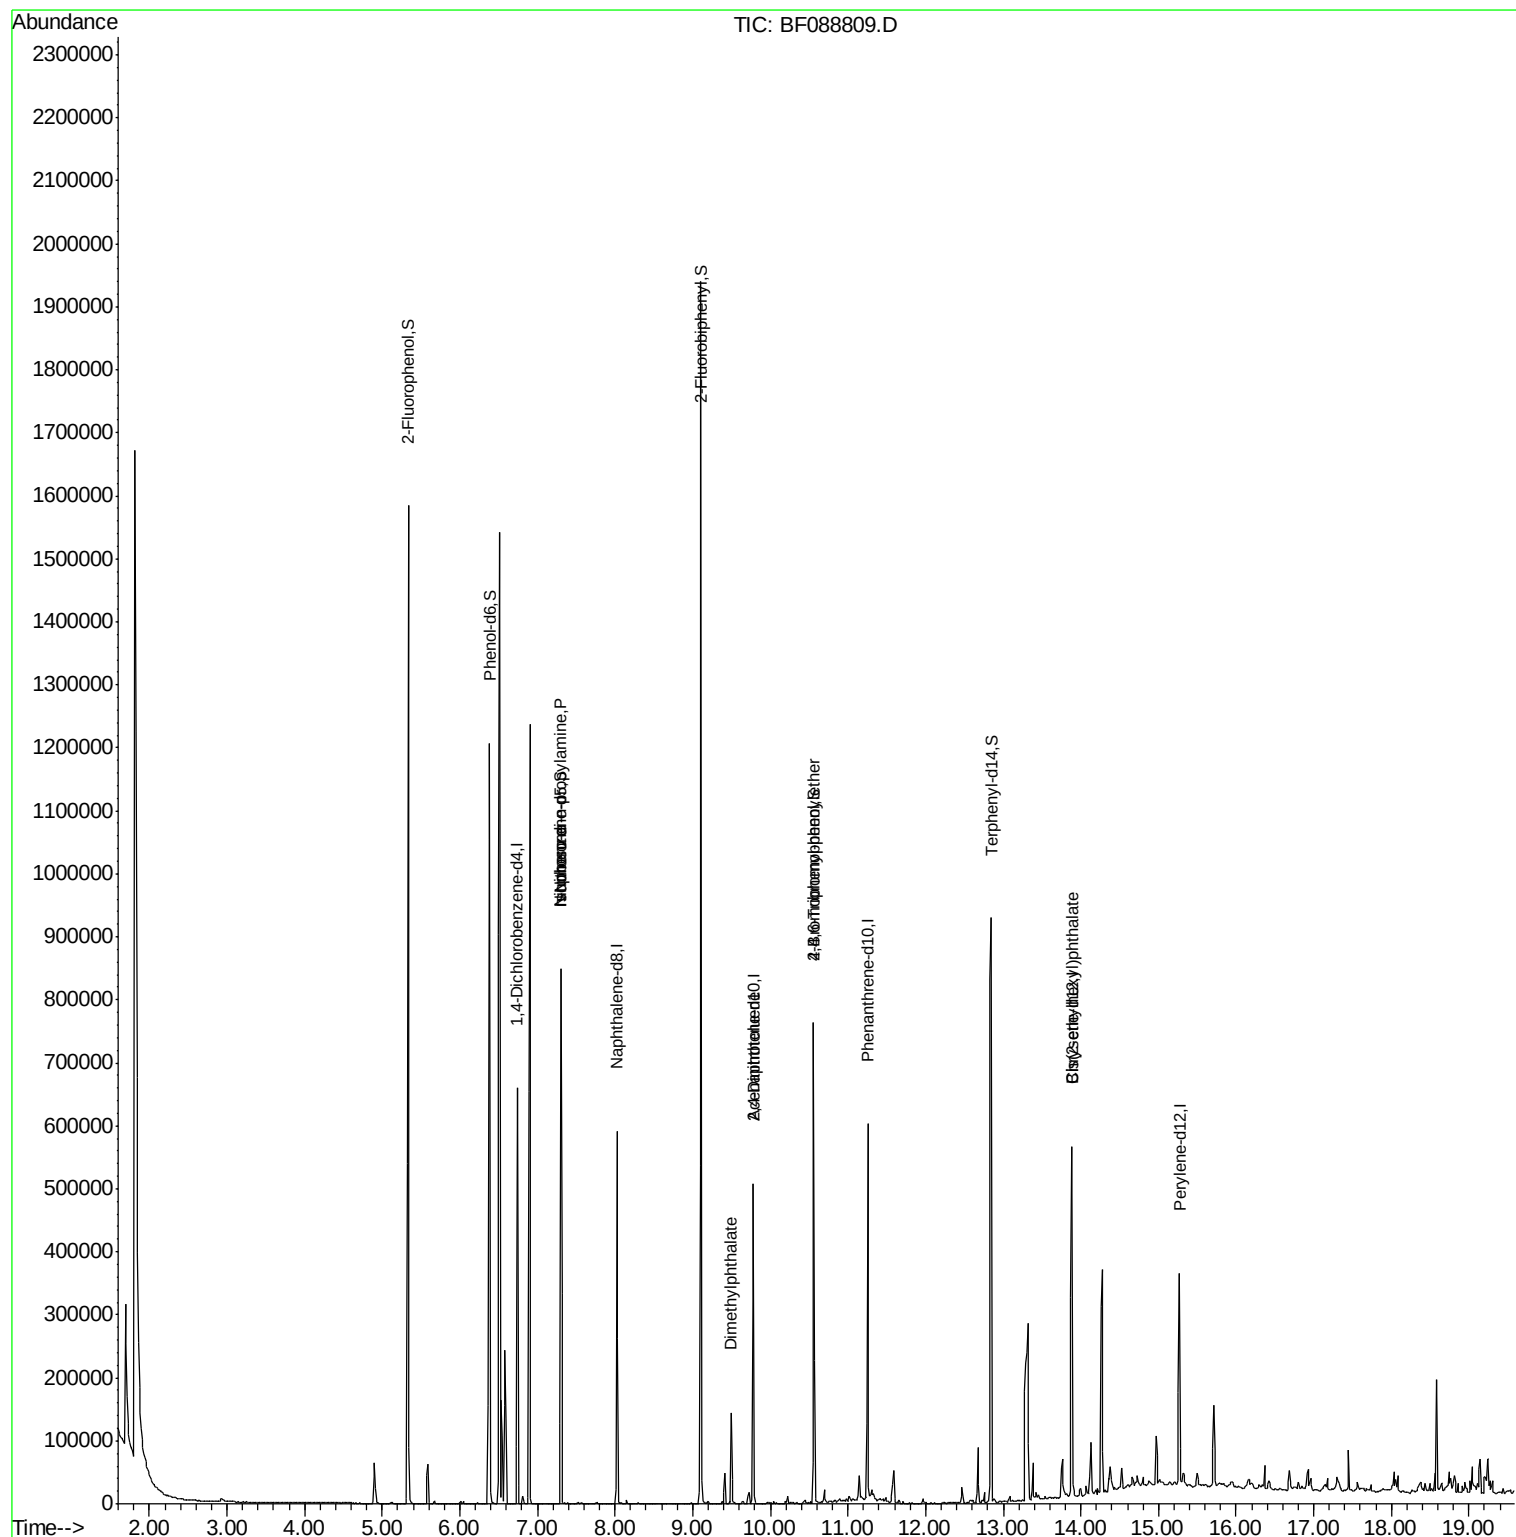

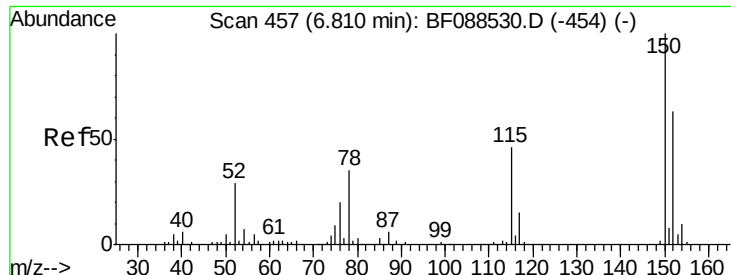

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 451

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Instrument :

BNA_F

ClientSampleId :

SB-04-COMP


Tgt Ion:152 Resp: 88953

Ion Ratio Lower Upper

152 100

150 154.0 123.8 185.6




115 65.3 39.6 59.4#

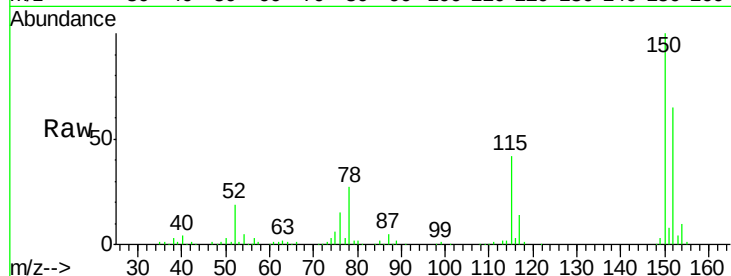

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

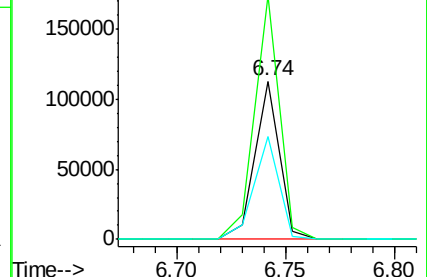

#5

2-Fluorophenol

Concen: 73.41 ng

RT: 5.34 min Scan# 328

Delta R.T. 0.01 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25


Tgt Ion:112 Resp: 435698

Ion Ratio Lower Upper

112 100

64 58.7 42.2 63.2



63 31.0 21.8 32.8




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

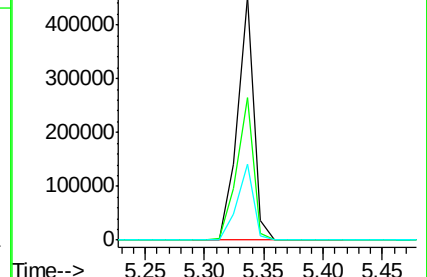

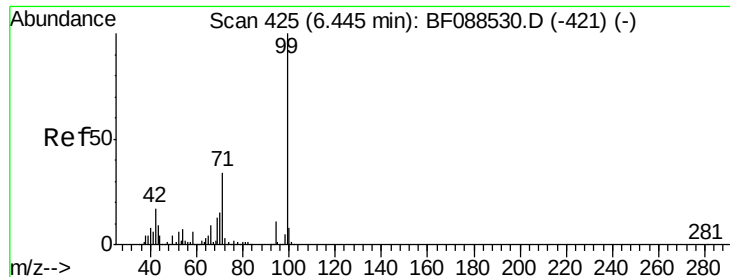

#7

Phenol-d6

Concen: 82.73 ng

RT: 6.39 min Scan# 420

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Instrument :

BNA_F

ClientSampleId :

SB-04-COMP





Tgt Ion: 99 Resp: 634477

Ion Ratio Lower Upper

99 100

42 12.3 12.2 18.2

71 31.5 23.4 35.0

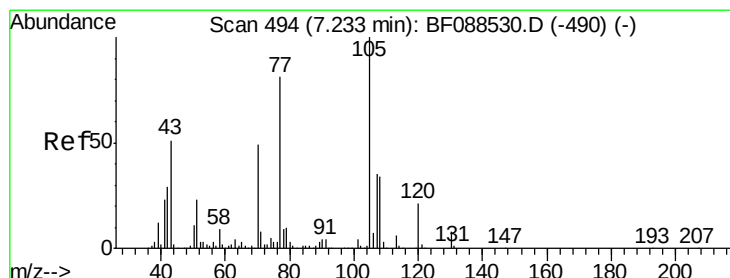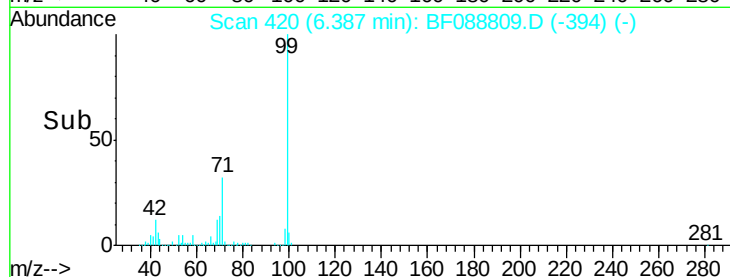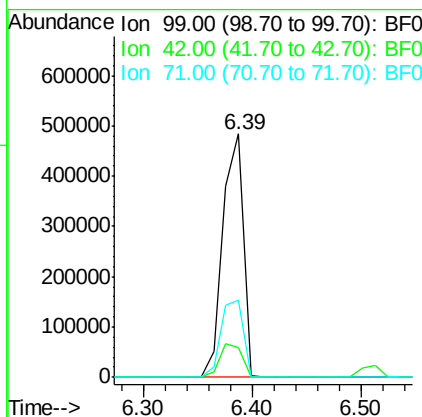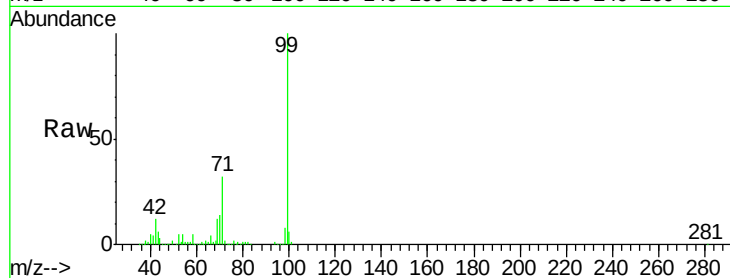

#19

n-Nitroso-di-n-propylamine

Concen: 8.16 ng

RT: 7.30 min Scan# 500

Delta R.T. 0.13 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Tgt Ion: 70 Resp: 42050




Ion Ratio Lower Upper


70 100

42 43.7 49.6 74.4#

101 0.0 7.1 10.7#

130 1.8 15.4 23.2#

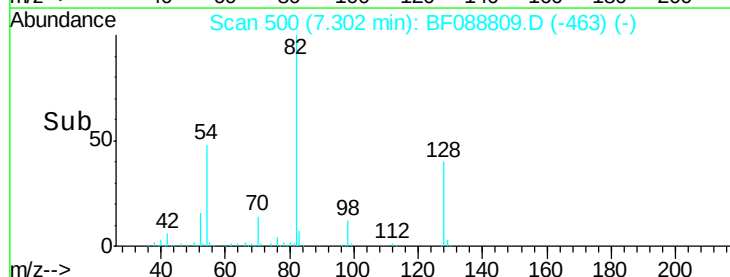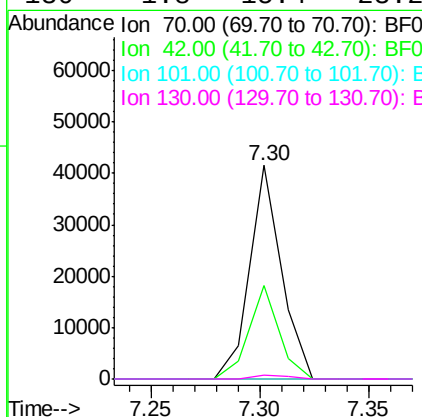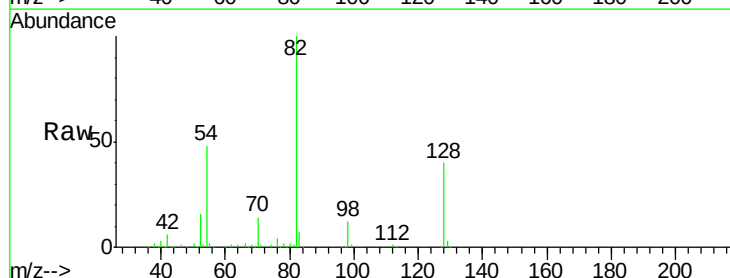







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.02 min Scan# 563
Delta R.T. -0.01 min
Lab File: BF088809.D
Acq: 8 Jul 2016 6:25

Instrument :
BNA_F
ClientSampleId :
SB-04-COMP

Tgt Ion:	136	Resp:	302777
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.1	13.7
54	9.2	6.6	10.0
68	7.3	5.1	7.7

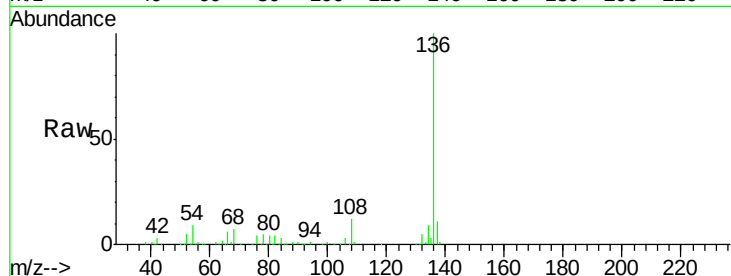


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

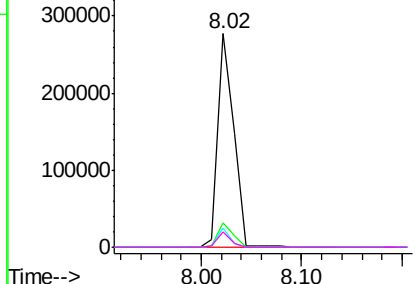




#23
Nitrobenzene-d5
Concen: 55.76 ng
RT: 7.30 min Scan# 500
Delta R.T. -0.01 min
Lab File: BF088809.D
Acq: 8 Jul 2016 6:25

Tgt Ion:	82	Resp:	322159
Ion	Ratio	Lower	Upper
82	100		
128	39.5	35.9	53.9
54	48.0	40.9	61.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

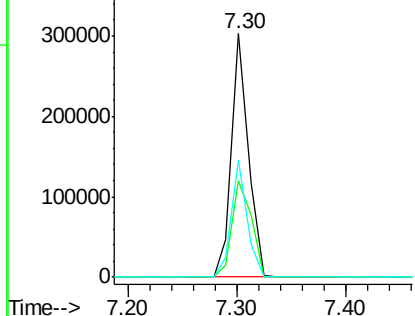



#25

Isophorone

Concen: 27.12 ng

RT: 7.30 min Scan# 500

Delta R.T. -0.27 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Instrument :

BNA_F

ClientSampleId :

SB-04-COMP





Tgt Ion: 82 Resp: 290225

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#

138 0.0 14.6 21.8#

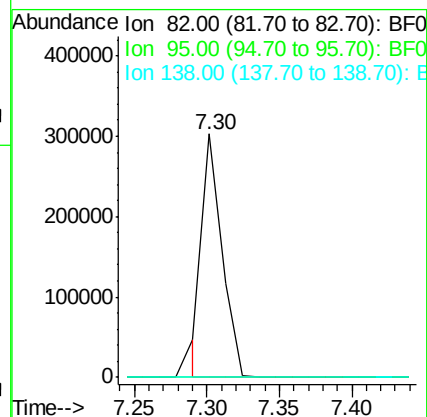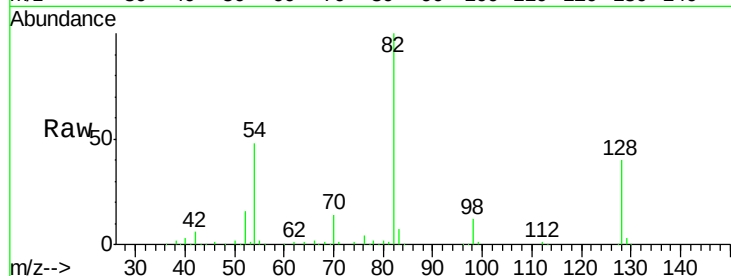

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.78 min Scan# 717

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25




Tgt Ion: 164 Resp: 124001


Ion Ratio Lower Upper

164 100

162 106.5 85.4 128.2

160 49.1 39.5 59.3

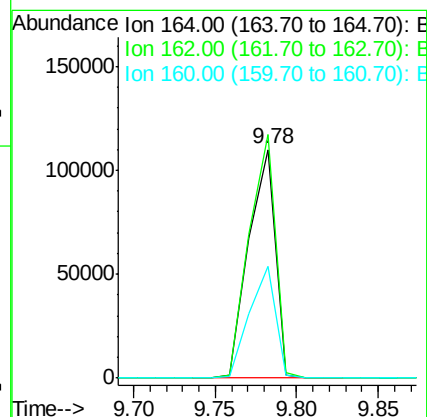


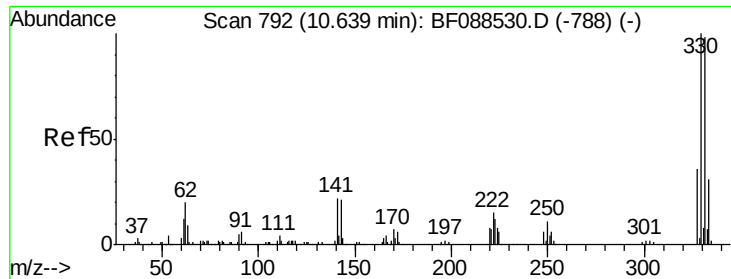




#41
 2,4,6-Tribromophenol
 Concen: 76.21 ng
 RT: 10.56 min Scan# 785
 Delta R.T. -0.01 min
 Lab File: BF088809.D
 Acq: 8 Jul 2016 6:25

Instrument :
 BNA_F
 ClientSampleId :
 SB-04-COMP

Tgt Ion:330 Resp: 87758
 Ion Ratio Lower Upper
 330 100
 332 96.1 0.0 0.0#
 141 38.9 0.0 0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

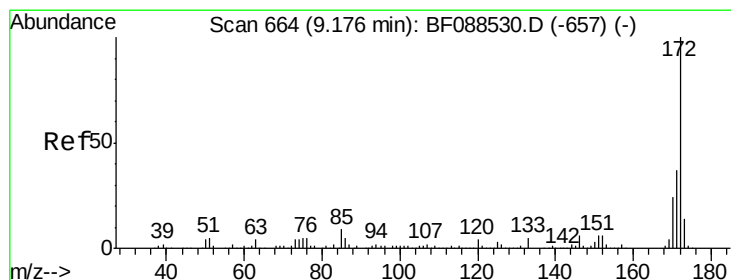
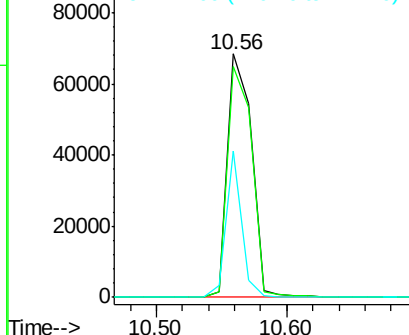



#44
 2-Fluorobiphenyl
 Concen: 74.41 ng
 RT: 9.11 min Scan# 658
 Delta R.T. 0.00 min
 Lab File: BF088809.D
 Acq: 8 Jul 2016 6:25

Tgt Ion:172 Resp: 584163
 Ion Ratio Lower Upper
 172 100
 171 36.1 28.6 43.0
 170 24.0 19.2 28.8

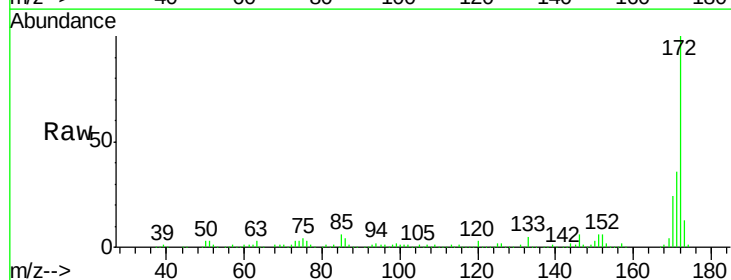

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

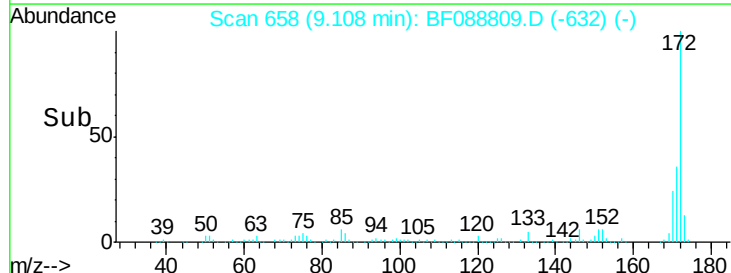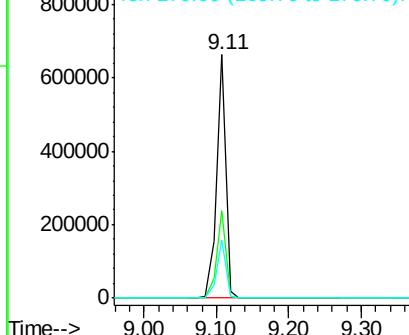



#49

Dimethylphthalate

Concen: 6.72 ng

RT: 9.50 min Scan# 692

Delta R.T. -0.02 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Instrument :

BNA_F

ClientSampleId :

SB-04-COMP


Tgt Ion:163 Resp: 59326

Ion Ratio Lower Upper

163 100

194 3.0 2.8 4.2




164 10.3 8.3 12.5



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

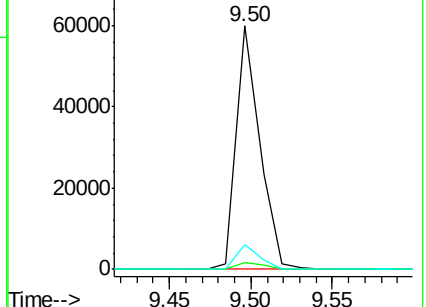

#56

2,4-Dinitrotoluene

Concen: 6.00 ng

RT: 9.78 min Scan# 717

Delta R.T. -0.19 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Tgt Ion:165 Resp: 15351


Ion Ratio Lower Upper

165 100

63 0.0 22.0 33.0#

89 0.0 41.1 61.7#

182 0.0 2.0 3.0#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

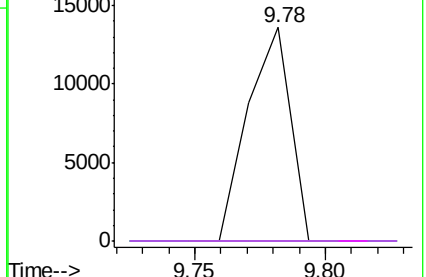


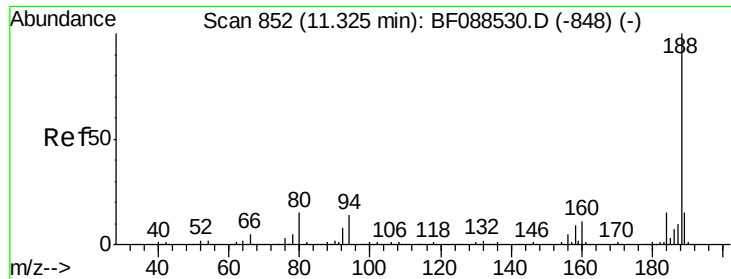




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.26 min Scan# 846
Delta R.T. 0.00 min
Lab File: BF088809.D
Acq: 8 Jul 2016 6:25

Instrument :
BNA_F
ClientSampleId :
SB-04-COMP

Tgt Ion:188 Resp: 200676
Ion Ratio Lower Upper
188 100
94 9.0 9.0 13.6
80 9.8 10.0 15.0#




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

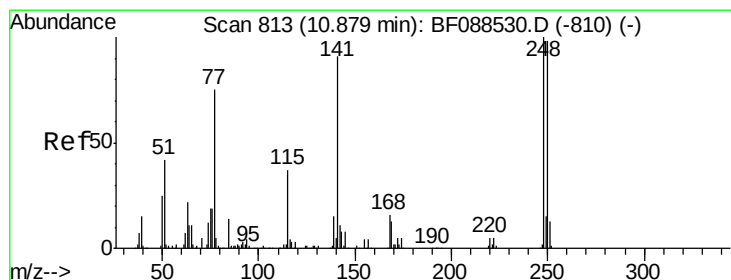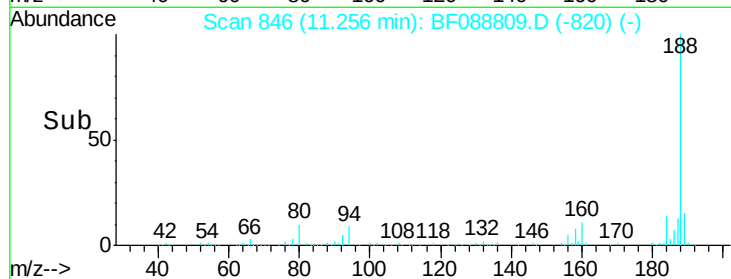
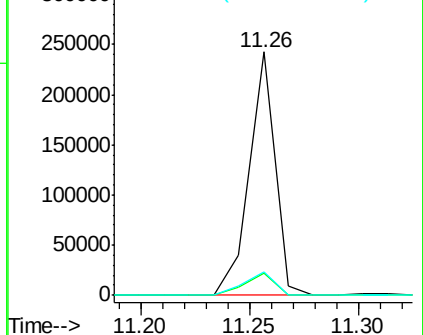



#66
4-Bromophenyl-phenylether
Concen: 2.83 ng
RT: 10.56 min Scan# 785
Delta R.T. -0.25 min
Lab File: BF088809.D
Acq: 8 Jul 2016 6:25

Tgt Ion:248 Resp: 5723
Ion Ratio Lower Upper
248 100
250 192.2 77.1 115.7#
141 680.9 50.6 76.0#

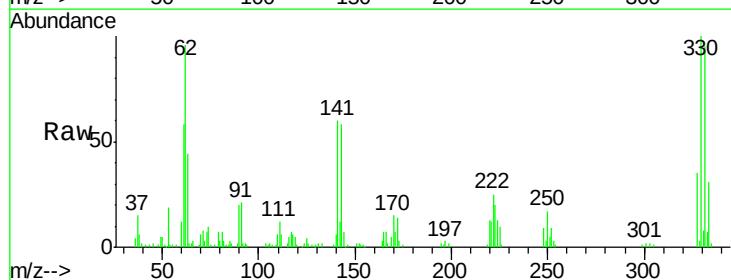

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

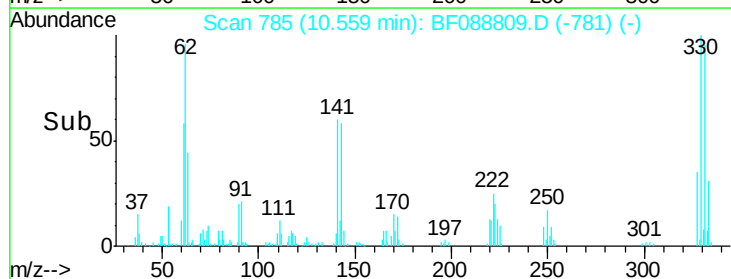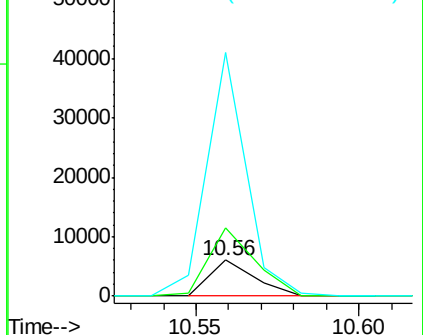

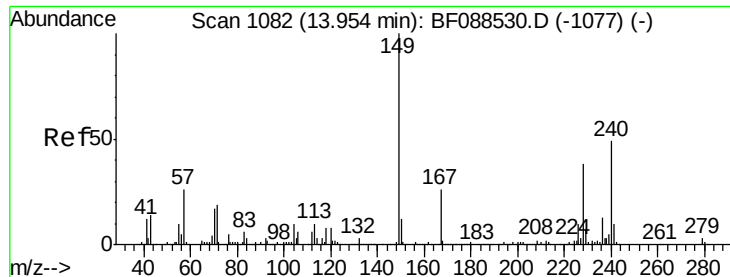

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.89 min Scan# 1076

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Instrument :

BNA_F

ClientSampleId :

SB-04-COMP


Tgt Ion:240 Resp: 186488

Ion Ratio Lower Upper

240 100

120 8.6 6.8 10.2




236 25.7 20.2 30.2

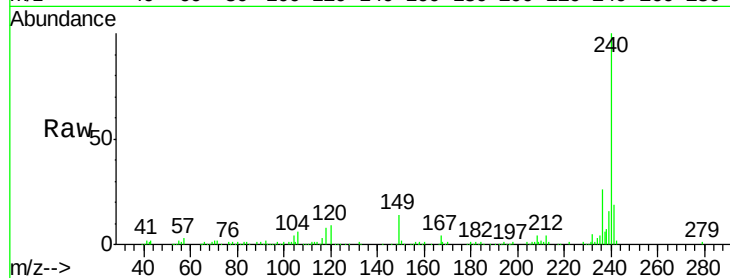

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

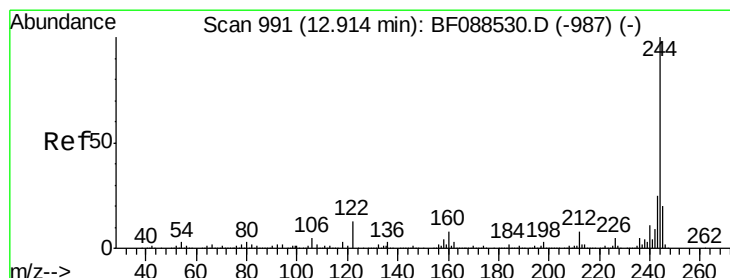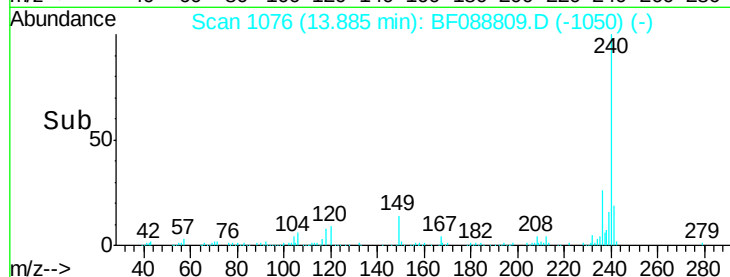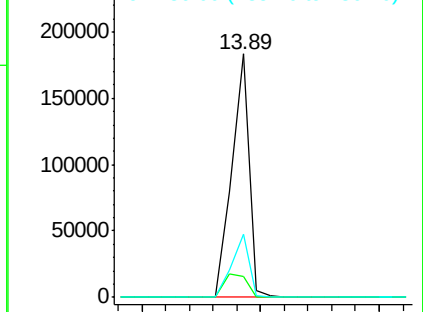

#78

Terphenyl-d14

Concen: 48.71 ng

RT: 12.85 min Scan# 985

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25


Tgt Ion:244 Resp: 407824

Ion Ratio Lower Upper

244 100

212 6.5 6.0 9.0



122 6.8 11.2 16.8#

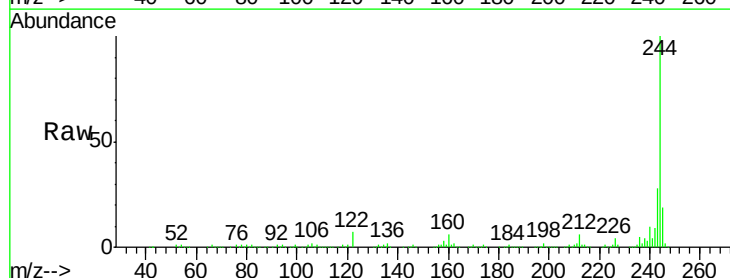


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

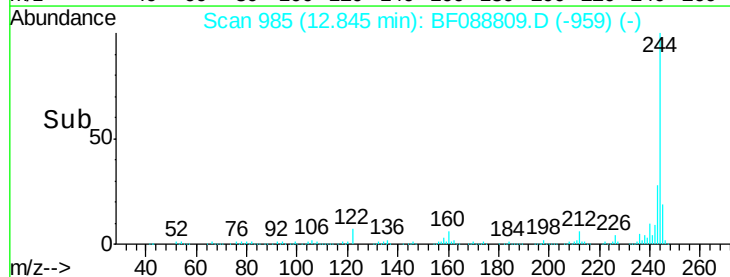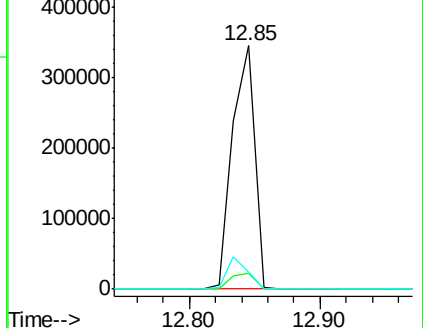

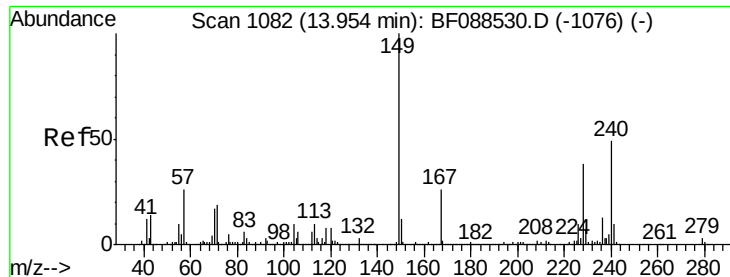

#83

Bis(2-ethylhexyl)phthalate

Concen: 3.06 ng

RT: 13.89 min Scan# 1076

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25

Instrument :

BNA_F

ClientSampleId :

SB-04-COMP


Tgt Ion:149 Resp: 24652

Ion Ratio Lower Upper

149 100

167 26.3 20.5 30.7




279 4.0 2.0 3.0#

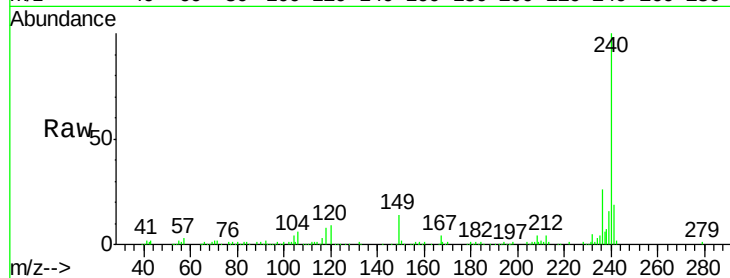

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

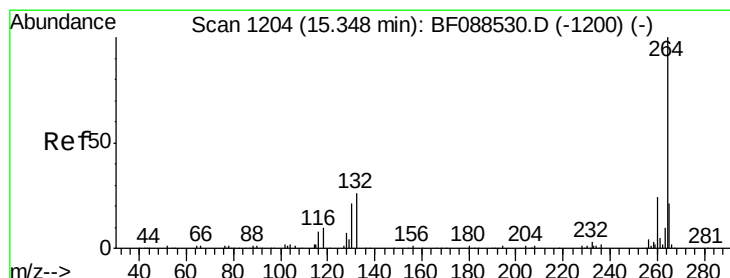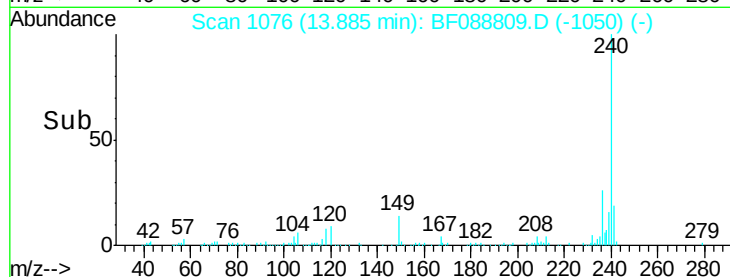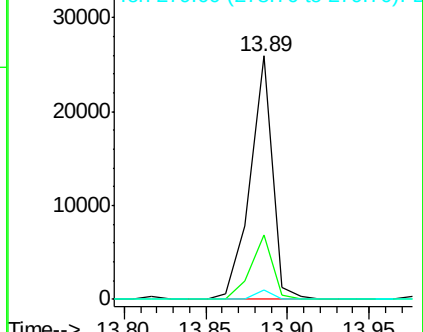

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.27 min Scan# 1197

Delta R.T. 0.00 min

Lab File: BF088809.D

Acq: 8 Jul 2016 6:25


Tgt Ion:264 Resp: 136469

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 21.8 16.9 25.3

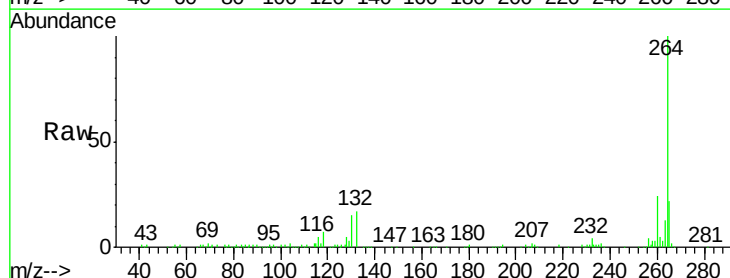

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

