
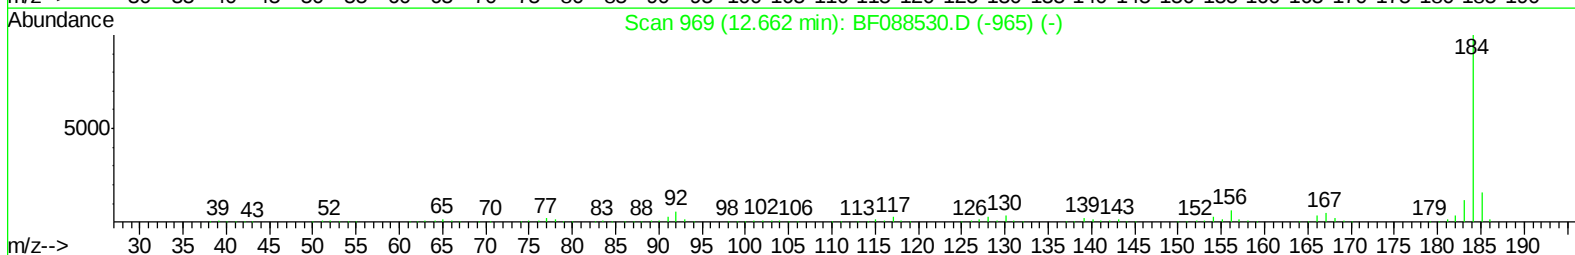
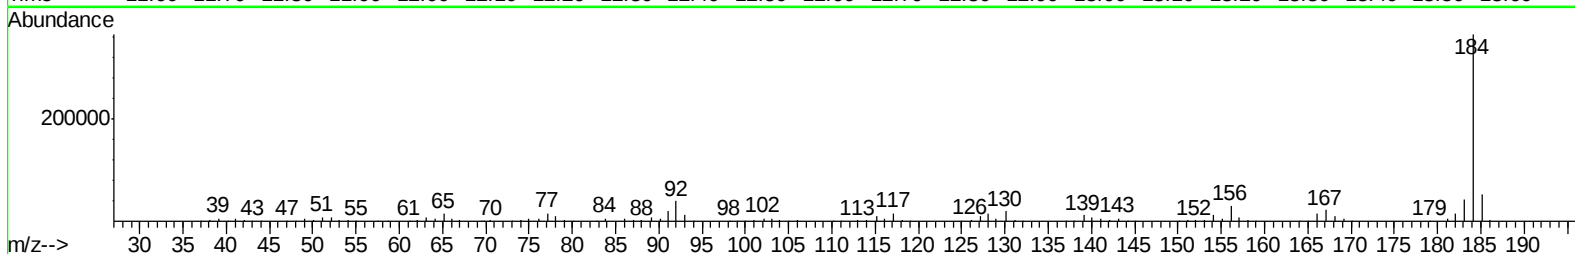


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
Data File : BF088772.D
Acq On : 7 Jul 2016 10:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:37:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:56:42 2016
Response via : Initial Calibration

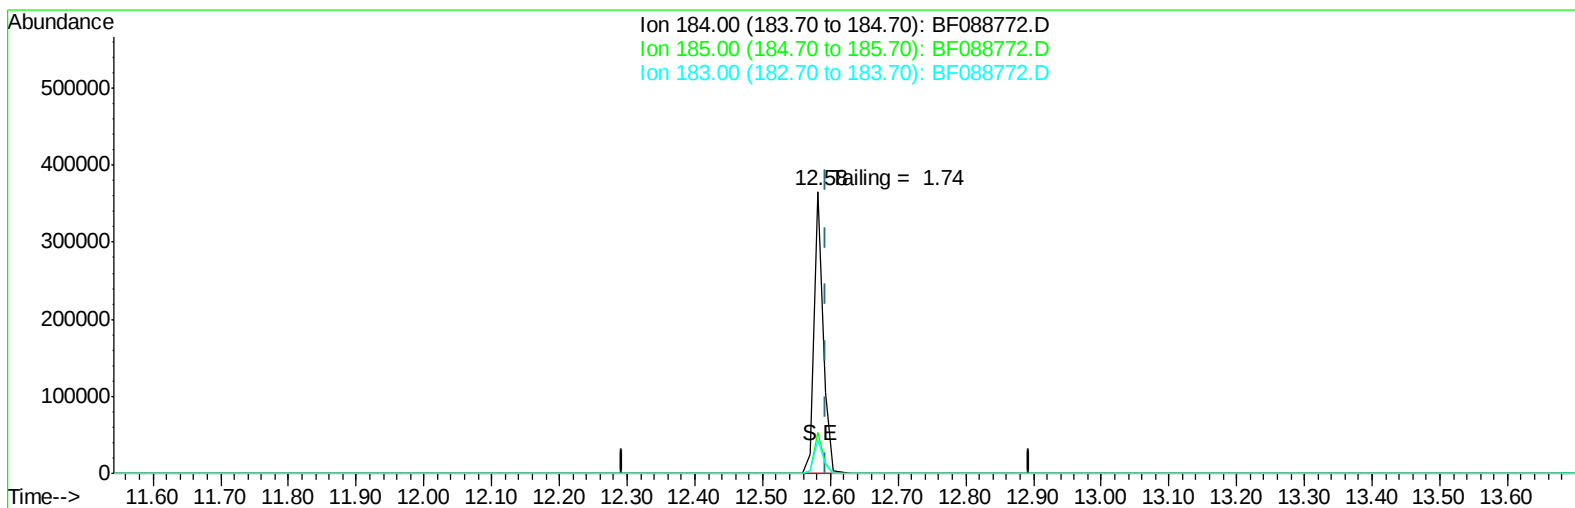

TIC: BF088772.D

(76) Benzidine




12.582min (-0.011) 0.00ng

response 345732

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.70
183.00	11.60	12.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
Data File : BF088772.D
Acq On : 7 Jul 2016 10:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:37:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:56:42 2016
Response via : Initial Calibration

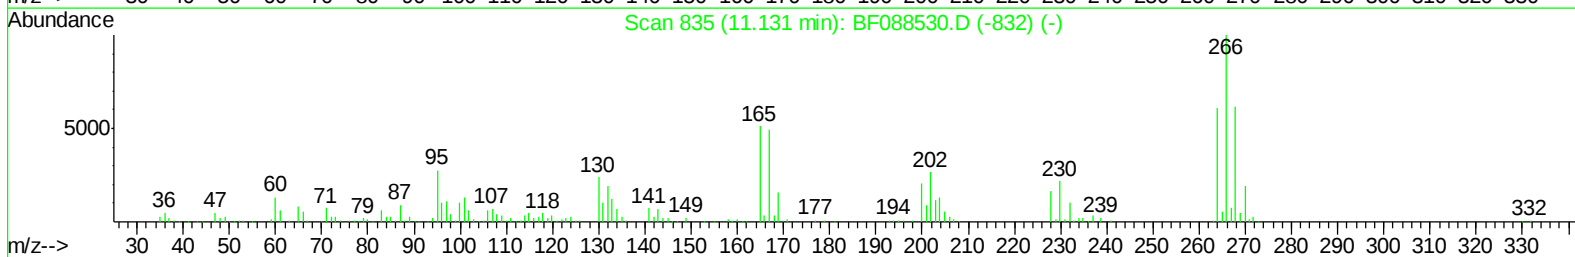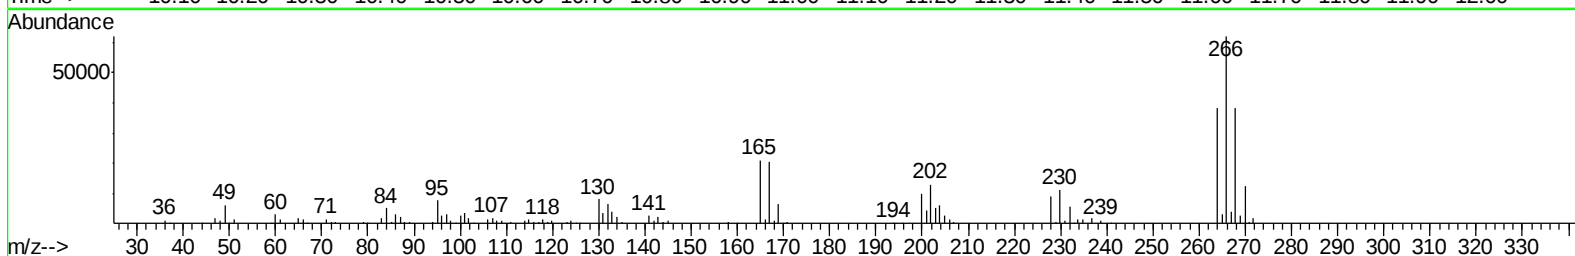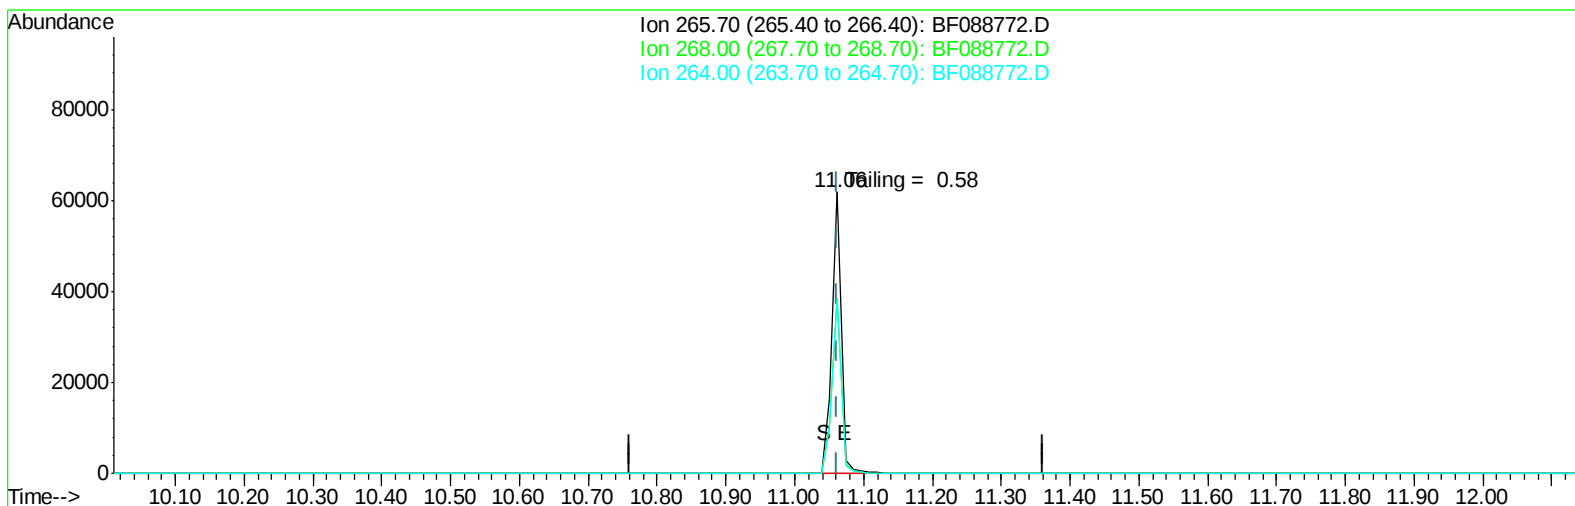

TIC: BF088772.D

(69) Pentachlorophenol (C)

11.062min (+0.000) 0.00ng

response 57284

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	62.13
264.00	62.00	61.65
0.00	0.00	0.00