

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070716\
 Data File : BF088816.D
 Acq On : 8 Jul 2016 9:48
 Operator : UM/SJ
 Sample : H3897-22
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP

Quant Time: Jul 08 13:22:24 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 05 17:15:08 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	85889	20.00	ng	-0.03
21) Naphthalene-d8	8.02	136	294385	20.00	ng	-0.05
38) Acenaphthene-d10	9.78	164	117376	20.00	ng	-0.03
63) Phenanthrene-d10	11.26	188	198418	20.00	ng	-0.03
75) Chrysene-d12	13.89	240	188849	20.00	ng	-0.03
86) Perylene-d12	15.27	264	141140	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	397378	69.34	ng	-0.03
7) Phenol-d6	6.38	99	431294	58.24	ng	-0.03
23) Nitrobenzene-d5	7.30	82	276621	49.24	ng	-0.05
41) 2,4,6-Tribromophenol	10.56	330	69903	64.13	ng	-0.05
44) 2-Fluorobiphenyl	9.11	172	524184	70.54	ng	-0.03
78) Terphenyl-d14	12.83	244	350884	41.38	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	9.51	163	440775	52.71	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070716\
Data File : BF088816.D
Acq On : 8 Jul 2016 9:48
Operator : UM/SJ
Sample : H3897-22
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-16-COMP

Quant Time: Jul 08 13:22:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

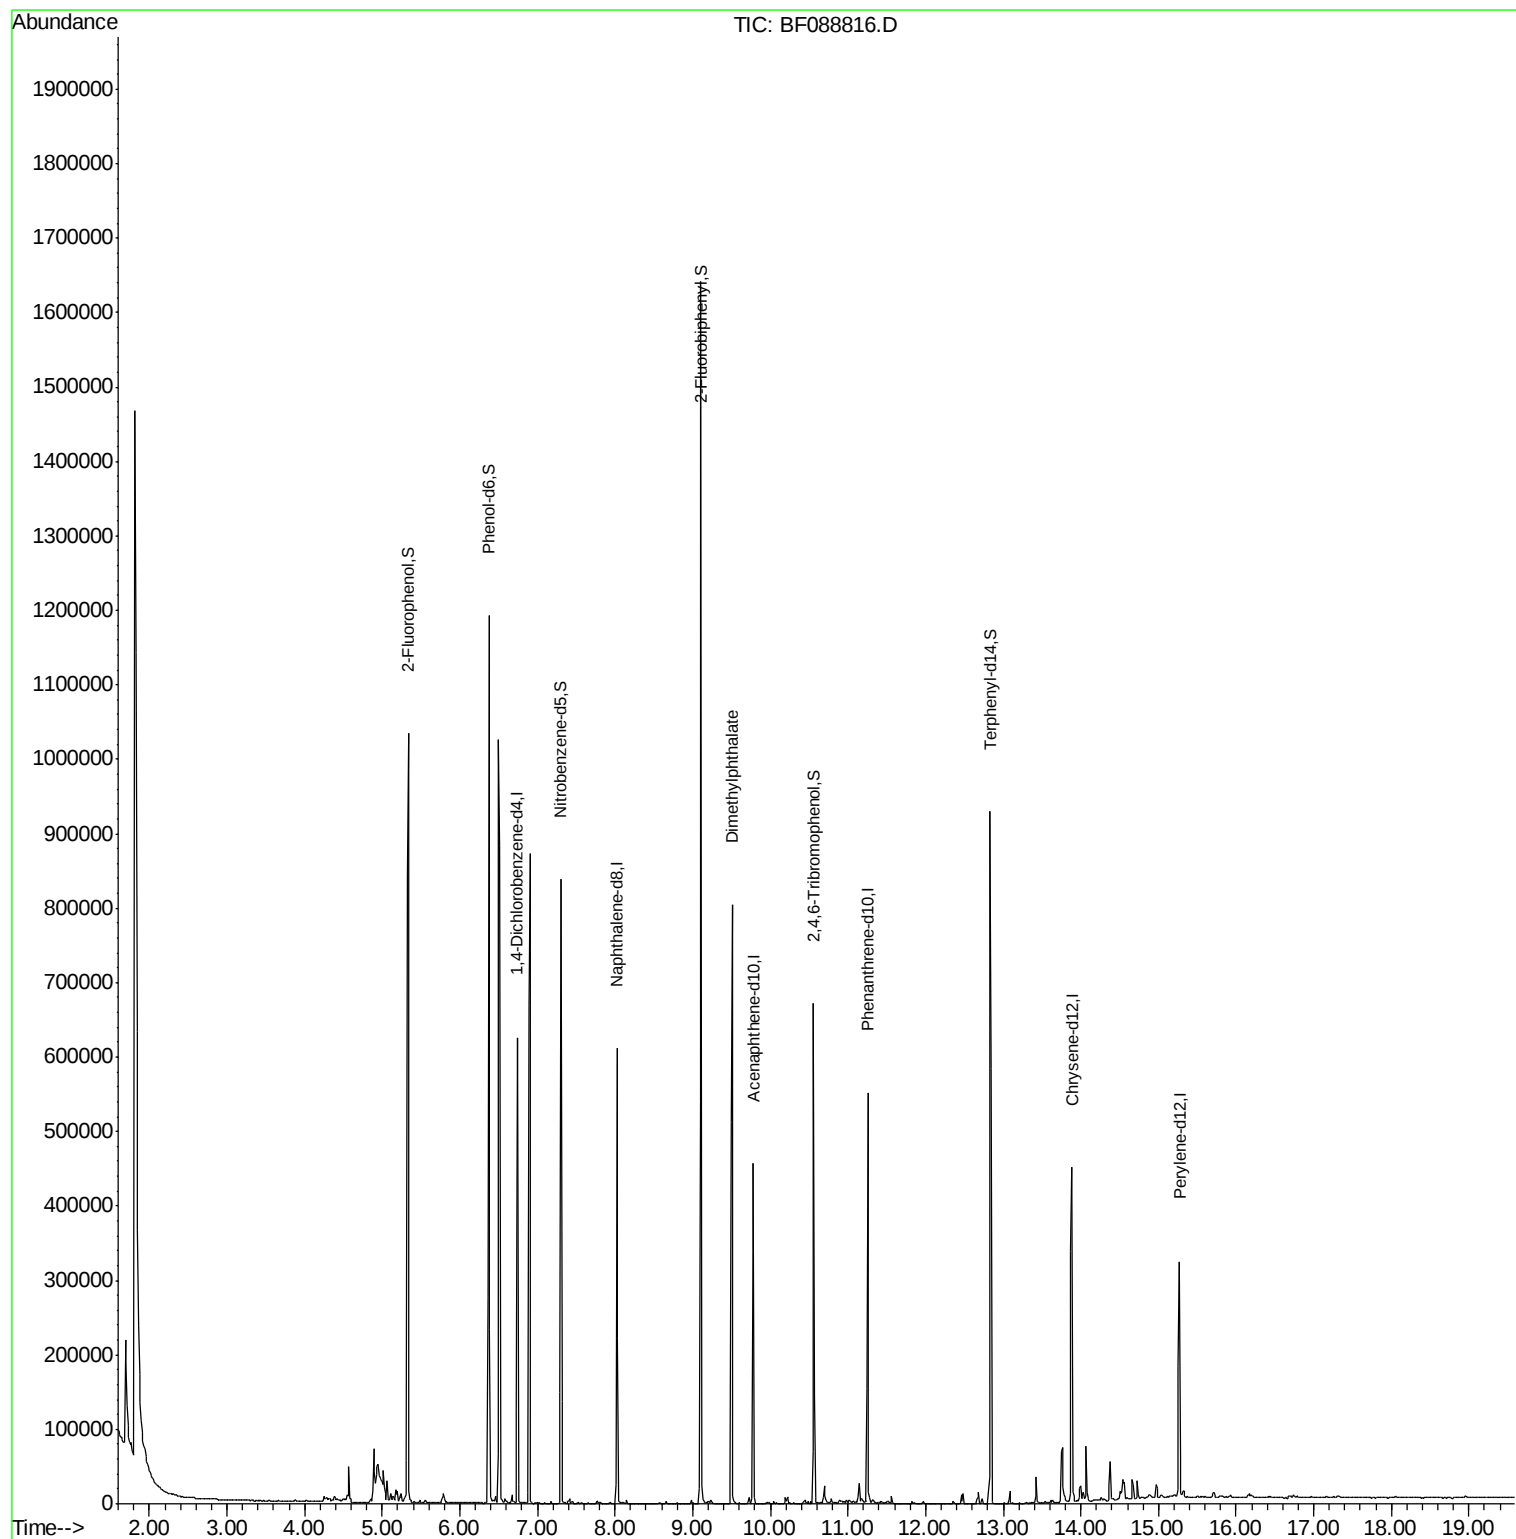

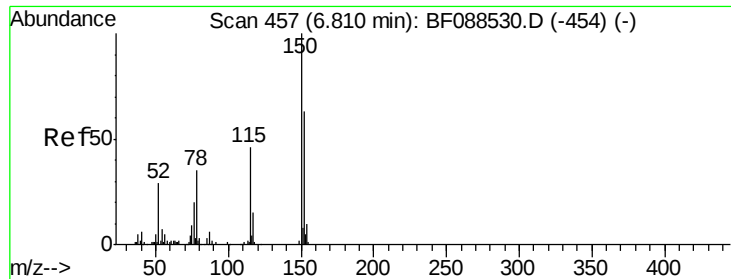

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 451

Delta R.T. -0.03 min

Lab File: BF088816.D

Acq: 8 Jul 2016 9:48

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tot Ion:152 Resp: 85889

Ion Ratio Lower Upper

152 100

150 156.2 123.8 185.6




115 64.6 39.6 59.4#

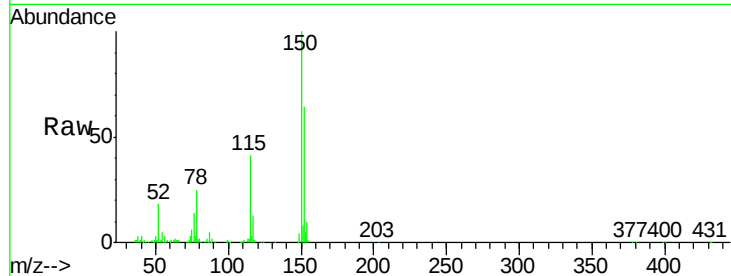

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

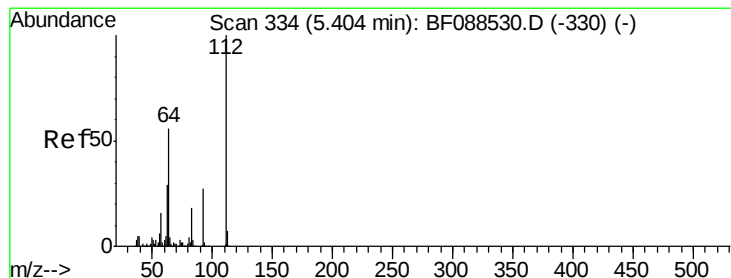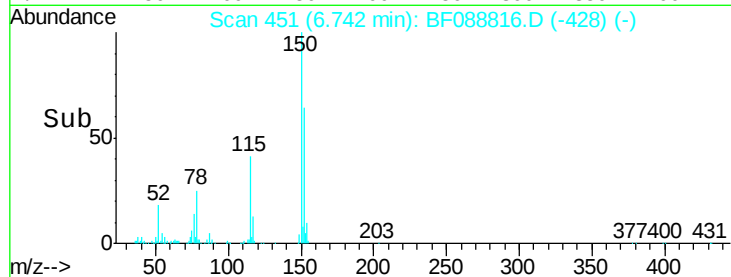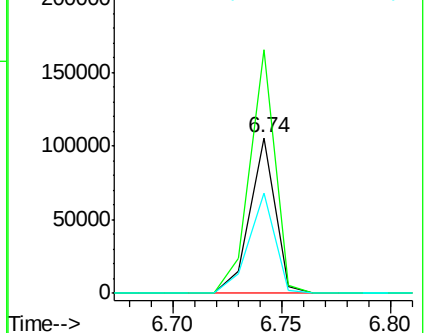

#5

2-Fluorophenol

Concen: 69.34 ng

RT: 5.34 min Scan# 328

Delta R.T. -0.03 min

Lab File: BF088816.D

Acq: 8 Jul 2016 9:48


Tgt Ion:112 Resp: 397378

Ion Ratio Lower Upper

112 100

64 48.6 42.2 63.2



63 25.3 21.8 32.8

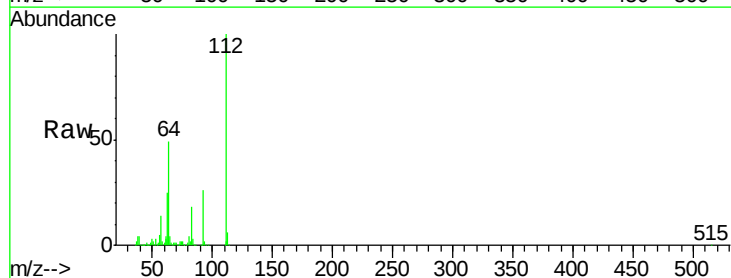

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

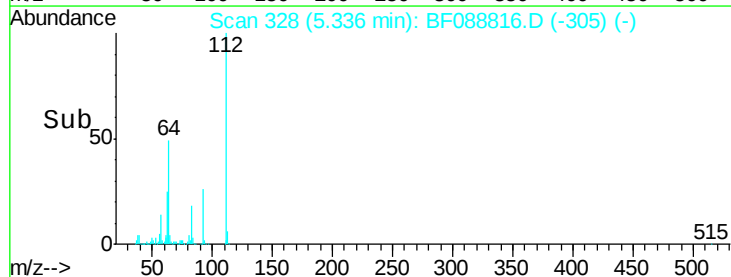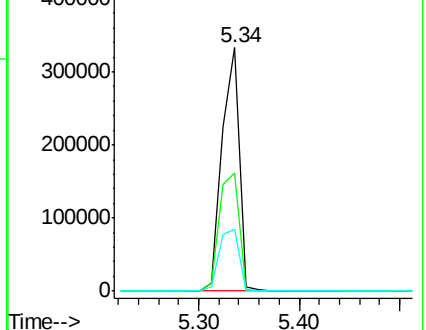



#7

Phenol-d6

Concen: 58.24 ng

RT: 6.38 min Scan# 419

Delta R.T. -0.03 min

Lab File: BF088816.D

Acq: 8 Jul 2016 9:48

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tot Ion: 99 Resp: 431294

Ion Ratio Lower Upper




99 100

42 17.7 12.2 18.2

71 37.2 23.4 35.0#

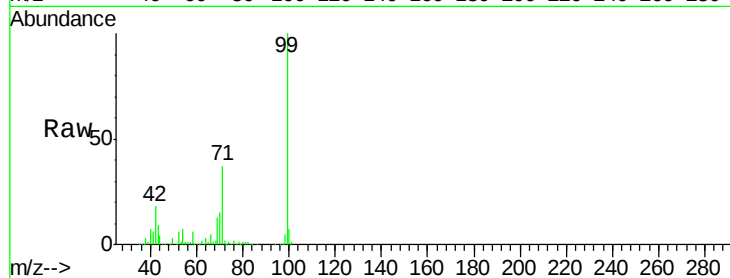

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

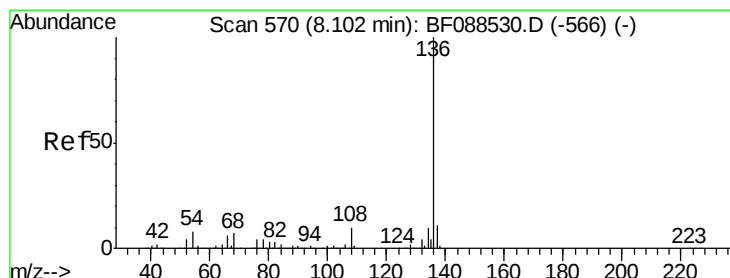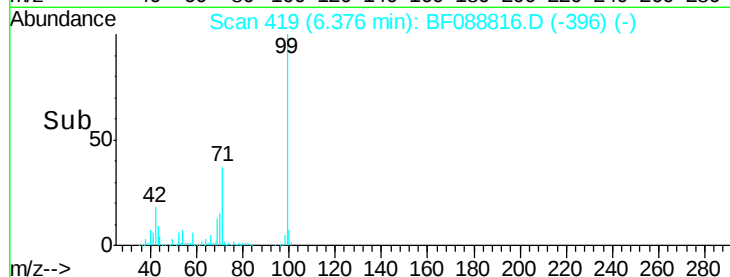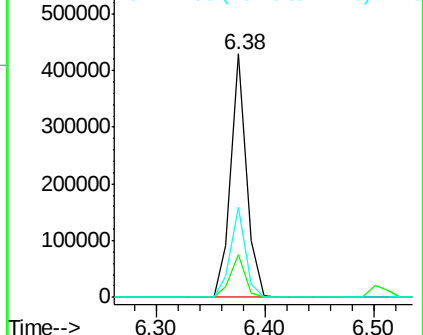

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.02 min Scan# 563

Delta R.T. -0.05 min

Lab File: BF088816.D

Acq: 8 Jul 2016 9:48

Tgt Ion: 136 Resp: 294385


Ion Ratio Lower Upper

136 100



137 11.1 9.1 13.7


54 9.1 6.6 10.0

68 7.0 5.1 7.7

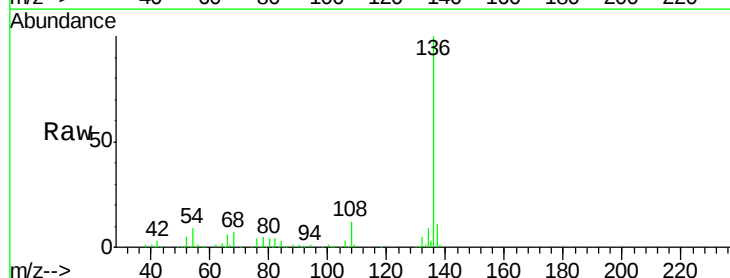

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0



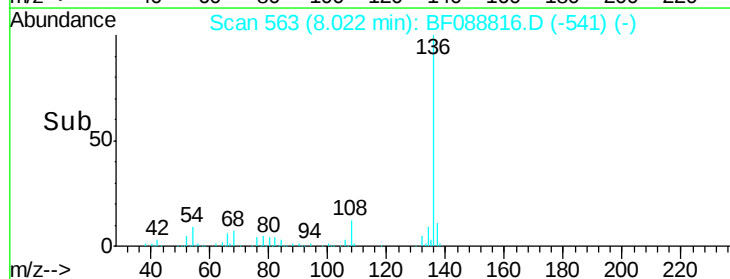
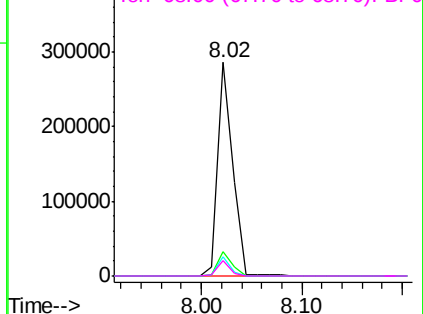


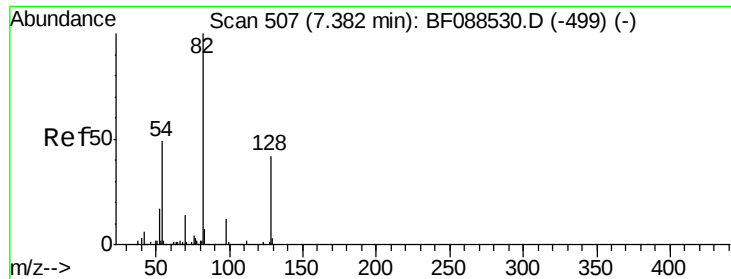

#23
 Nitrobenzene-d5
 Concen: 49.24 ng
 RT: 7.30 min Scan# 500
 Delta R.T. -0.05 min
 Lab File: BF088816.D
 Acq: 8 Jul 2016 9:48




Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP

Tot Ion	82	Resp	276621
Ion Ratio	Lower	Upper	
82	100		
128	39.6	35.9	53.9
54	47.6	40.9	61.3

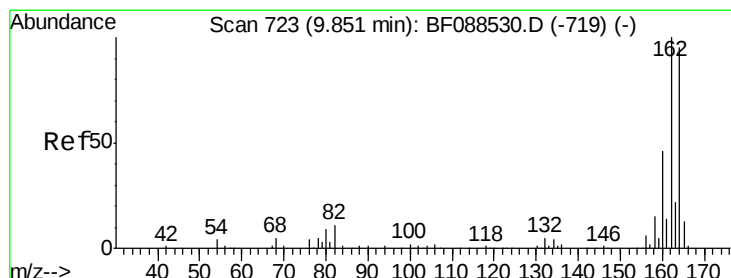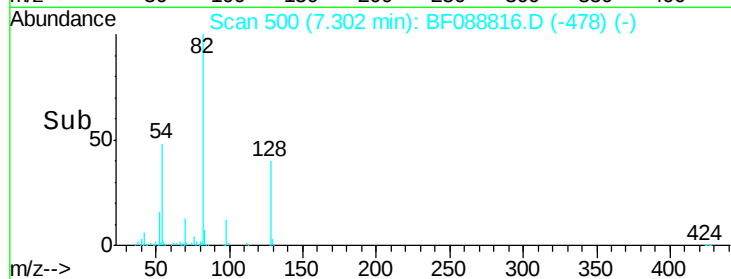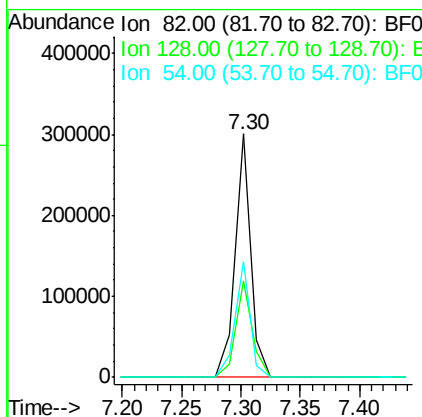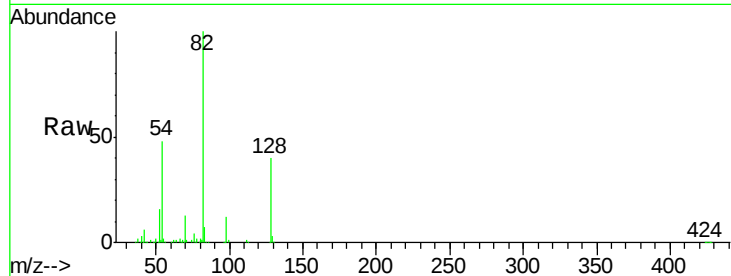

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.78 min Scan# 717
 Delta R.T. -0.03 min
 Lab File: BF088816.D
 Acq: 8 Jul 2016 9:48

Tgt Ion	164	Resp	117376
Ion Ratio	Lower	Upper	
164	100		
162	108.6	85.4	128.2
160	49.4	39.5	59.3

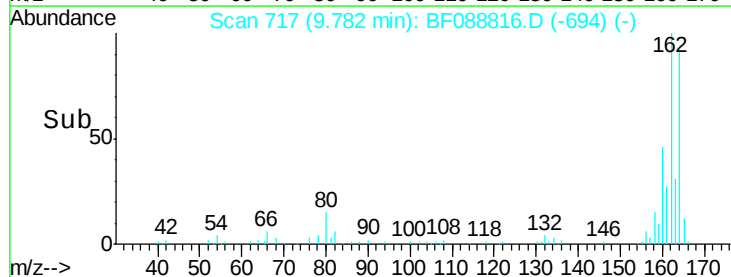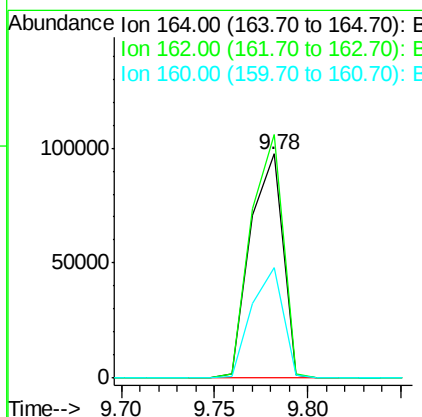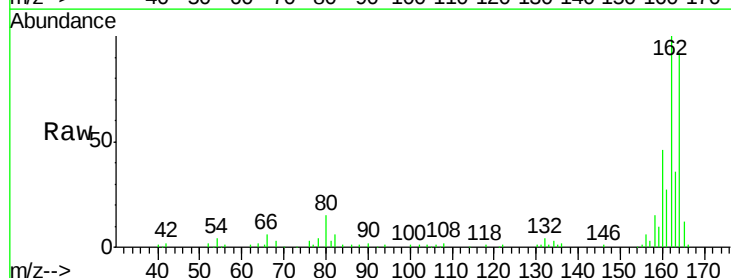







#41
 2,4,6-Tribromophenol
 Concen: 64.13 ng
 RT: 10.56 min Scan# 785
 Delta R.T. -0.05 min
 Lab File: BF088816.D
 Acq: 8 Jul 2016 9:48

Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP

Tot Ion:330 Resp: 69903
 Ion Ratio Lower Upper
 330 100
 332 97.7 0.0 0.0#
 141 43.2 0.0 0.0#

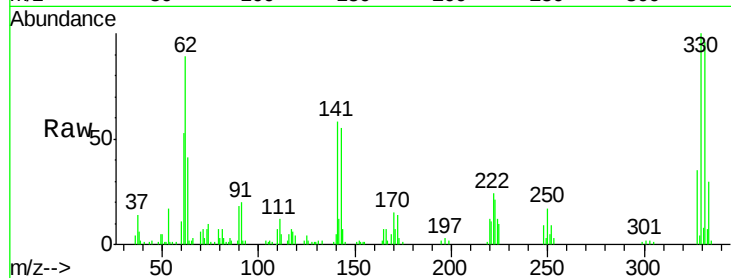


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

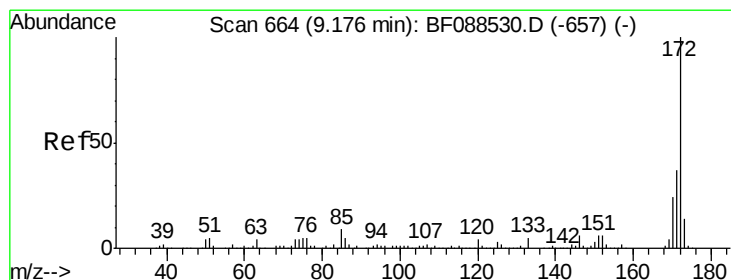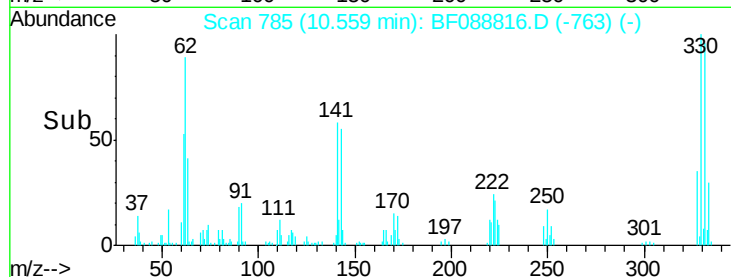
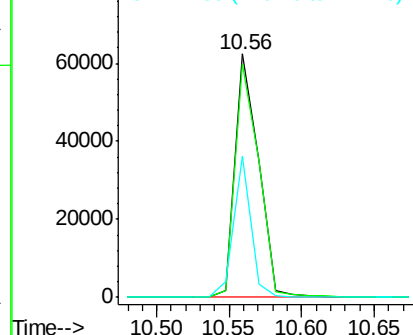



#44
 2-Fluorobiphenyl
 Concen: 70.54 ng
 RT: 9.11 min Scan# 658
 Delta R.T. -0.03 min
 Lab File: BF088816.D
 Acq: 8 Jul 2016 9:48

Tgt Ion:172 Resp: 524184
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 43.0
 170 23.5 19.2 28.8

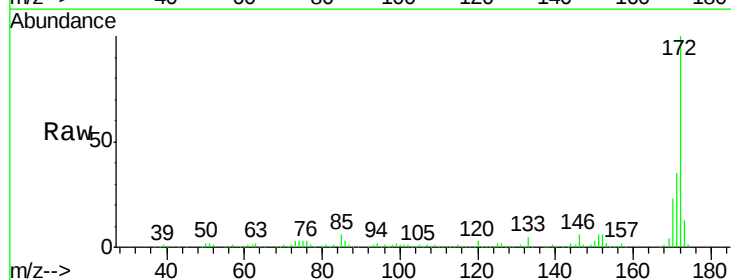

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

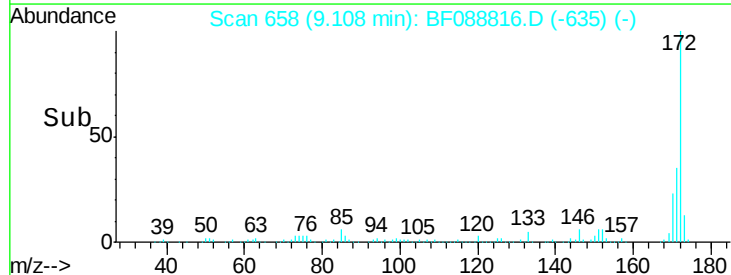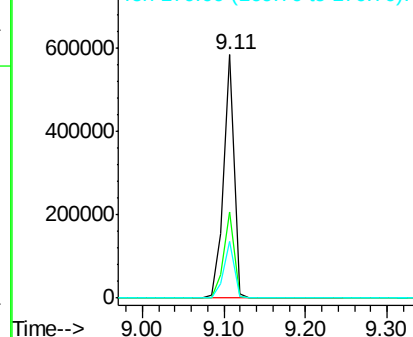


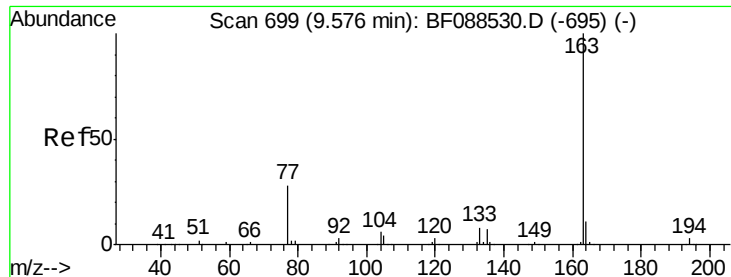




#49
Dimethylphthalate
Concen: 52.71 ng
RT: 9.51 min Scan# 693
Delta R.T. -0.03 min
Lab File: BF088816.D
Acq: 8 Jul 2016 9:48

Instrument :
BNA_F
ClientSampleId :
SB-16-COMP

Tot Ion:163 Resp: 440775
Ion Ratio Lower Upper
163 100
194 3.7 2.8 4.2
164 9.6 8.3 12.5

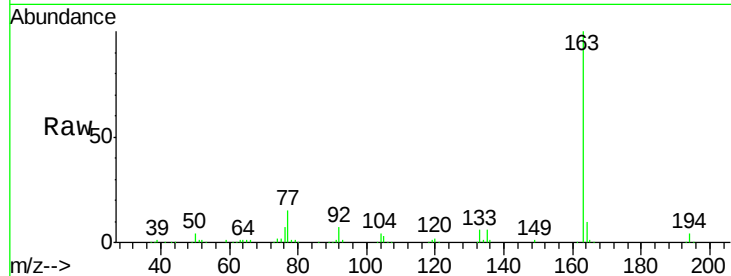


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

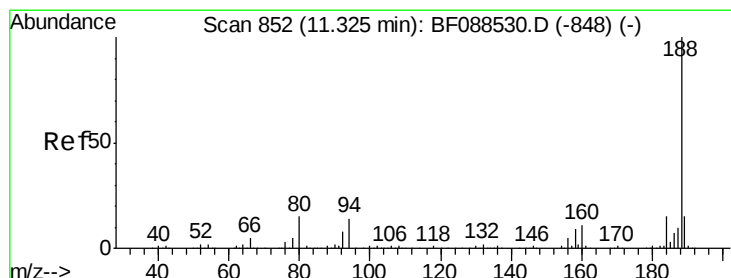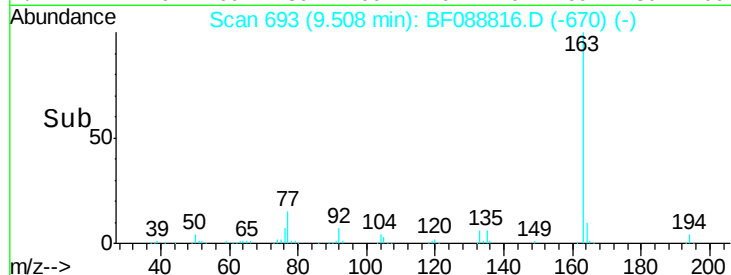
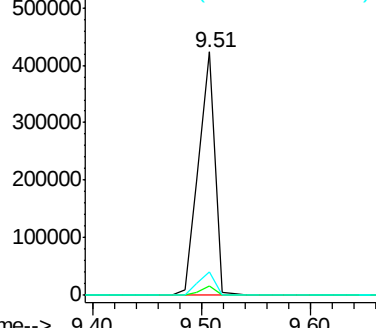



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.26 min Scan# 846
Delta R.T. -0.03 min
Lab File: BF088816.D
Acq: 8 Jul 2016 9:48

Tgt Ion:188 Resp: 198418
Ion Ratio Lower Upper
188 100
94 8.1 9.0 13.6#
80 8.7 10.0 15.0#

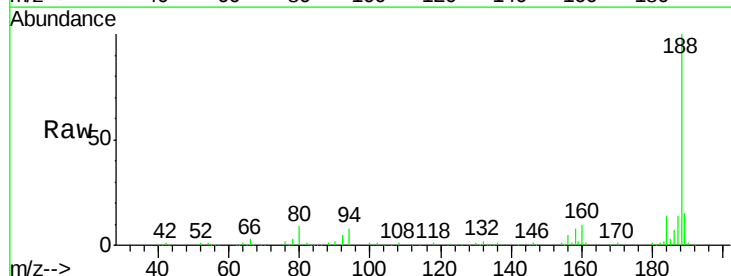

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

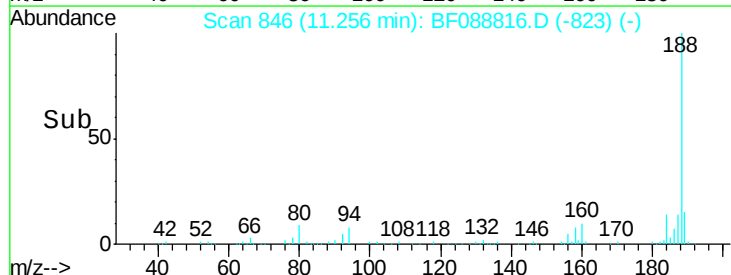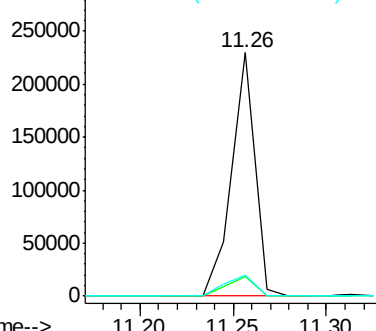

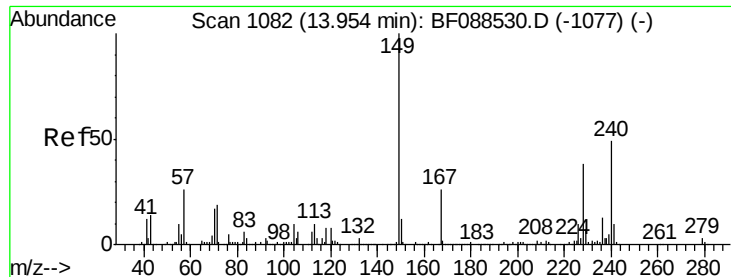

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.89 min Scan# 1076

Delta R.T. -0.03 min

Lab File: BF088816.D

Acq: 8 Jul 2016 9:48

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tot Ion:240 Resp: 188849

Ion Ratio Lower Upper

240 100

120 7.5 6.8 10.2




236 25.5 20.2 30.2

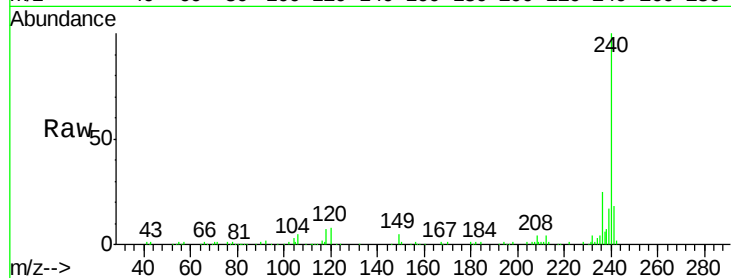

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

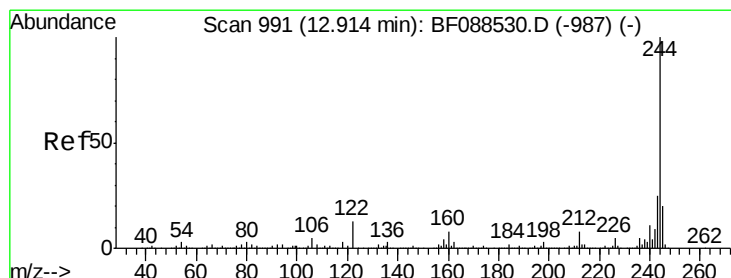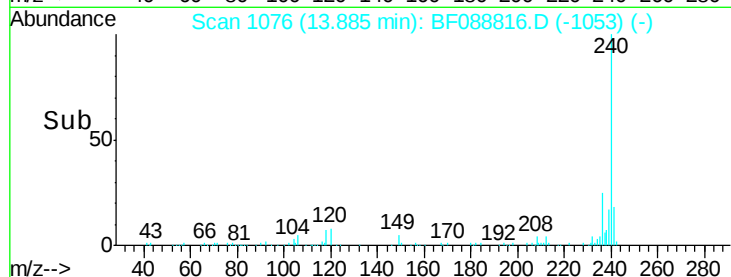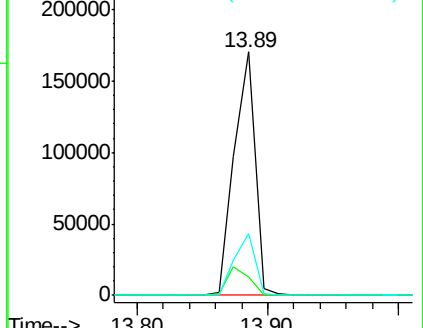

#78

Terphenyl-d14

Concen: 41.38 ng

RT: 12.83 min Scan# 984

Delta R.T. -0.03 min

Lab File: BF088816.D

Acq: 8 Jul 2016 9:48


Tgt Ion:244 Resp: 350884

Ion Ratio Lower Upper

244 100

212 8.1 6.0 9.0



122 18.2 11.2 16.8#



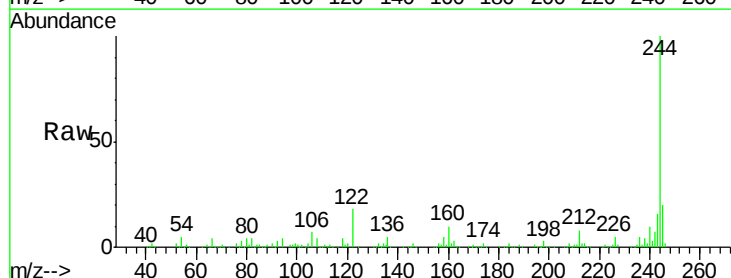


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

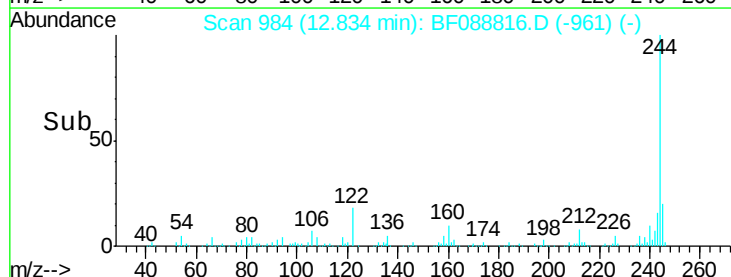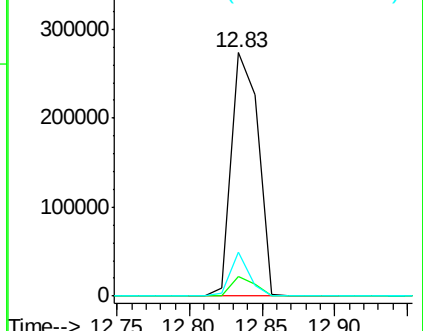

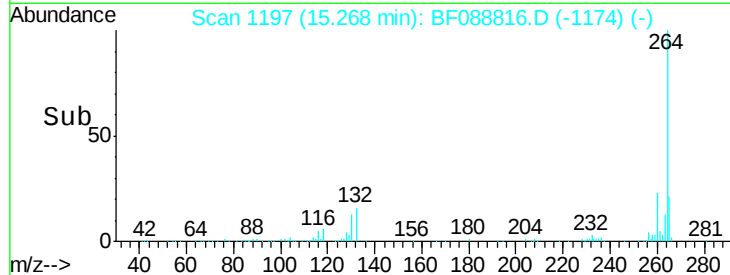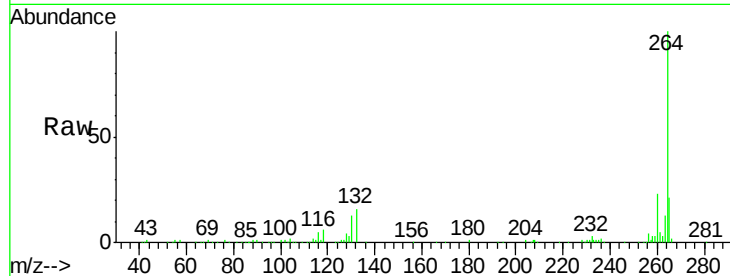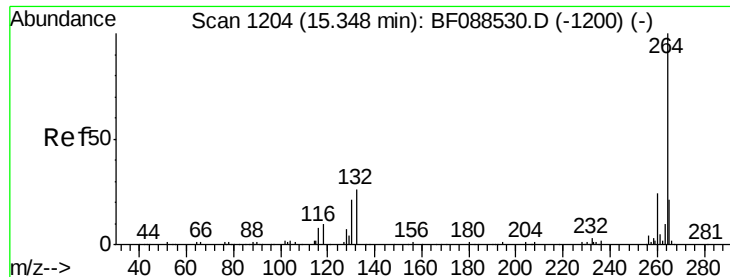

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.27 min Scan# 1197
 Delta R.T. -0.03 min
 Lab File: BF088816.D
 Acq: 8 Jul 2016 9:48

Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP

Tot Ion:	264	Resp:	141140
Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	21.1	16.9	25.3

