

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
 Data File : BF088797.D
 Acq On : 8 Jul 2016 00:05
 Operator : UM/SJ
 Sample : H3889-12 20X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS-12

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.815	19	20	67	rVB	1675026	4555588	100.00%	49.934%
2	5.324	324	327	331	rBV	42826	51407	1.13%	0.563%
3	6.364	416	418	421	rBV	60733	58895	1.29%	0.646%
4	6.502	428	430	432	rVB	80063	62250	1.37%	0.682%
5	6.742	449	451	453	rBV	641072	554781	12.18%	6.081%
6	6.890	463	464	466	rBB	49825	45881	1.01%	0.503%
7	8.022	561	563	566	rBV	679463	655398	14.39%	7.184%
8	9.108	656	658	660	rBV	43176	56641	1.24%	0.621%
9	9.782	714	717	719	rBV	513380	623963	13.70%	6.839%
10	11.256	843	846	847	rBV	574340	532907	11.70%	5.841%
11	11.279	847	848	850	rVV	89634	63262	1.39%	0.693%
12	12.457	949	951	954	rBV	175147	158352	3.48%	1.736%
13	12.685	968	971	973	rBV	182198	179427	3.94%	1.967%
14	12.834	983	984	987	rVB2	53292	46474	1.02%	0.509%
15	13.885	1073	1076	1077	rBV2	492096	642811	14.11%	7.046%
16	13.908	1077	1078	1080	rVV	74087	52173	1.15%	0.572%
17	14.880	1161	1163	1168	rBV	78632	145978	3.20%	1.600%
18	15.154	1184	1187	1190	rVB	42486	47916	1.05%	0.525%
19	15.211	1190	1192	1194	rBV	44706	66023	1.45%	0.724%
20	15.268	1194	1197	1204	rVV	377065	477267	10.48%	5.231%
21	16.571	1308	1311	1316	rVB2	21842	45912	1.01%	0.503%


Sum of corrected areas: 9123306

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
Data File : BF088797.D
Acq On : 8 Jul 2016 00:05
Operator : UM/SJ
Sample : H3889-12 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SS-12

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

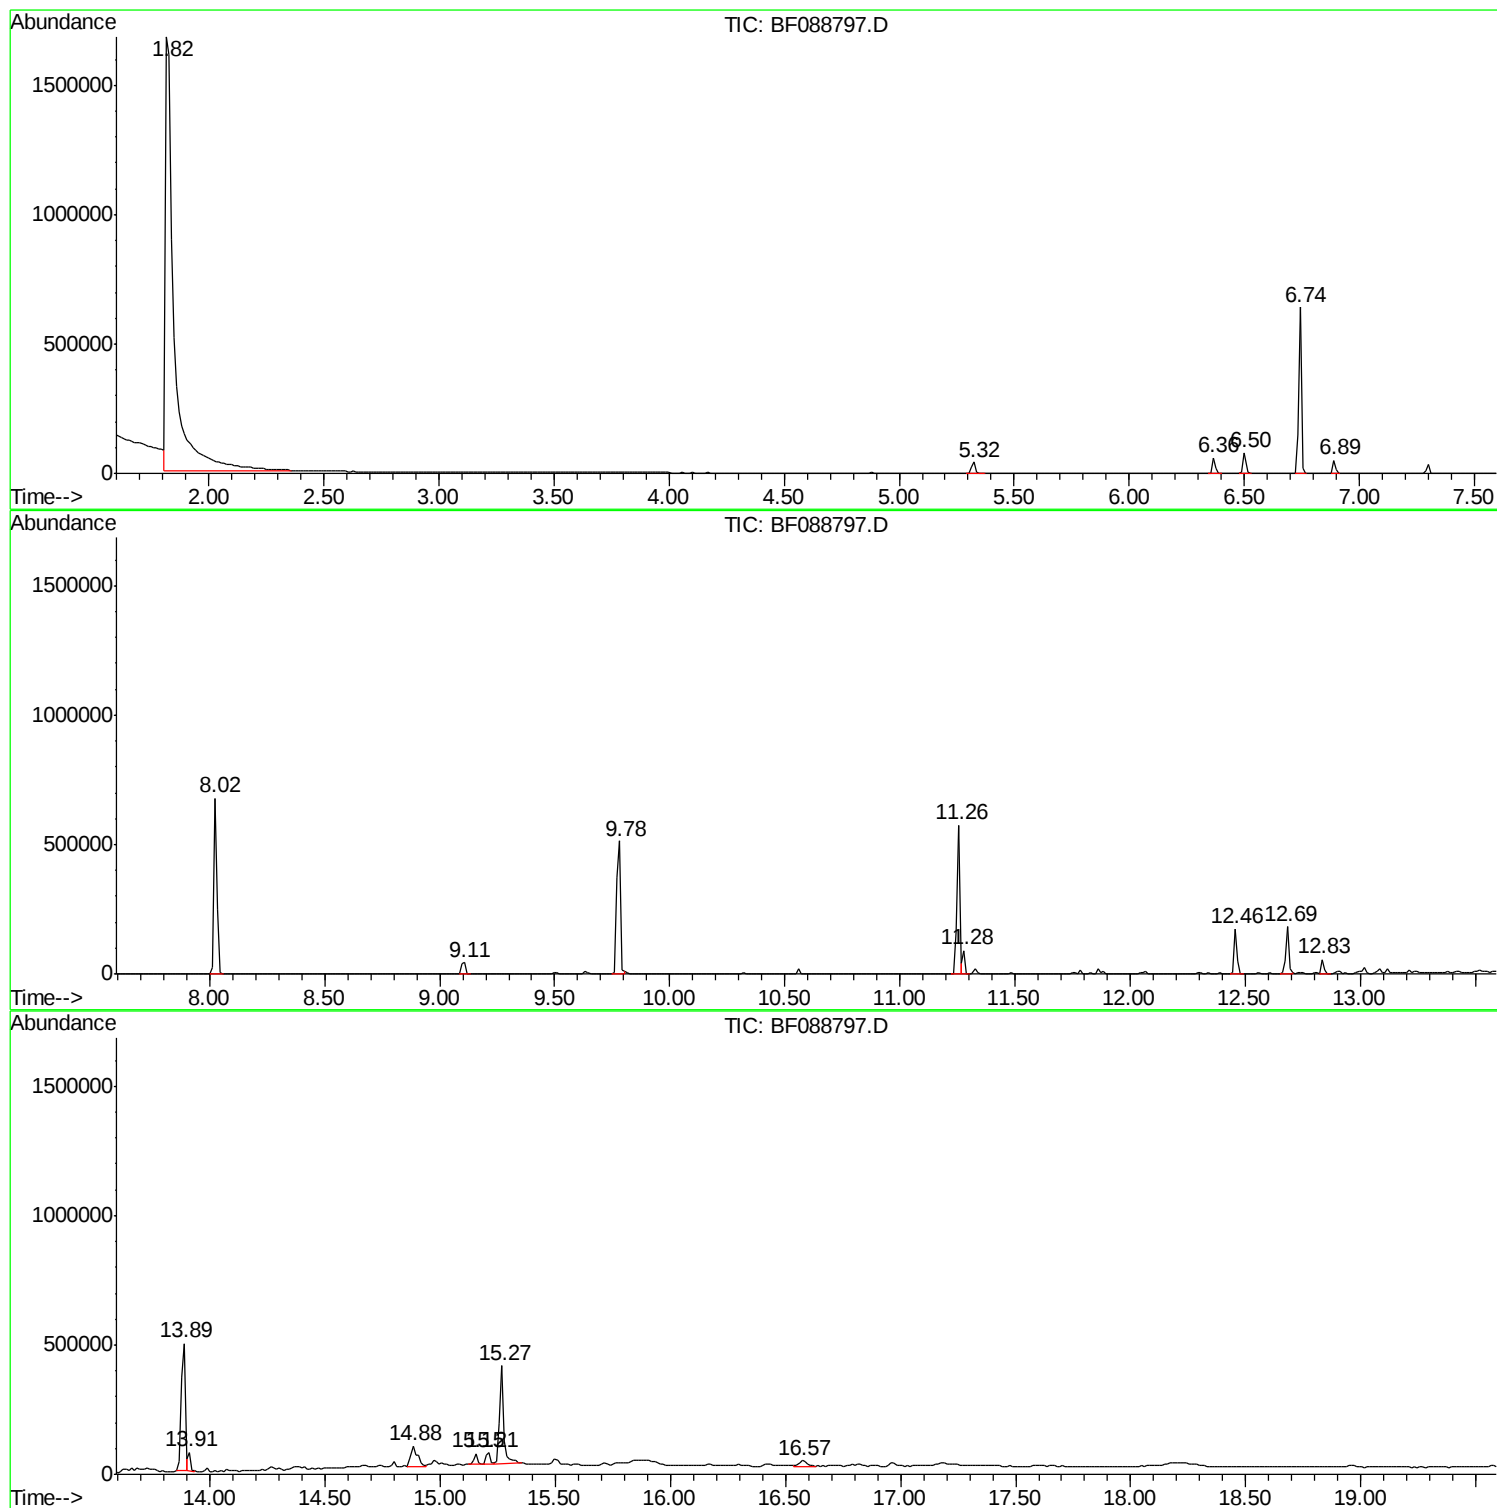

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
Data File : BF088797.D
Acq On : 8 Jul 2016 00:05
Operator : UM/SJ
Sample : H3889-12 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-12










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.50 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	2.24 ng	62250	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

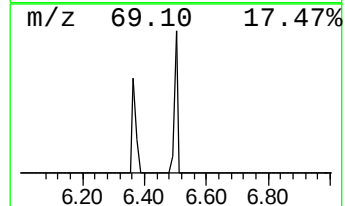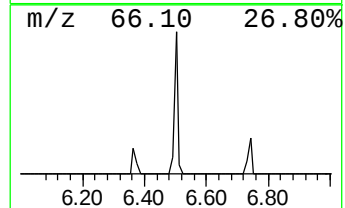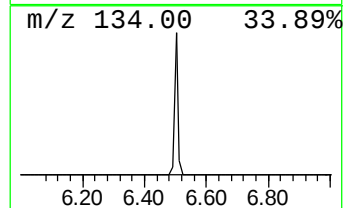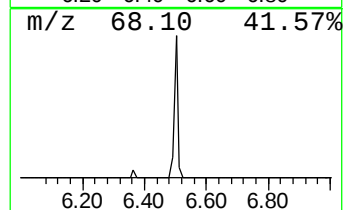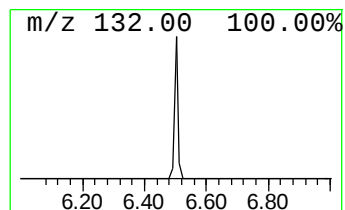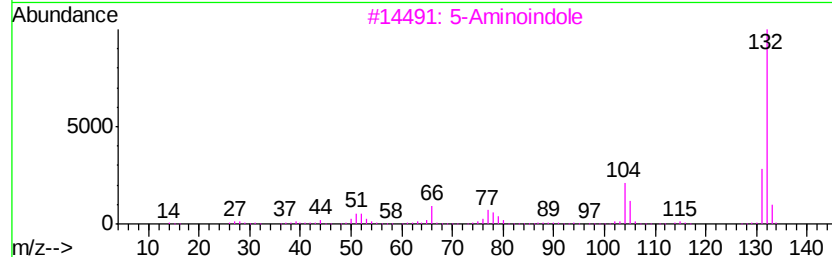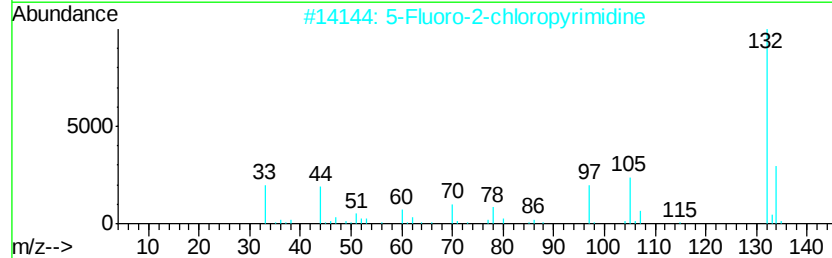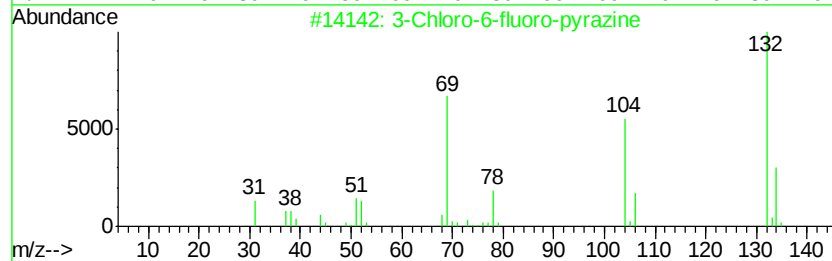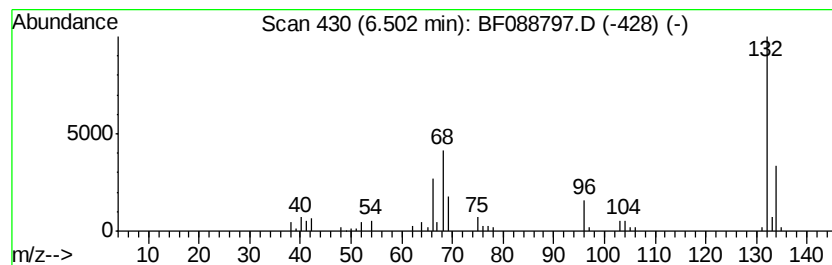

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
Data File : BF088797.D
Acq On : 8 Jul 2016 00:05
Operator : UM/SJ
Sample : H3889-12 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-12

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	2.2	ng	62250	1	6.74	554781	20.0