


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
 Data File : BF088772.D
 Acq On : 7 Jul 2016 10:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 17:15:08 2016

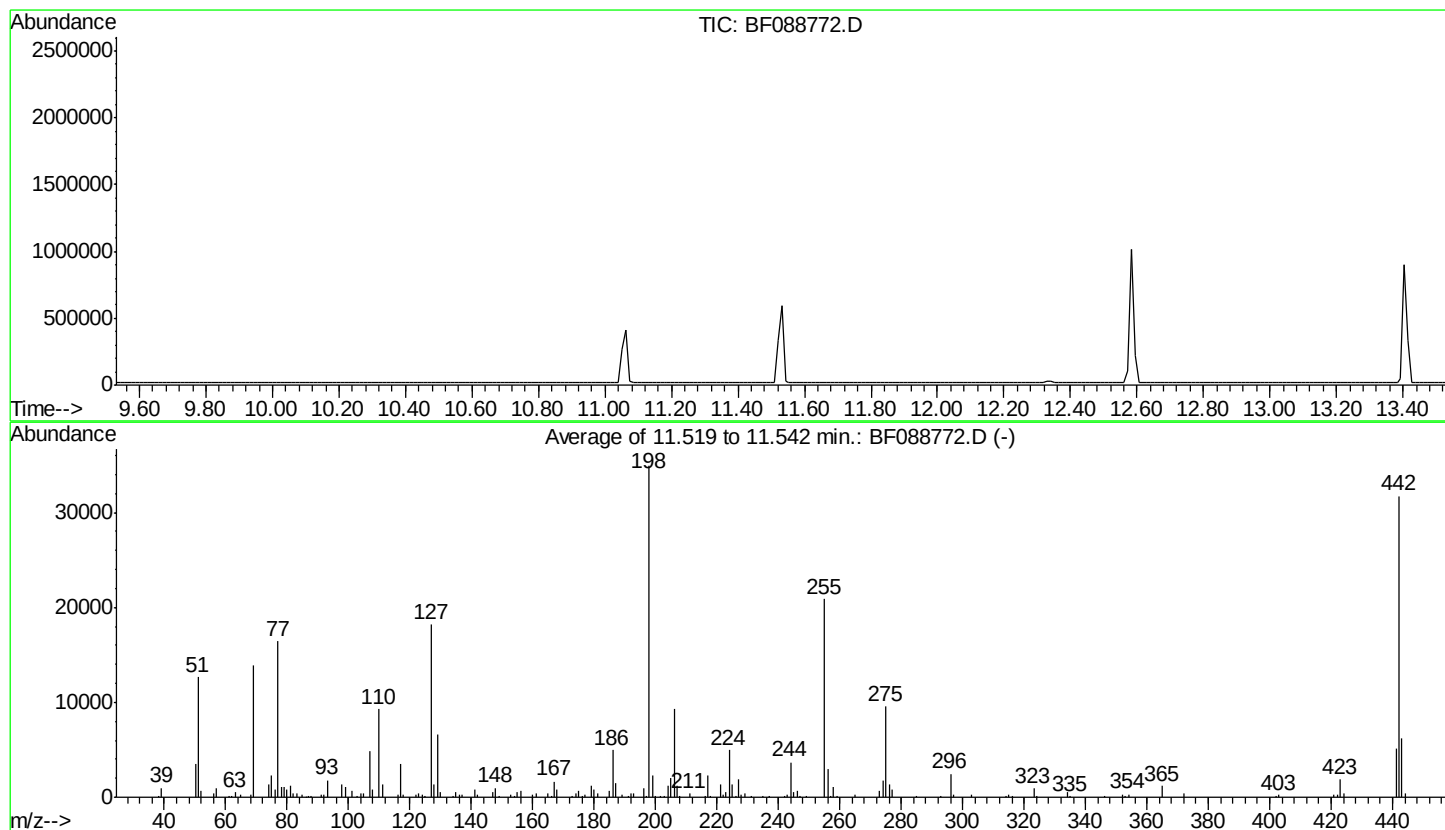

AutoFind: Scans 869, 870, 871; Background Corrected with Scan 865

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	12664	PASS
68	69	0.00	2	2.0	271	PASS
69	198	0.00	100	39.8	13896	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	18154	PASS
197	198	0.00	2	0.3	101	PASS
198	198	100	100	100.0	34949	PASS
199	198	5	9	6.7	2330	PASS
275	198	10	60	27.3	9539	PASS
365	198	1	100	3.5	1206	PASS
441	442	0.01	24	16.1	5107	PASS
442	198	50	100	90.9	31773	PASS
443	442	15	24	19.7	6253	PASS