


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070716\
 Data File : BF088780.D
 Acq On : 7 Jul 2016 15:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 17:15:08 2016

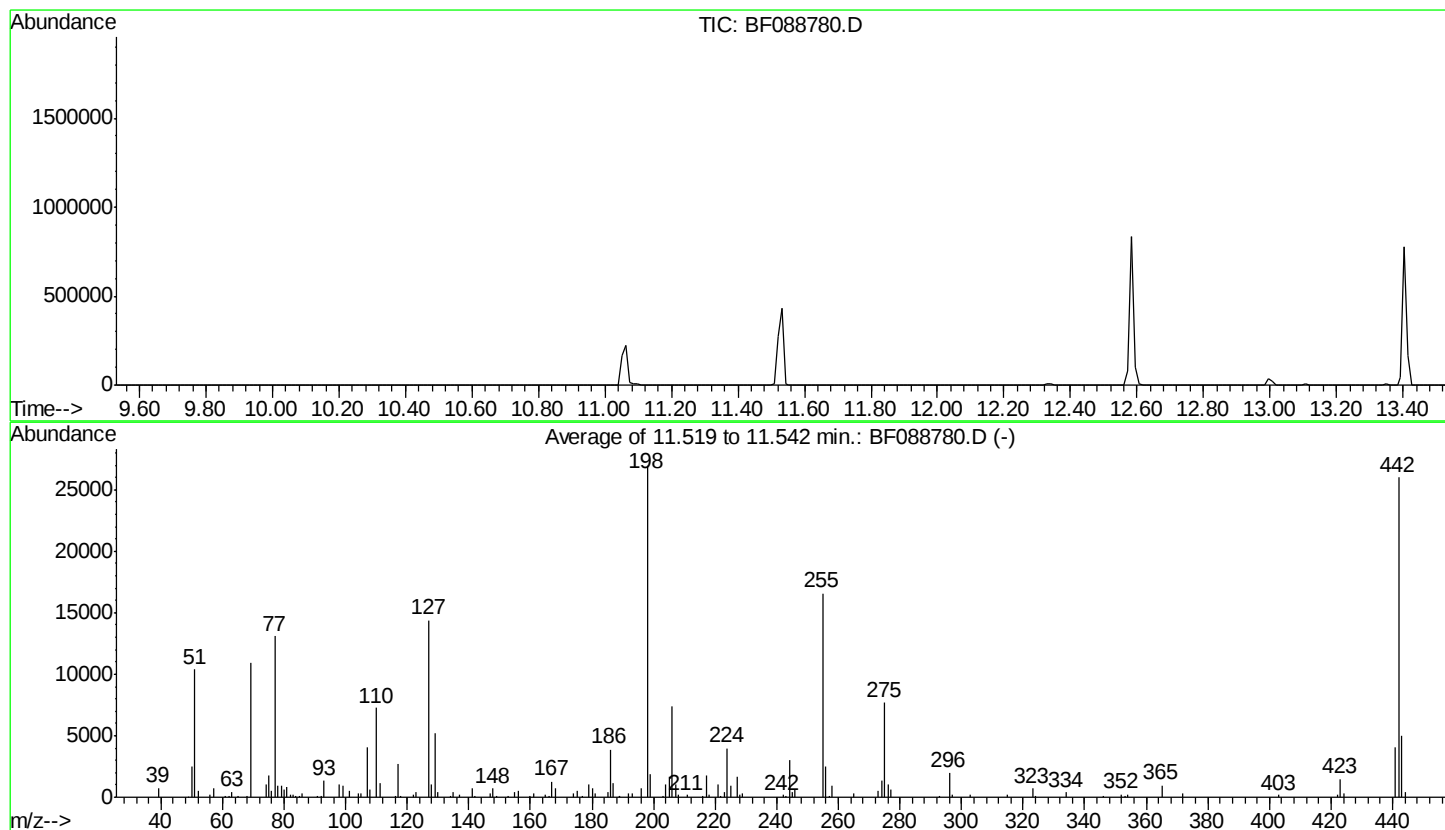

AutoFind: Scans 869, 870, 871; Background Corrected with Scan 865

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	10383	PASS
68	69	0.00	2	1.3	139	PASS
69	198	0.00	100	40.5	10926	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	14394	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26956	PASS
199	198	5	9	6.8	1825	PASS
275	198	10	60	28.6	7699	PASS
365	198	1	100	3.6	973	PASS
441	442	0.01	24	15.7	4081	PASS
442	198	50	100	96.4	25978	PASS
443	442	15	24	19.3	5017	PASS