


Data Path : Z:\HPCHEM1\BNA F\DATA\BF070717\
Data File : BF096549.D
Acq On : 7 Jul 2017 10:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 02:06:16 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

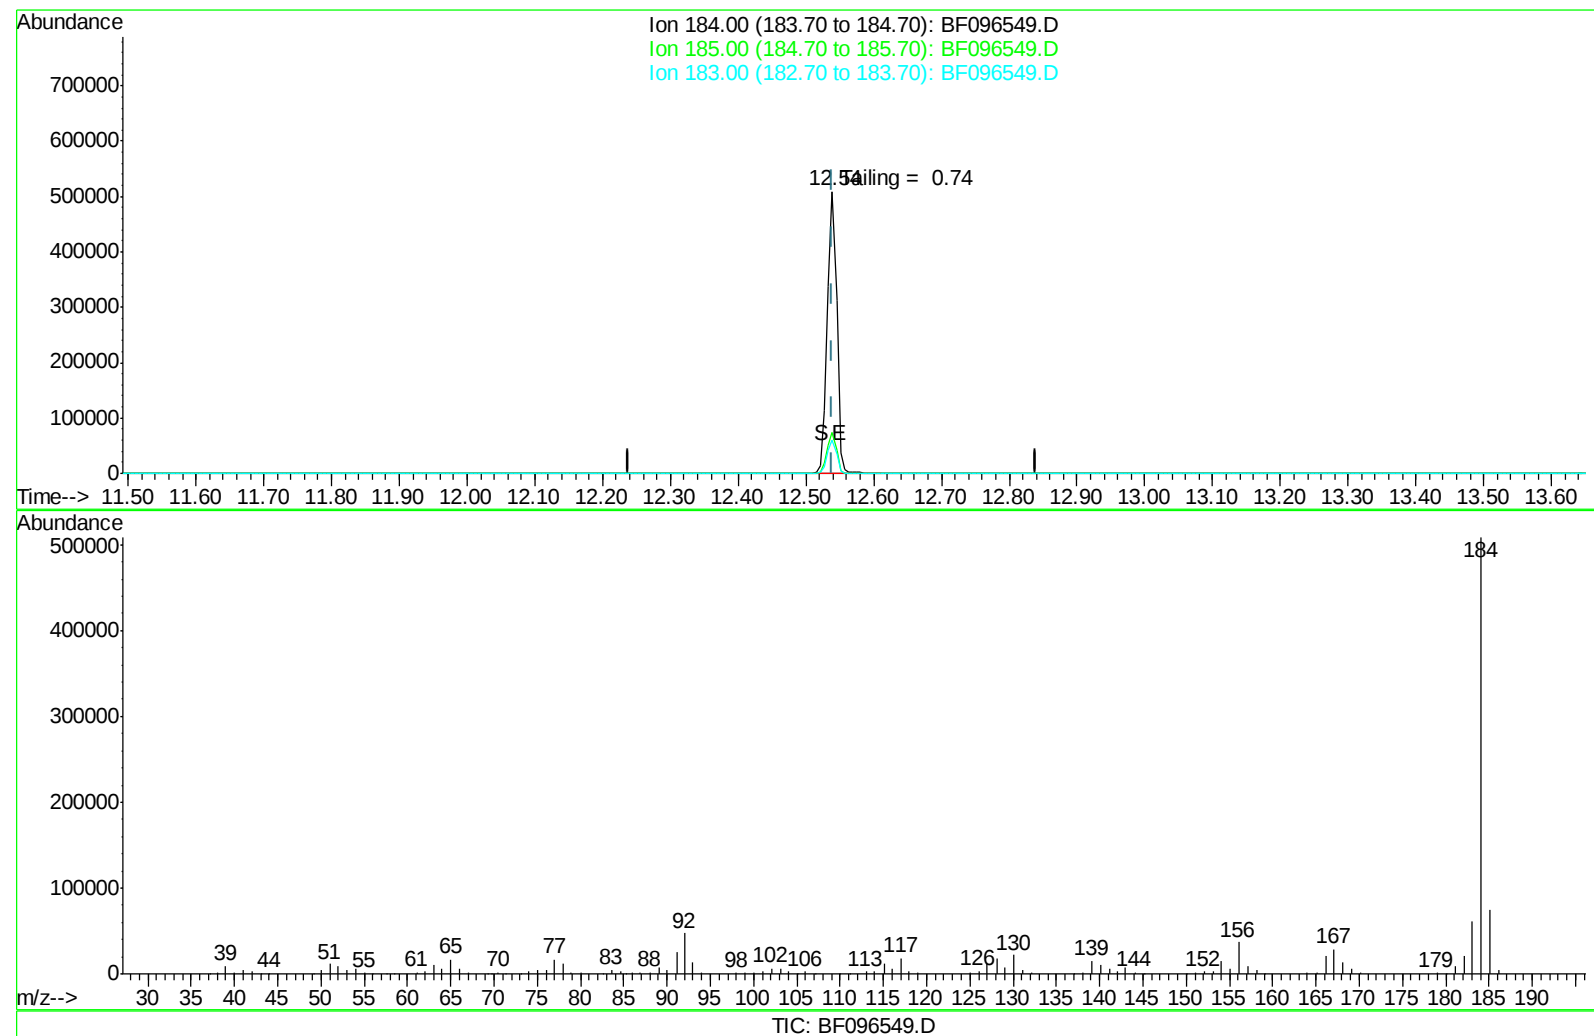

(76) Benzidine



12.539min (-0.000) 0.00ng

response 475833

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.67#
183.00	12.20	12.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070717\
Data File : BF096549.D
Acq On : 7 Jul 2017 10:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 02:06:16 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

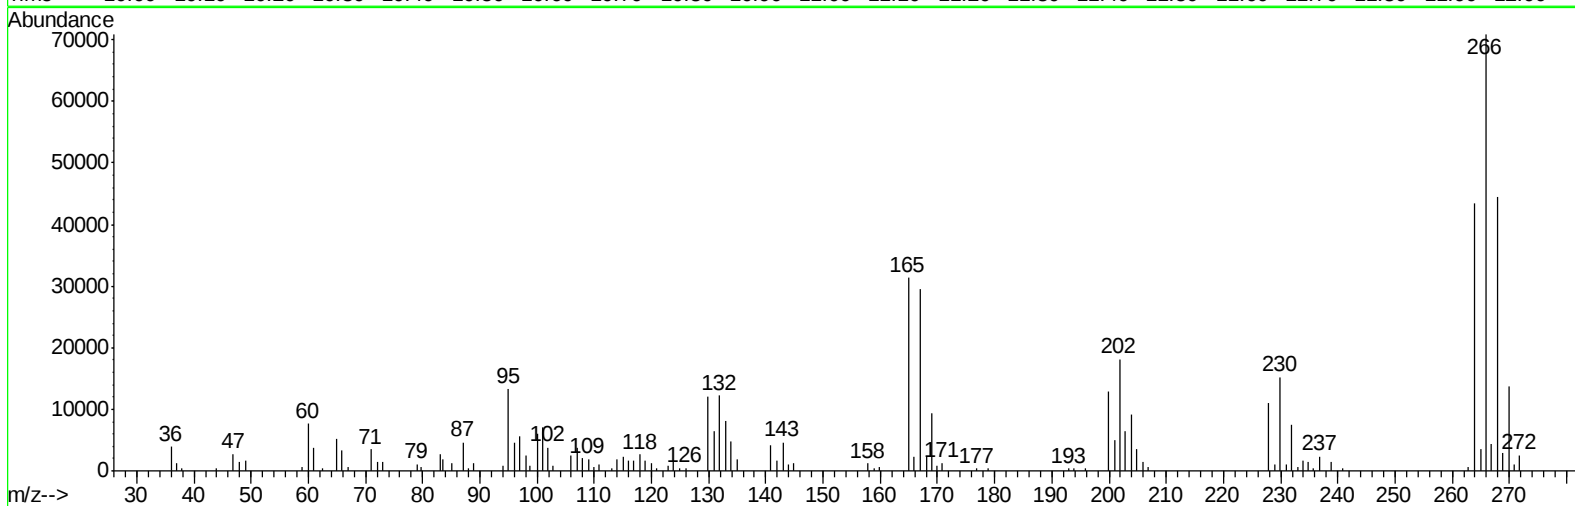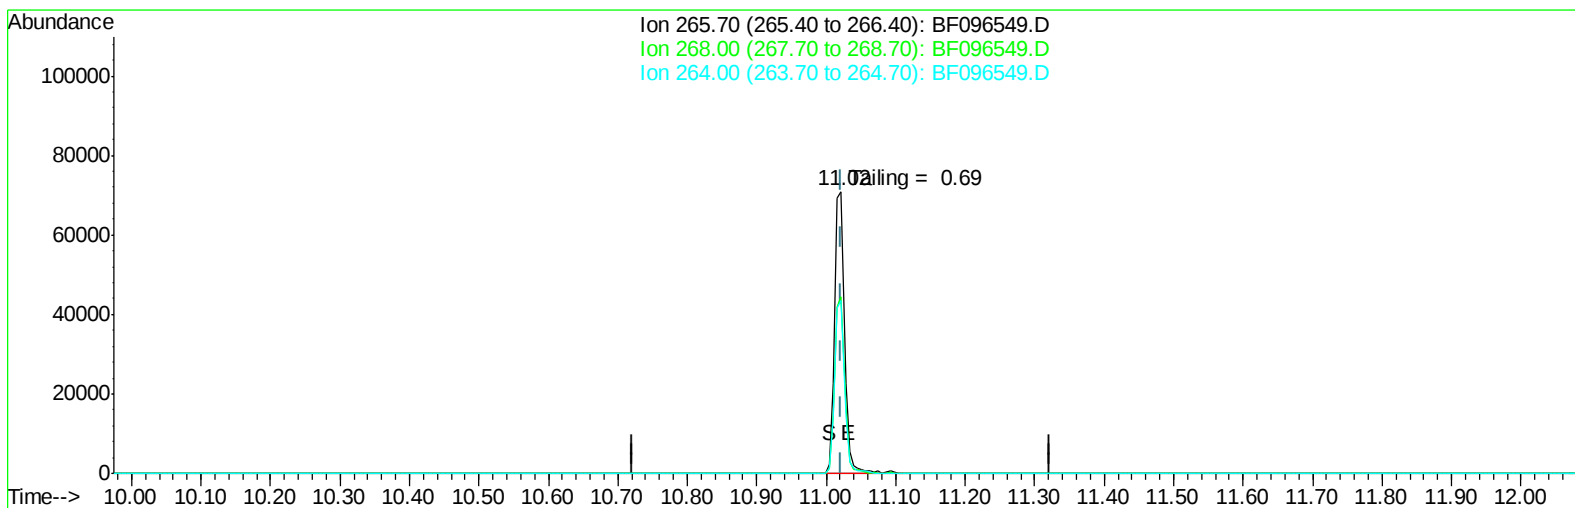

TIC: BF096549.D

(69) Pentachlorophenol (C)

11.022min (-0.000) 38713.40ng

response 70661

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.82
264.00	64.60	61.34
0.00	0.00	0.00