
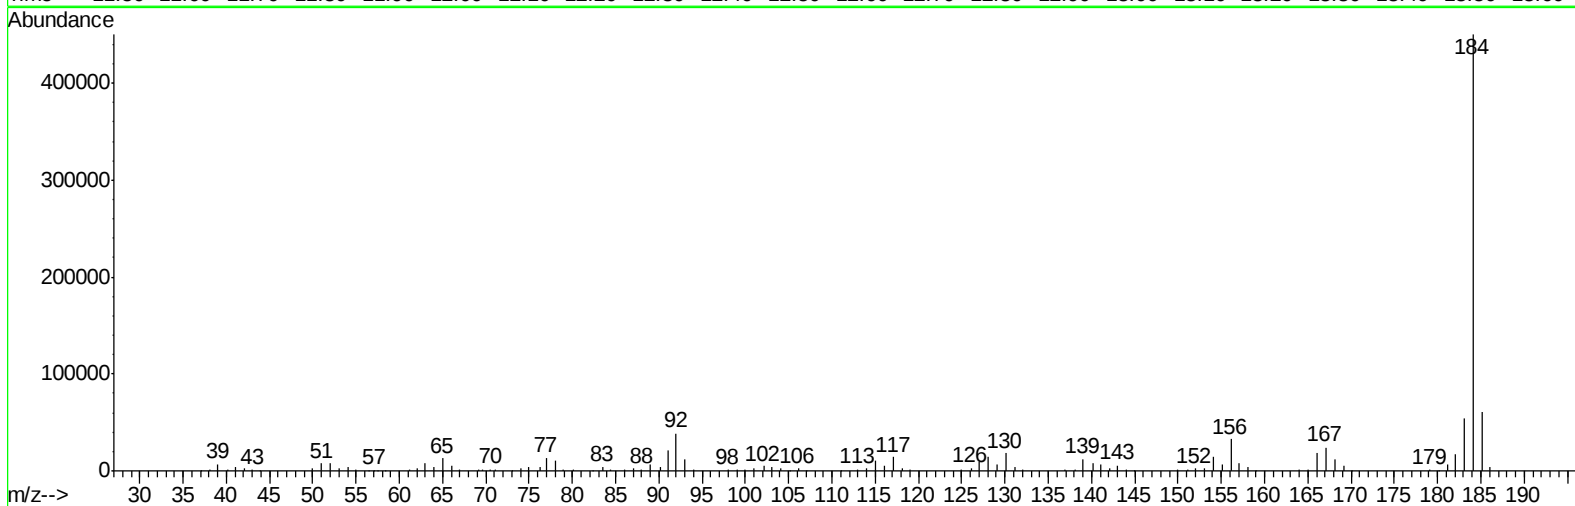


Data Path : Z:\HPCHEM1\BNA F\DATA\BF070717\
Data File : BF096563.D
Acq On : 7 Jul 2017 17:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 18:00:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

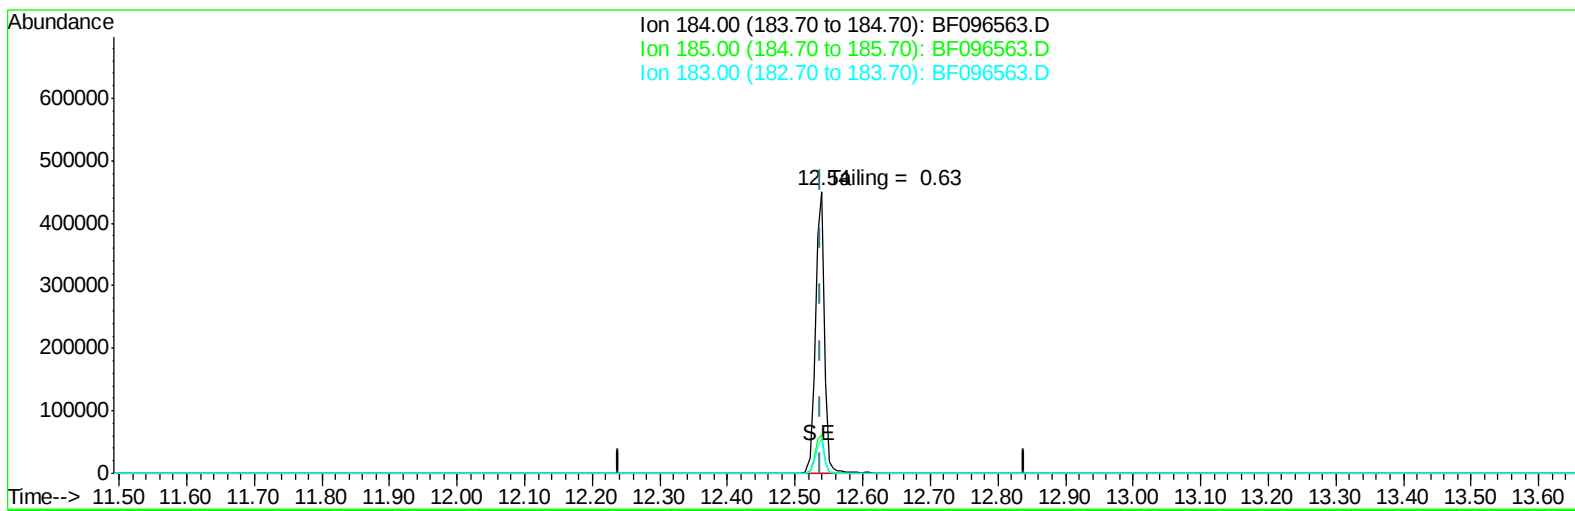

TIC: BF096563.D

(76) Benzidine



12.539min (-0.000) 0.00ng

response 424489

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.63#
183.00	12.20	12.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070717\
Data File : BF096563.D
Acq On : 7 Jul 2017 17:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 18:00:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

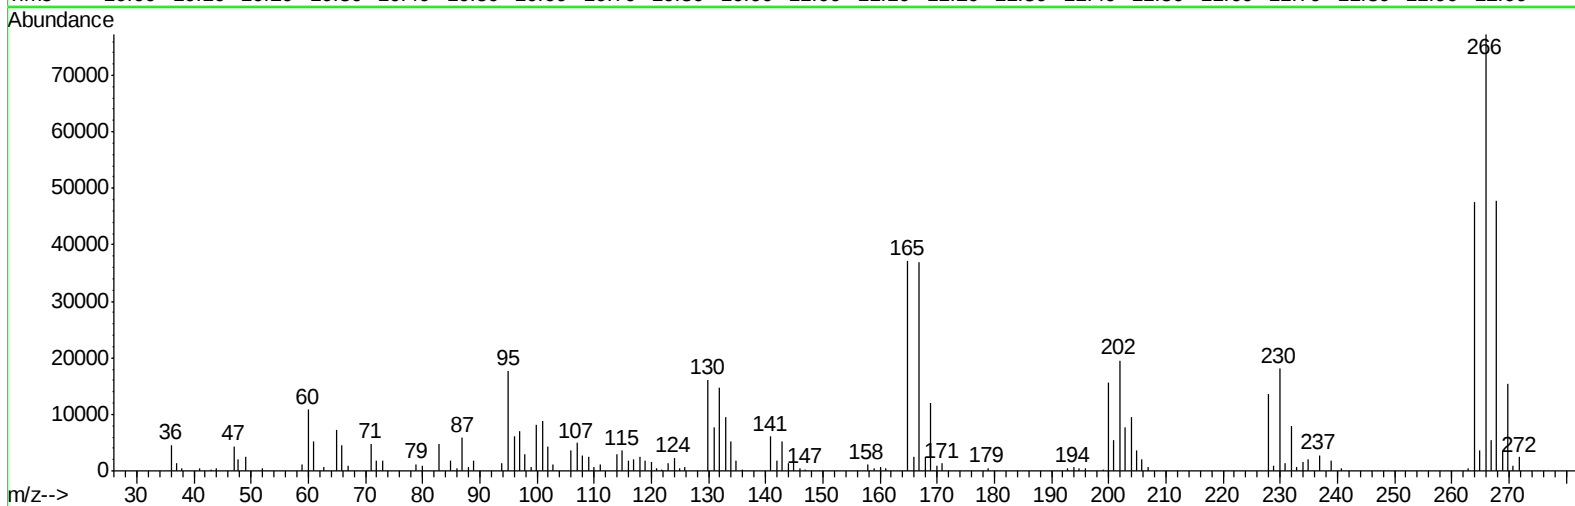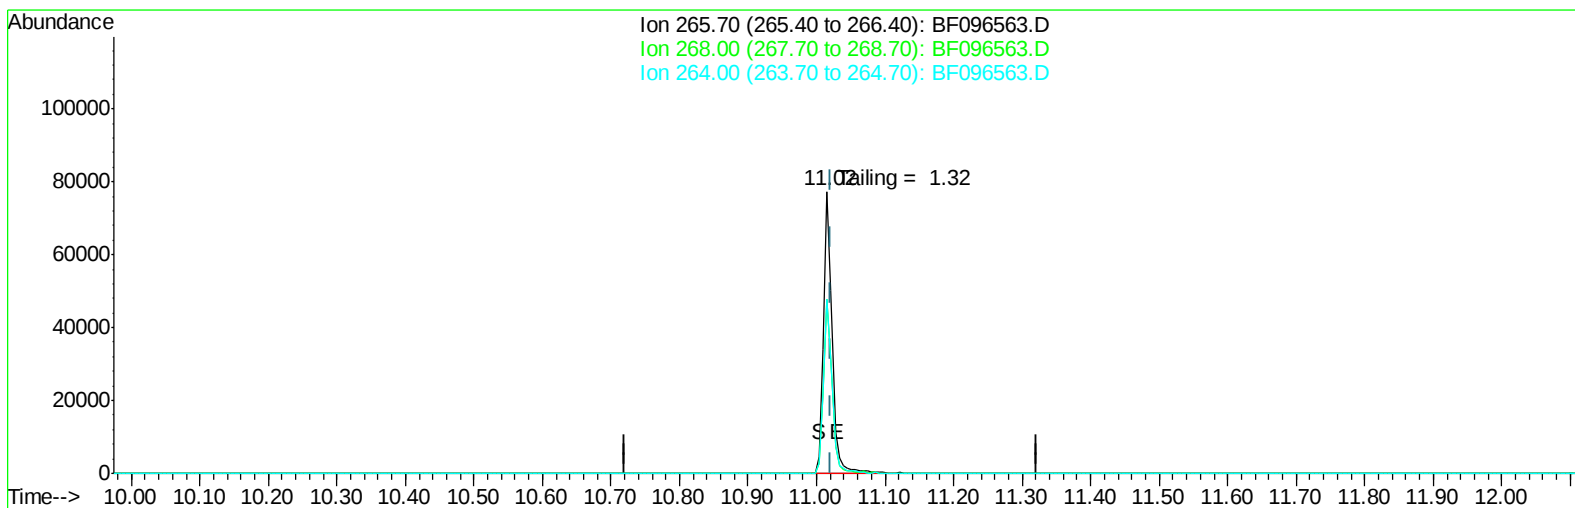

TIC: BF096563.D

(69) Pentachlorophenol (C)

11.016min (-0.006) 65790.52ng

response 67313

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.87
264.00	64.60	61.63
0.00	0.00	0.00