

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070717\
 Data File : BF096583.D
 Acq On : 8 Jul 2017 2:28
 Operator : SJ/MA
 Sample : I4092-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-010

Quant Time: Jul 08 04:34:13 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 13:02:33 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	106004	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	405969	20.00	ng	0.00
38) Acenaphthene-d10	9.73	164	159054	20.00	ng	0.00
63) Phenanthrene-d10	11.21	188	242826	20.00	ng	0.00
75) Chrysene-d12	13.84	240	209569	20.00	ng	0.00
86) Perylene-d12	15.24	264	155820	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	690898	96.20	ng	0.00
7) Phenol-d6	6.34	99	753750	85.37	ng	0.00
23) Nitrobenzene-d5	7.26	82	449515	66.54	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	120923	97.33	ng	0.00
44) 2-Fluorobiphenyl	9.06	172	706458	75.94	ng	0.00
78) Terphenyl-d14	12.80	244	542712	55.34	ng	0.00
Target Compounds						
10) Phenol	6.35	94	23235	2.310	ng	94
49) Dimethylphthalate	9.45	163	118983	10.021	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070717\
Data File : BF096583.D
Acq On : 8 Jul 2017 2:28
Operator : SJ/MA
Sample : I4092-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-010

Quant Time: Jul 08 04:34:13 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

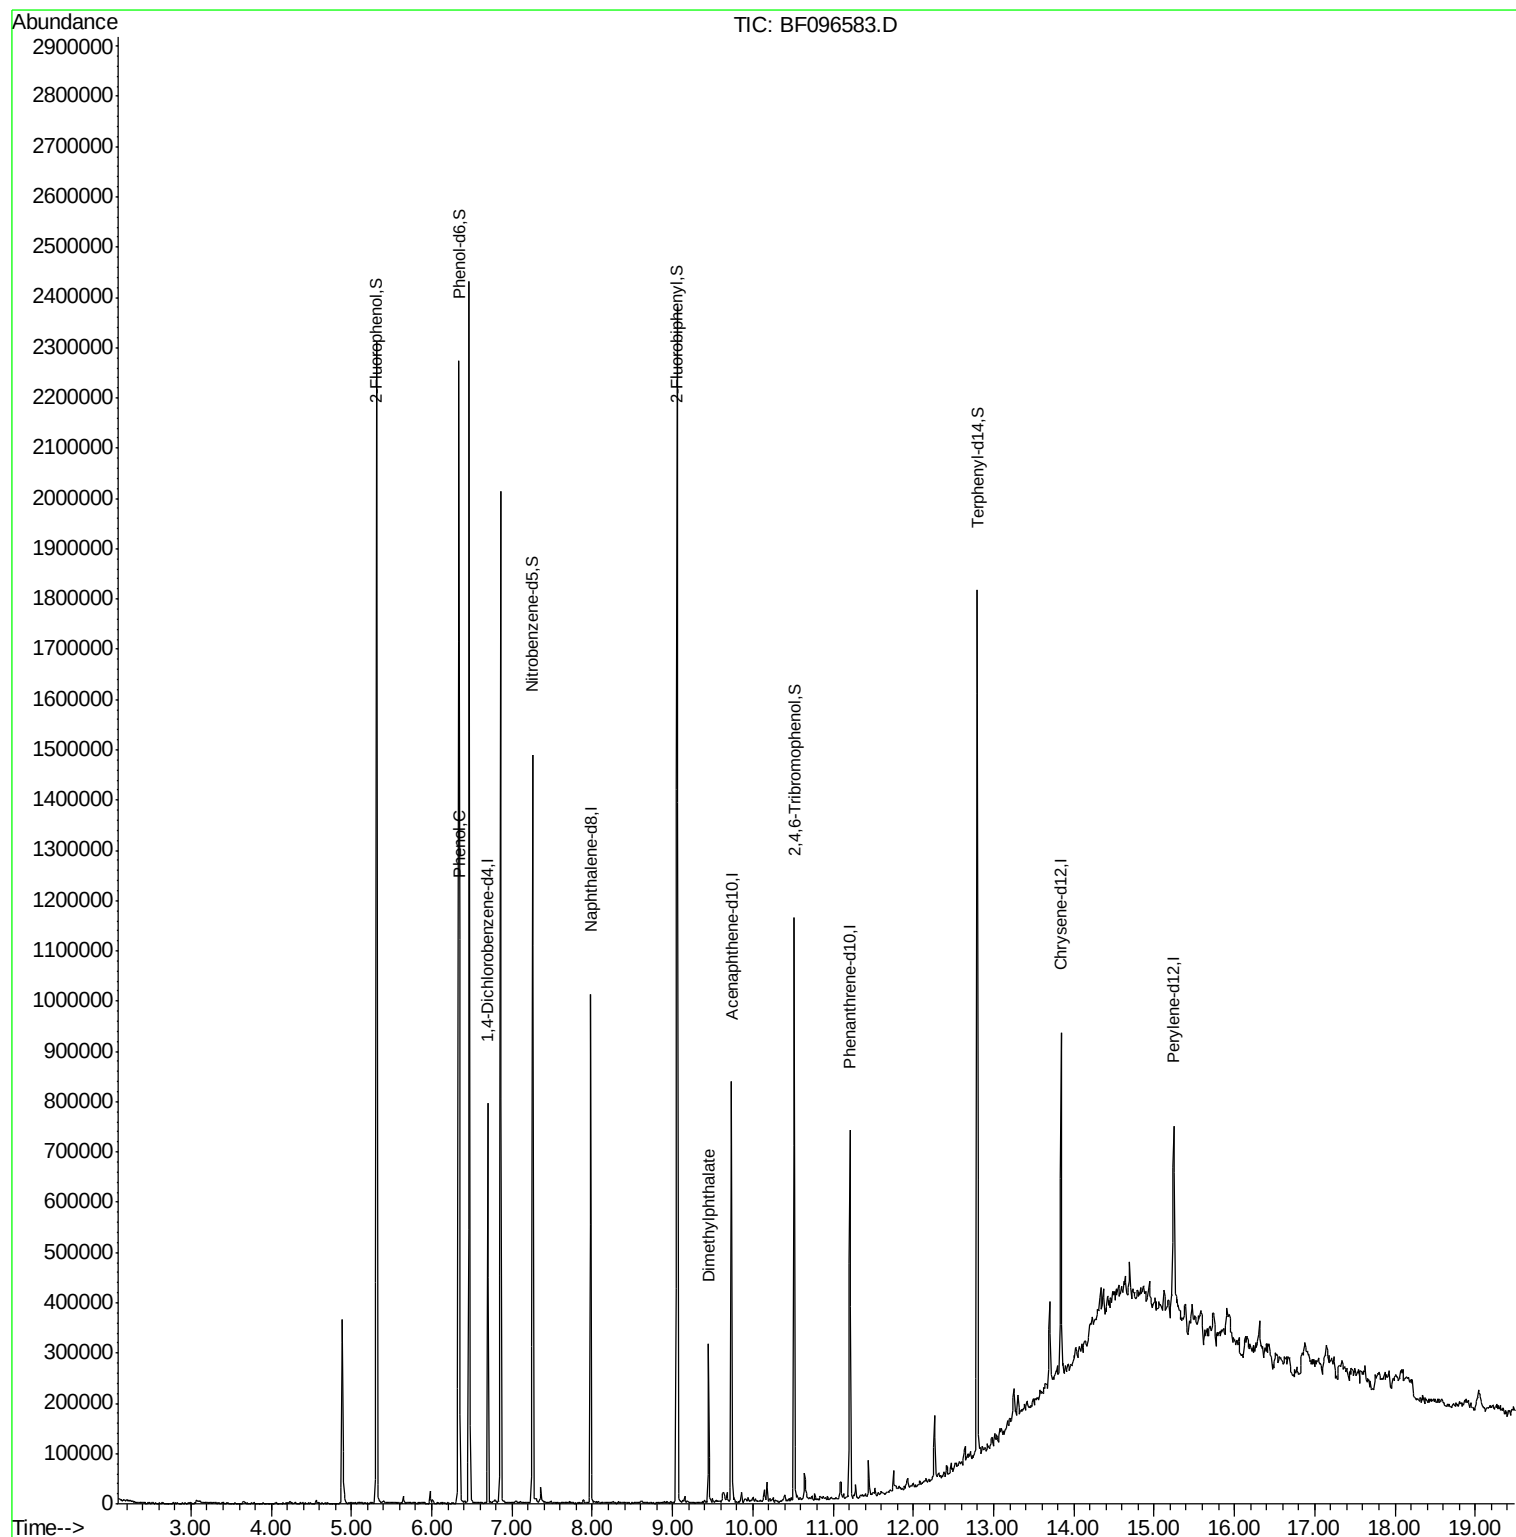

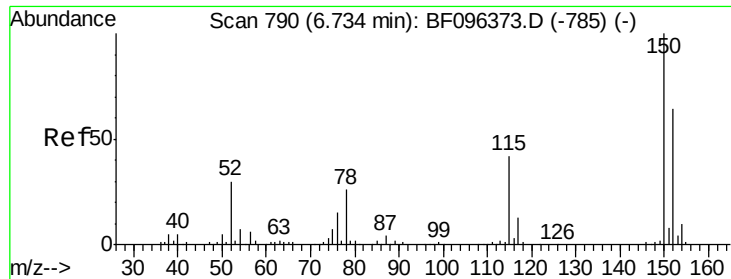


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 784
Delta R.T. -0.00 min
Lab File: BF096583.D
Acq: 8 Jul 2017 2:28

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-010

Tgt Ion:152 Resp: 106004
Ion Ratio Lower Upper
152 100
150 157.8 126.2 189.2
115 65.1 52.2 78.2

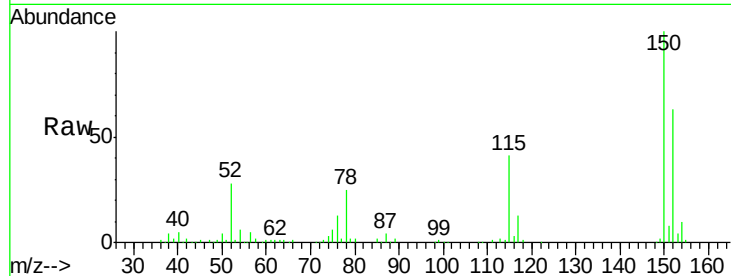


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

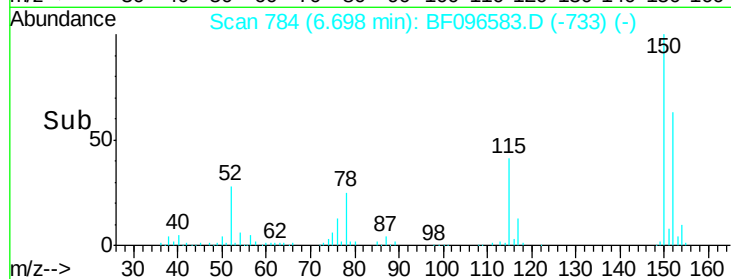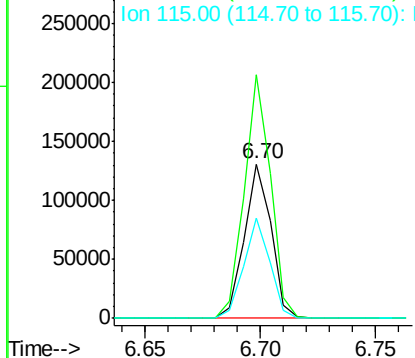



#5


2-Fluorophenol
Concen: 96.199 ng
RT: 5.32 min Scan# 549
Delta R.T. 0.01 min
Lab File: BF096583.D
Acq: 8 Jul 2017 2:28

Tgt Ion:112 Resp: 690898
Ion Ratio Lower Upper
112 100
64 61.0 46.0 69.0
63 31.3 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

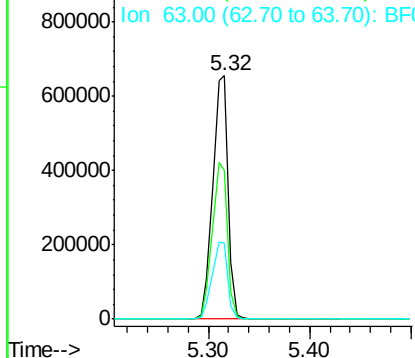

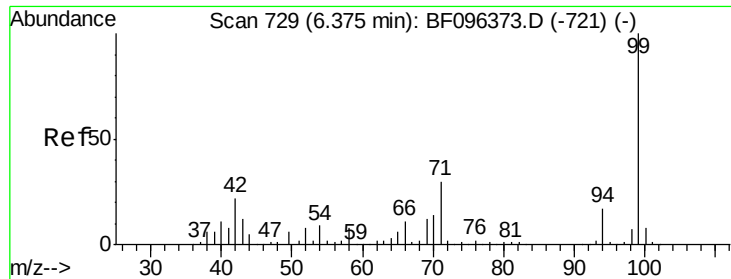

#7

Phenol-d6

Concen: 85.369 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.01 min

Lab File: BF096583.D

Acq: 8 Jul 2017 2:28

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-010


Tgt Ion: 99 Resp: 753750

Ion Ratio Lower Upper

99 100

42 22.3 13.5 20.3#




71 31.7 24.5 36.7



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

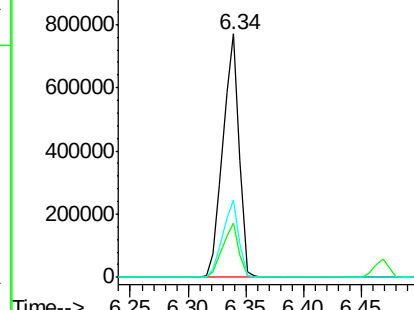

#10

Phenol

Concen: 2.310 ng

RT: 6.35 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF096583.D

Acq: 8 Jul 2017 2:28


Tgt Ion: 94 Resp: 23235

Ion Ratio Lower Upper

94 100

65 30.5 9.9 49.9



66 36.7 23.1 63.1




Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

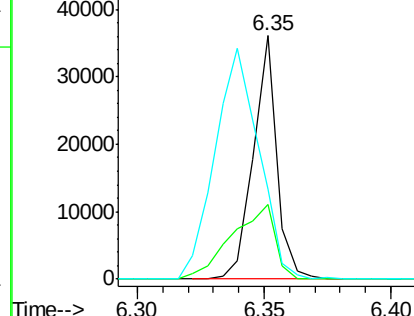

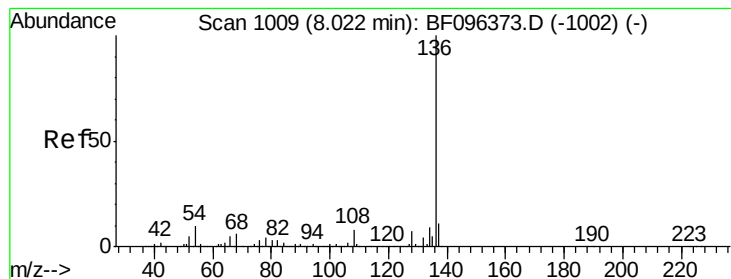

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF096583.D

Acq: 8 Jul 2017 2:28

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-010

Tgt Ion: 136 Resp: 405969


Ion Ratio Lower Upper

136 100

137 10.5 8.5 12.7

54 10.4 4.9 7.3#

68 5.6 4.1 6.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

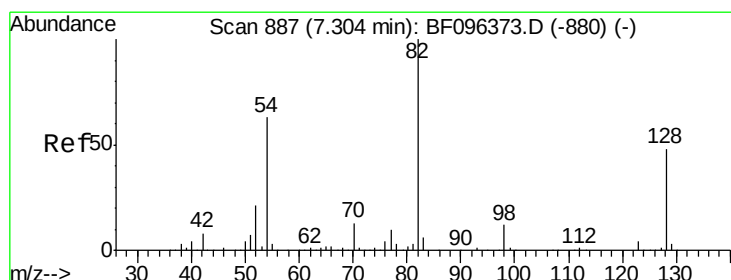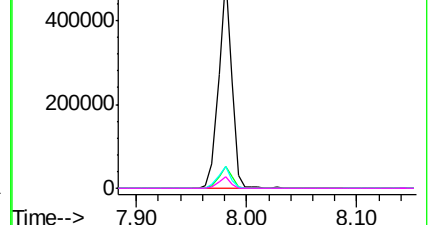

#23

Nitrobenzene-d5

Concen: 66.536 ng

RT: 7.26 min Scan# 879

Delta R.T. -0.01 min

Lab File: BF096583.D

Acq: 8 Jul 2017 2:28


Tgt Ion: 82 Resp: 449515

Ion Ratio Lower Upper

82 100

128 45.4 34.0 51.0



54 64.7 42.2 63.2#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

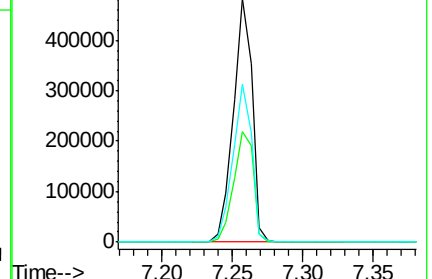



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.73 min Scan# 1300

Delta R.T. -0.00 min

Lab File: BF096583.D

Acq: 8 Jul 2017 2:28

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-010





Tgt Ion:164 Resp: 159054

Ion Ratio Lower Upper

164 100

162 106.4 82.6 123.8

160 47.0 36.2 54.2

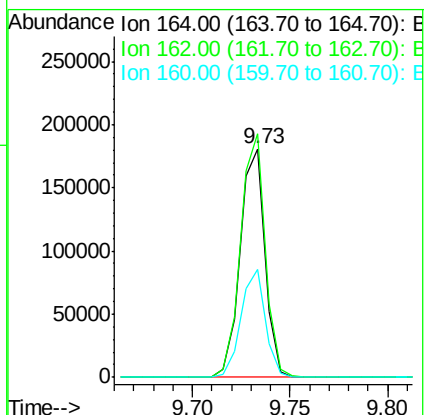

#41

2,4,6-Tribromophenol

Concen: 97.330 ng

RT: 10.52 min Scan# 1433

Delta R.T. -0.01 min

Lab File: BF096583.D

Acq: 8 Jul 2017 2:28




Tgt Ion:330 Resp: 120923


Ion Ratio Lower Upper

330 100

332 98.7 76.6 115.0

141 38.5 31.4 47.2


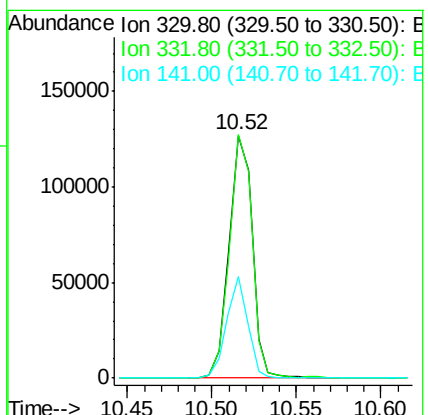




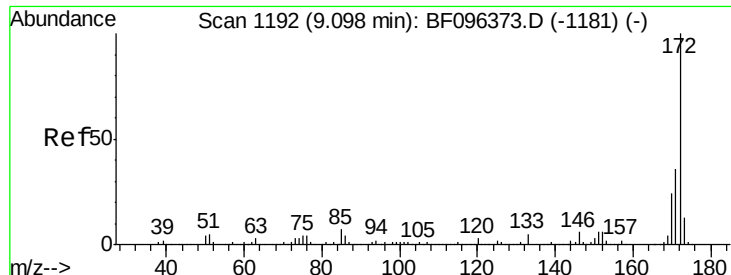

#44
 2-Fluorobiphenyl
 Concen: 75.942 ng
 RT: 9.06 min Scan# 1185
 Delta R.T. -0.01 min
 Lab File: BF096583.D
 Acq: 8 Jul 2017 2:28




Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-010


Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.6	44.4
170	23.5	19.8	29.8

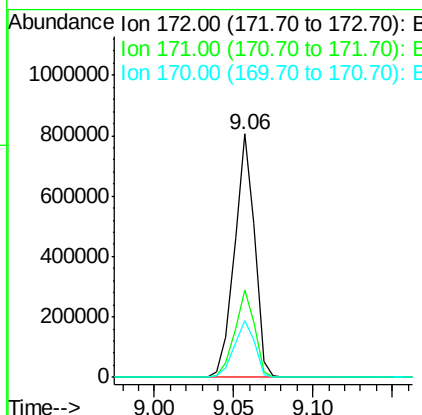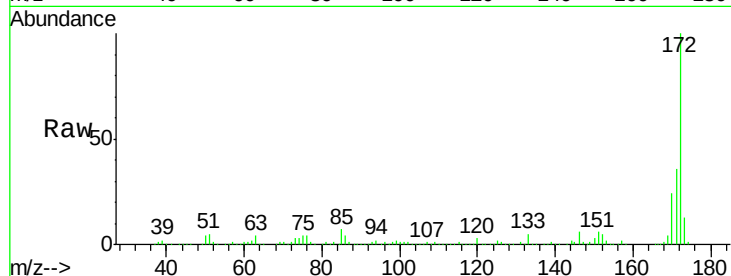

#49
 Dimethylphthalate
 Concen: 10.021 ng
 RT: 9.45 min Scan# 1252
 Delta R.T. -0.02 min
 Lab File: BF096583.D
 Acq: 8 Jul 2017 2:28

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.4	2.6	4.0
164	9.6	8.4	12.6

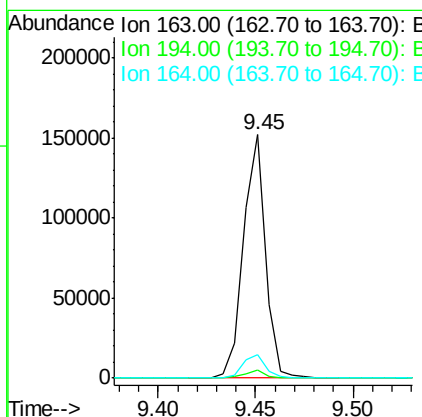







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.00 min
Lab File: BF096583.D
Acq: 8 Jul 2017 2:28

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-010

Tgt Ion:188 Resp: 242826
Ion Ratio Lower Upper
188 100
94 10.8 9.4 14.2
80 10.8 10.2 15.2

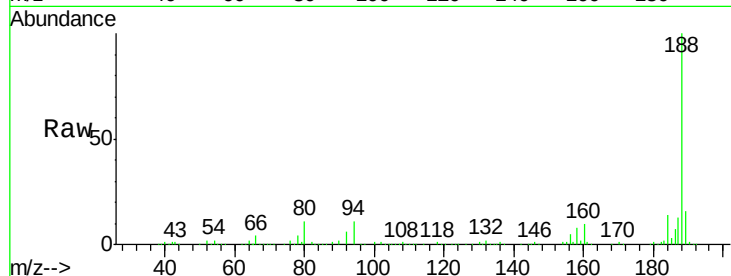


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


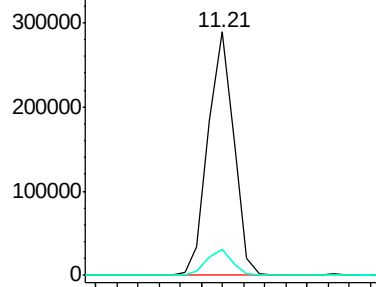



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.84 min Scan# 1998
Delta R.T. -0.01 min
Lab File: BF096583.D
Acq: 8 Jul 2017 2:28

Tgt Ion:240 Resp: 209569
Ion Ratio Lower Upper
240 100
120 15.1 5.8 8.8#
236 26.3 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




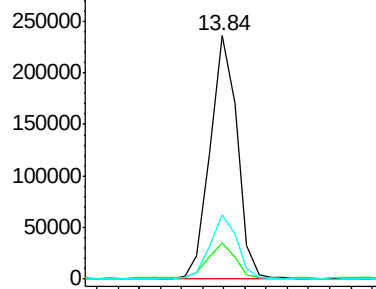


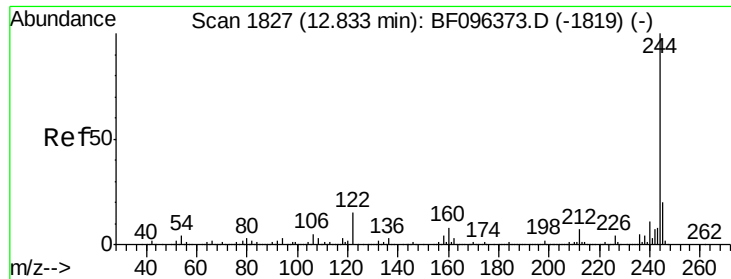

#78
 Terphenyl-d14
 Concen: 55.337 ng
 RT: 12.80 min Scan# 1821
 Delta R.T. -0.00 min
 Lab File: BF096583.D
 Acq: 8 Jul 2017 2:28

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-010

Tgt Ion:244 Resp: 542712
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 13.3 10.3 15.5

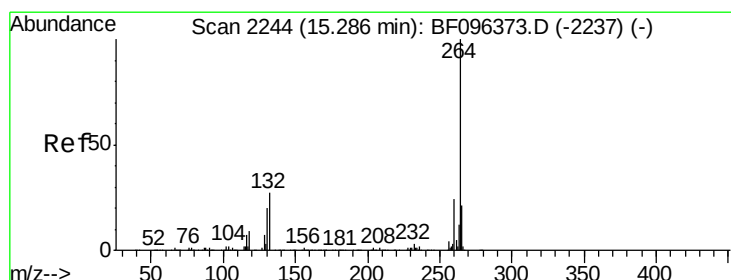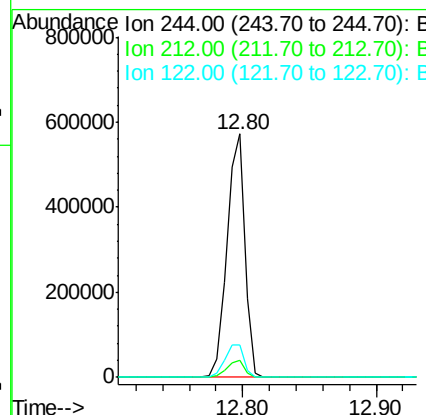

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.24 min Scan# 2237
 Delta R.T. -0.00 min
 Lab File: BF096583.D
 Acq: 8 Jul 2017 2:28

Tgt Ion:264 Resp: 155820
 Ion Ratio Lower Upper
 264 100
 260 25.2 19.5 29.3
 265 20.2 17.2 25.8

